

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030955.D
 Acq On : 09 Apr 2019 14:07
 Operator : JC/SP
 Sample : K2286-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZF3

Quant Time: Apr 10 03:11:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 01:53:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	223968	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	221123	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	87870	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	85624	5.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.00%
7) Chloroethane-d5	1.68	69	76204	5.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.40%
11) 1,1-Dichloroethene-d2	2.27	63	132514	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	4.19	46	262566	59.54	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.08%
24) Chloroform-d	4.64	84	141141	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	5.31	65	89013	5.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	115.60%
32) Benzene-d6	5.33	84	287642	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.33	67	103553	5.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.00%
41) Toluene-d8	7.56	98	225810	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
43) trans-1,3-Dichloropropene-	7.85	79	32454	4.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.60%
46) 2-Hexanone-d5	8.31	63	162370	51.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.96%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	81463	5.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	116.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	80759	5.49	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	6018	1.765 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030955.D
Acq On : 09 Apr 2019 14:07
Operator : JC/SP
Sample : K2286-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZF3

Quant Time: Apr 10 03:11:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 01:53:07 2019
Response via : Initial Calibration

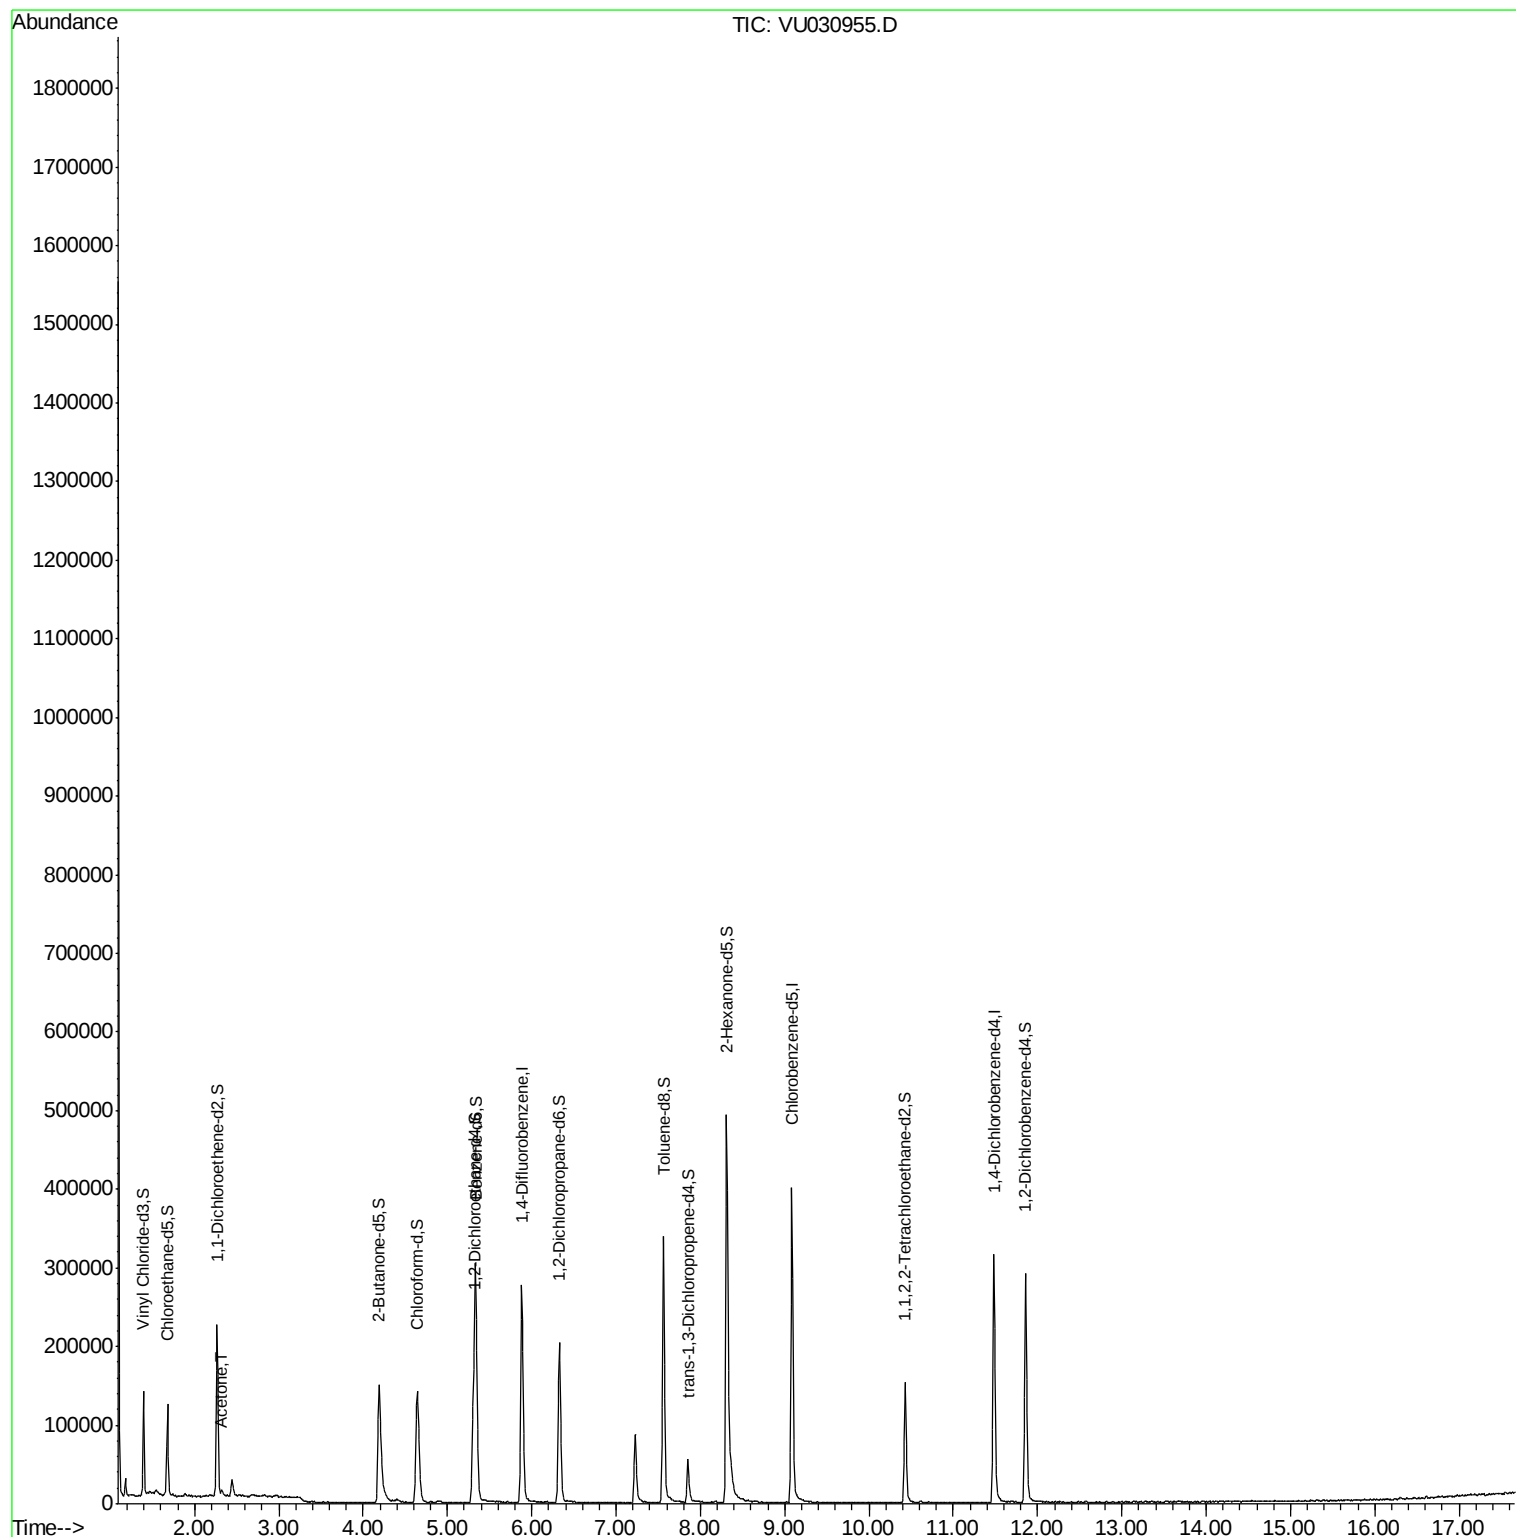

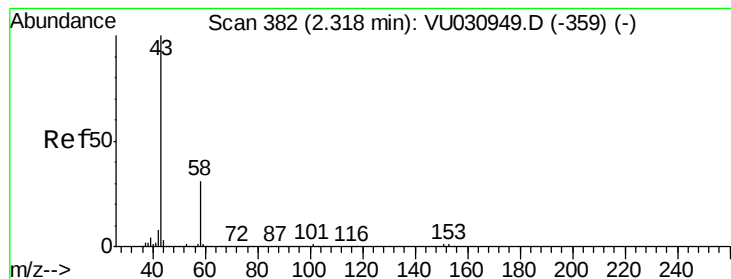

#13

Acetone

Concen: 1.765 ug/L

RT: 2.32 min Scan# 383

Delta R.T. 0.00 min

Lab File: VU030955.D

Acq: 09 Apr 2019 14:07

Instrument :
MSVOA_U
ClientSampleId :
BEZF3

Tot Ion: 43 Resp: 6018

Ion Ratio Lower Upper

43 100

58 31.1 0.0 62.8

