

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030958.D
 Acq On : 09 Apr 2019 15:19
 Operator : JC/SP
 Sample : K2286-18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZF6

Quant Time: Apr 10 03:22:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 01:53:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	220836	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	224284	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	90156	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	85297	5.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.00%
7) Chloroethane-d5	1.68	69	77148	5.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.40%
11) 1,1-Dichloroethene-d2	2.27	63	130005	3.76	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.20%
20) 2-Butanone-d5	4.19	46	270715	62.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.50%
24) Chloroform-d	4.64	84	147971	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.40%
26) 1,2-Dichloroethane-d4	5.31	65	92070	6.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.20%
32) Benzene-d6	5.33	84	292879	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.33	67	102721	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.56	98	222648	4.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.40%
43) trans-1,3-Dichloropropene-	7.85	79	34028	4.63	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.60%
46) 2-Hexanone-d5	8.31	63	168948	52.81	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.62%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	85511	6.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	120.60%#
64) 1,2-Dichlorobenzene-d4	11.86	152	82898	5.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.00%


Target Compounds				Ovalue
13) Acetone	2.32	43	11797	3.509 ug/L 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030958.D
Acq On : 09 Apr 2019 15:19
Operator : JC/SP
Sample : K2286-18
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZF6

Quant Time: Apr 10 03:22:47 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 01:53:07 2019
Response via : Initial Calibration

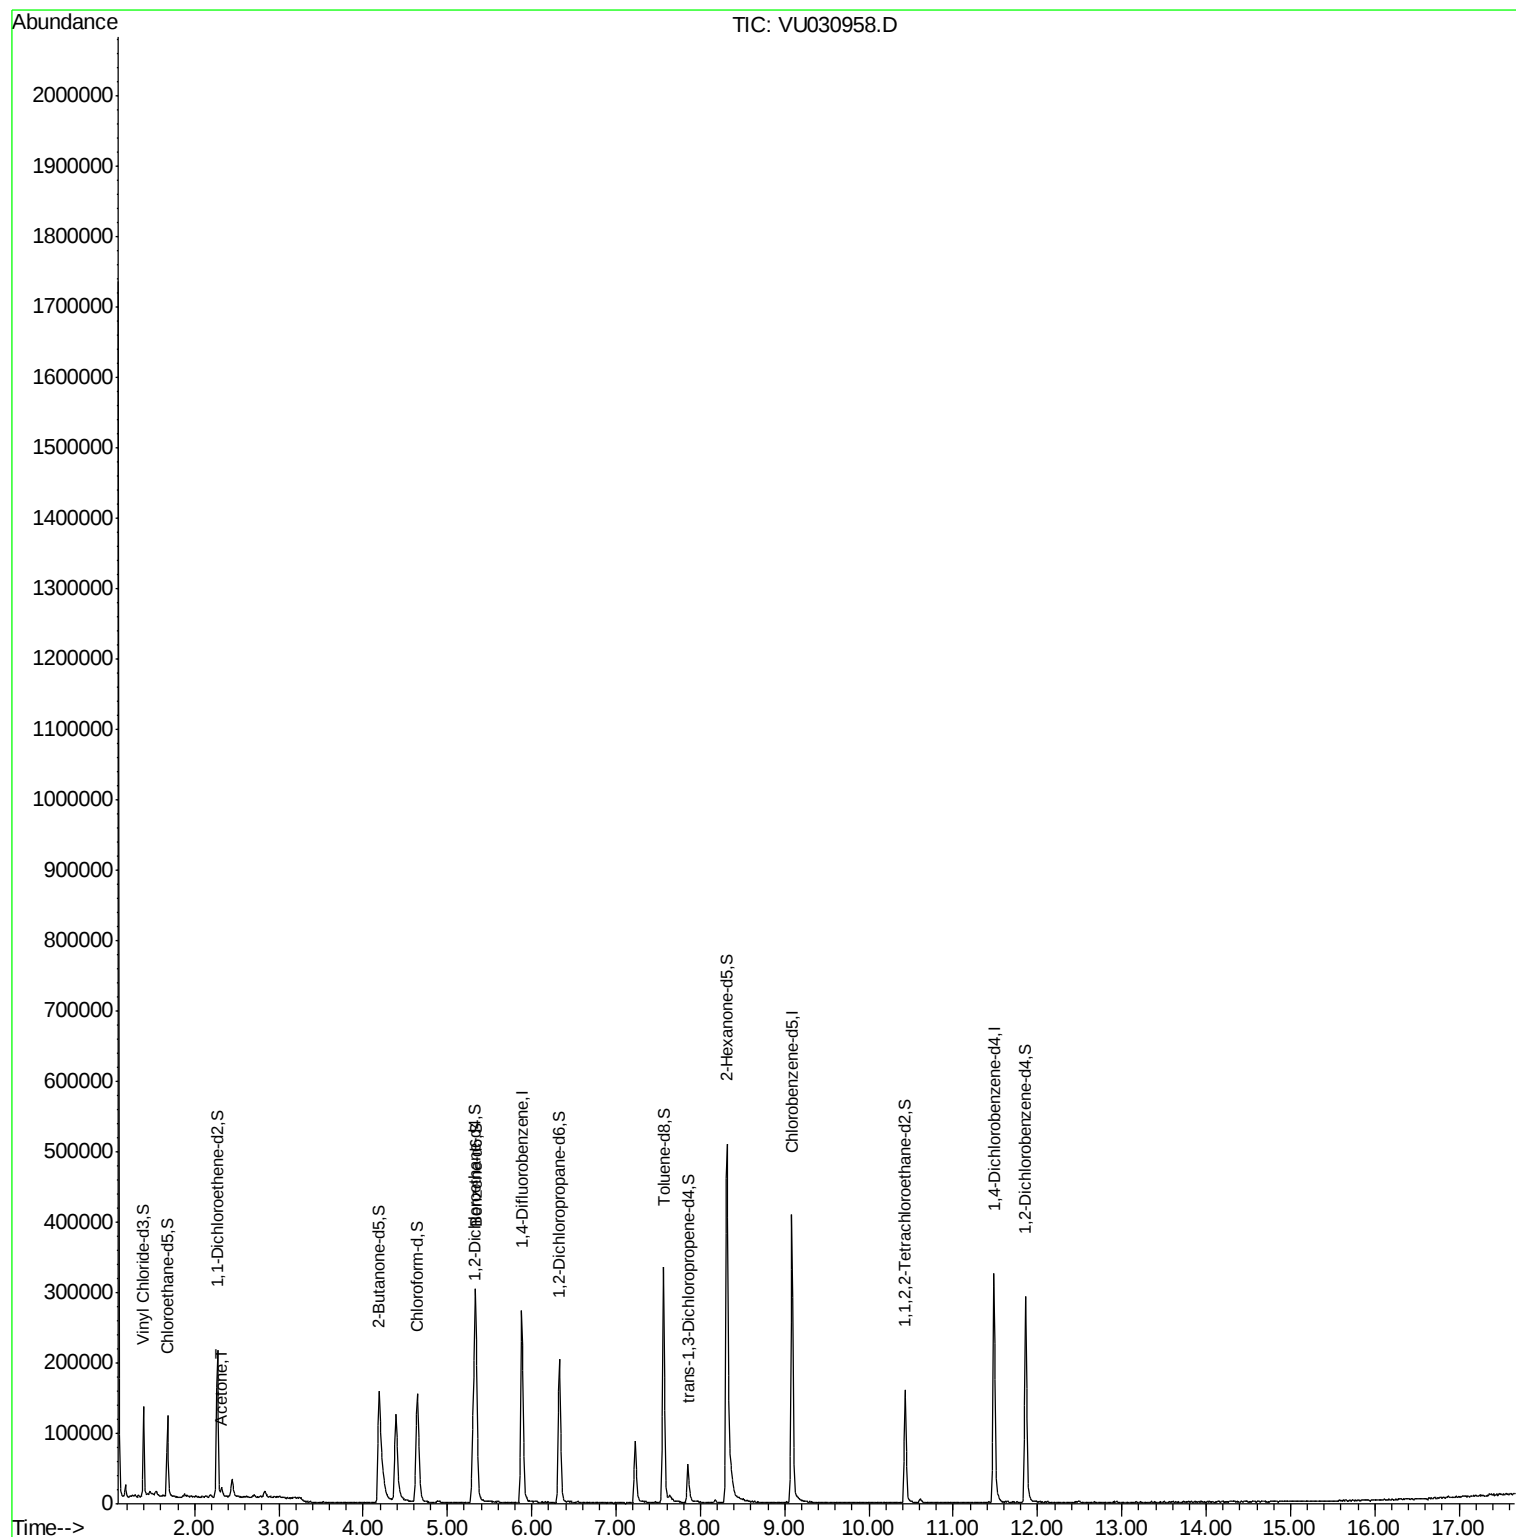

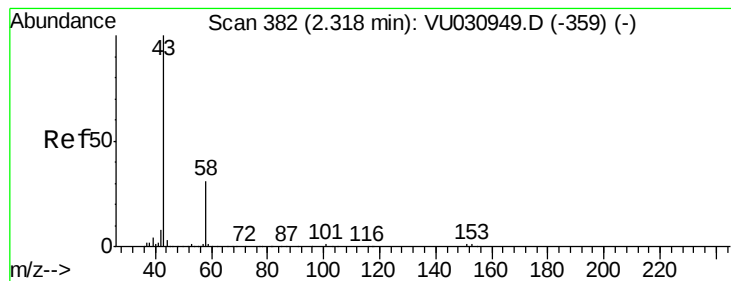

#13
 Acetone
 Concen: 3.509 ug/L
 RT: 2.32 min Scan# 383
 Delta R.T. 0.00 min
 Lab File: VU030958.D
 Acq: 09 Apr 2019 15:19

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZF6

Tot Ion: 43 Resp: 11797
 Ion Ratio Lower Upper
 43 100
 58 28.8 0.0 62.8

