

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030970.D
 Acq On : 09 Apr 2019 20:33
 Operator : JC/SP
 Sample : K2286-05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZE3

Quant Time: Apr 10 04:12:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 01:53:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	215869	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	219001	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	86251	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	78509	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.68	69	75533	5.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.60%
11) 1,1-Dichloroethene-d2	2.27	63	120770	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.60%
20) 2-Butanone-d5	4.19	46	273419	64.32	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.64%
24) Chloroform-d	4.64	84	134505	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
26) 1,2-Dichloroethane-d4	5.31	65	89137	6.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.00%
32) Benzene-d6	5.33	84	286691	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	6.33	67	99318	5.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.60%
41) Toluene-d8	7.56	98	218080	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	7.85	79	32983	4.59	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.80%
46) 2-Hexanone-d5	8.31	63	162757	52.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.20%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	86232	6.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	124.40%#
64) 1,2-Dichlorobenzene-d4	11.86	152	82246	5.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	4757	1.448 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030970.D
Acq On : 09 Apr 2019 20:33
Operator : JC/SP
Sample : K2286-05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZE3

Quant Time: Apr 10 04:12:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 01:53:07 2019
Response via : Initial Calibration

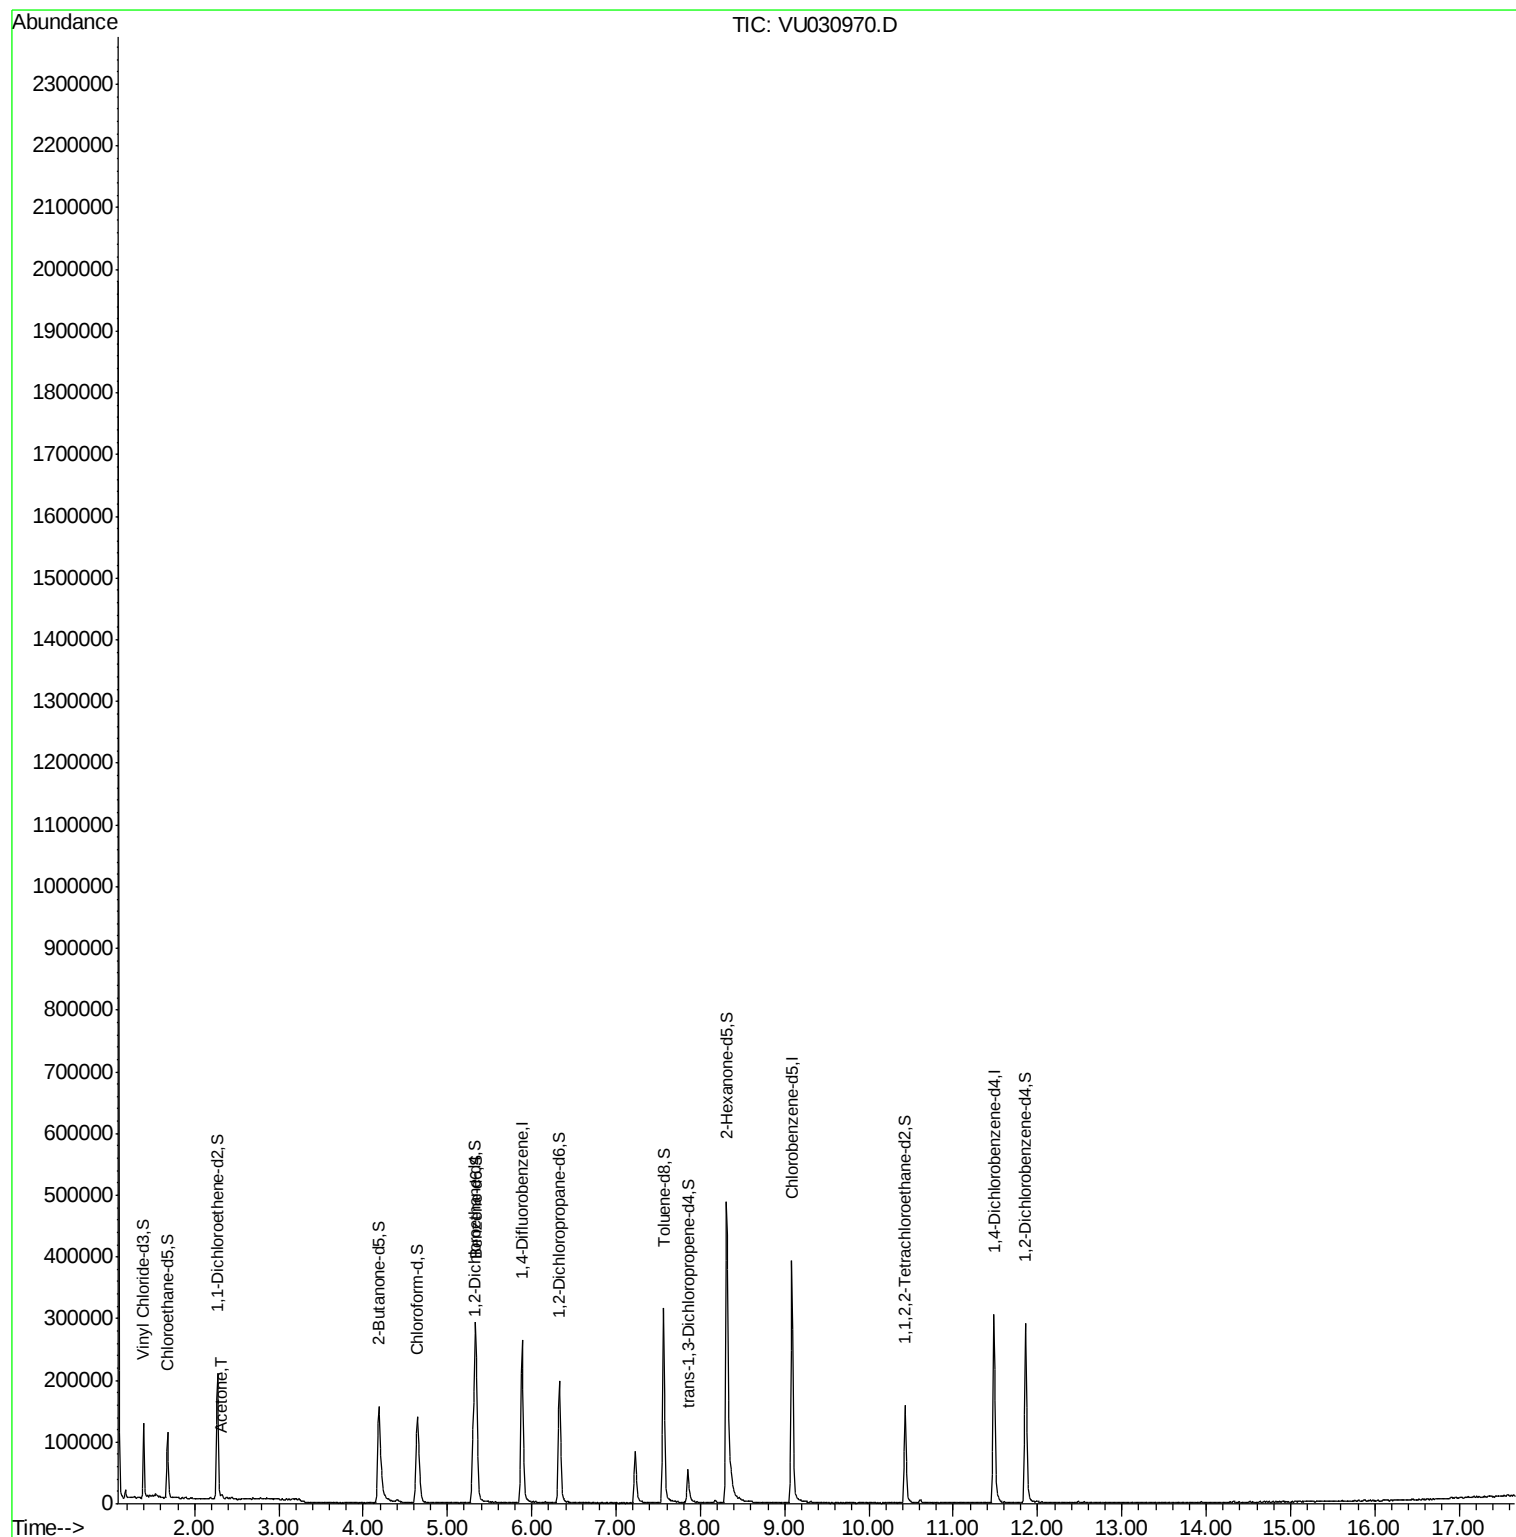

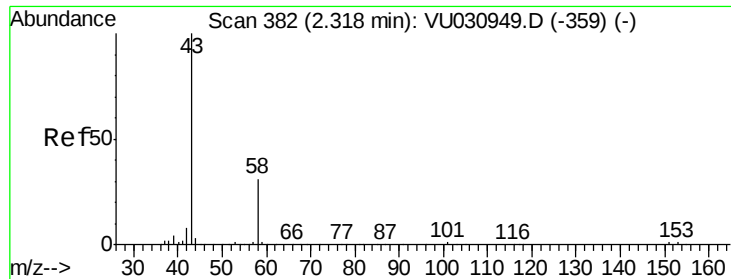

#13

Acetone

Concen: 1.448 ug/L

RT: 2.32 min Scan# 381

Delta R.T. -0.00 min

Lab File: VU030970.D

Acq: 09 Apr 2019 20:33

Instrument :
MSVOA_U
ClientSampleId :
BEZE3

Tot Ion: 43 Resp: 4757

Ion Ratio Lower Upper

43 100

58 27.6 0.0 62.8

