

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030989.D
 Acq On : 10 Apr 2019 05:08
 Operator : JC/SP
 Sample : K2290-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZH2

Quant Time: Apr 10 05:47:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 05:35:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	214864	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	223591	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	87786	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	59843	3.64	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.80%
7) Chloroethane-d5	1.68	69	63722	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.20%
11) 1,1-Dichloroethene-d2	2.27	63	61863	1.84	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	36.80%#
20) 2-Butanone-d5	4.19	46	267815	63.30	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.60%
24) Chloroform-d	4.64	84	126431	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.31	65	81337	5.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.00%
32) Benzene-d6	5.33	84	247501	4.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.20%
36) 1,2-Dichloropropane-d6	6.33	67	91384	4.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.60%
41) Toluene-d8	7.56	98	178824	3.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.00%#
43) trans-1,3-Dichloropropene-	7.85	79	29388	4.01	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.20%
46) 2-Hexanone-d5	8.31	63	159038	49.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.74%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	77131	5.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	72850	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	11583	3.541 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030989.D
Acq On : 10 Apr 2019 05:08
Operator : JC/SP
Sample : K2290-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZH2

Quant Time: Apr 10 05:47:48 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 05:35:34 2019
Response via : Initial Calibration

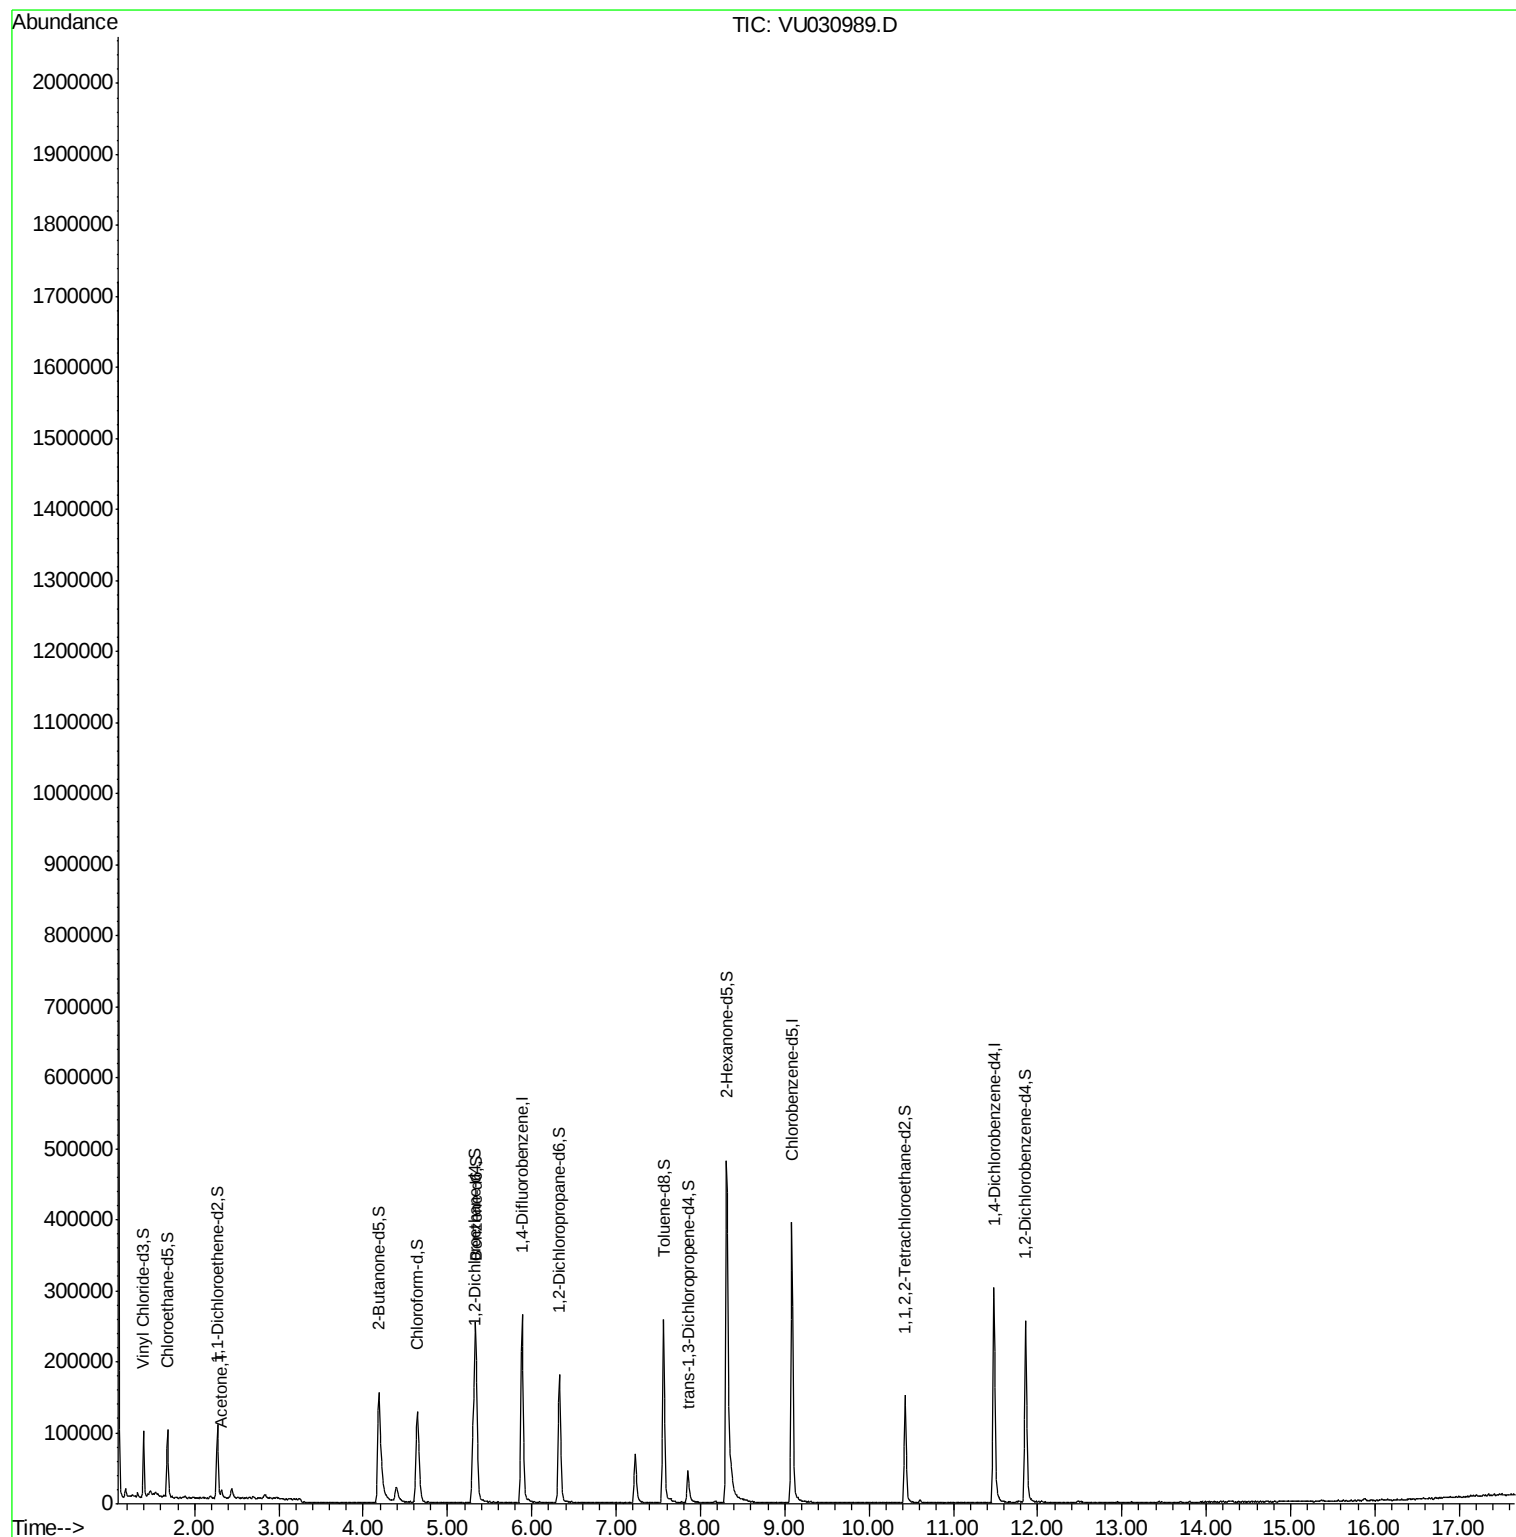

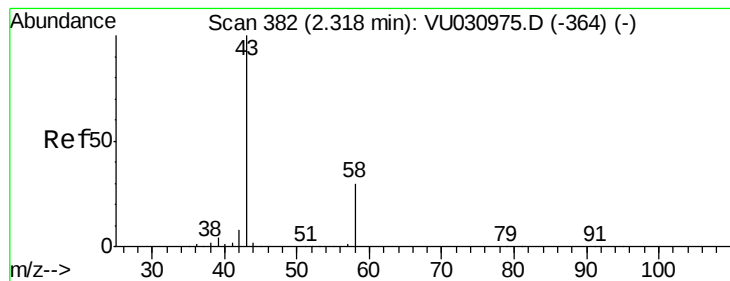

#13

Acetone

Concen: 3.541 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU030989.D

Acq: 10 Apr 2019 05:08

Instrument :
MSVOA_U
ClientSampleId :
BEZH2

Tot Ion: 43 Resp: 11583

Ion Ratio Lower Upper

43 100

58 27.8 0.0 62.8

