

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030992.D
 Acq On : 10 Apr 2019 06:21
 Operator : JC/SP
 Sample : K2290-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZH5

Quant Time: Apr 10 08:47:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Apr 10 08:26:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	187114	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	195968	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	76197	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	64520	4.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.20%
7) Chloroethane-d5	1.68	69	62451	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.40%
11) 1,1-Dichloroethene-d2	2.27	63	96495	3.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.00%
20) 2-Butanone-d5	4.19	46	261493	70.97	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	141.94%#
24) Chloroform-d	4.64	84	120221	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.31	65	80765	6.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	125.60%
32) Benzene-d6	5.33	84	238636	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
36) 1,2-Dichloropropane-d6	6.33	67	85646	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	7.56	98	182683	3.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.40%
43) trans-1,3-Dichloropropene-	7.85	79	27834	4.33	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.60%
46) 2-Hexanone-d5	8.31	63	159046	56.90	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.80%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	81243	6.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	131.00%#
64) 1,2-Dichlorobenzene-d4	11.86	152	71293	5.59	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.80%


Target Compounds					Ovalue
13) Acetone	2.32	43	5022	1.763 ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030992.D
Acq On : 10 Apr 2019 06:21
Operator : JC/SP
Sample : K2290-07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZH5

Quant Time: Apr 10 08:47:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Apr 10 08:26:32 2019
Response via : Initial Calibration

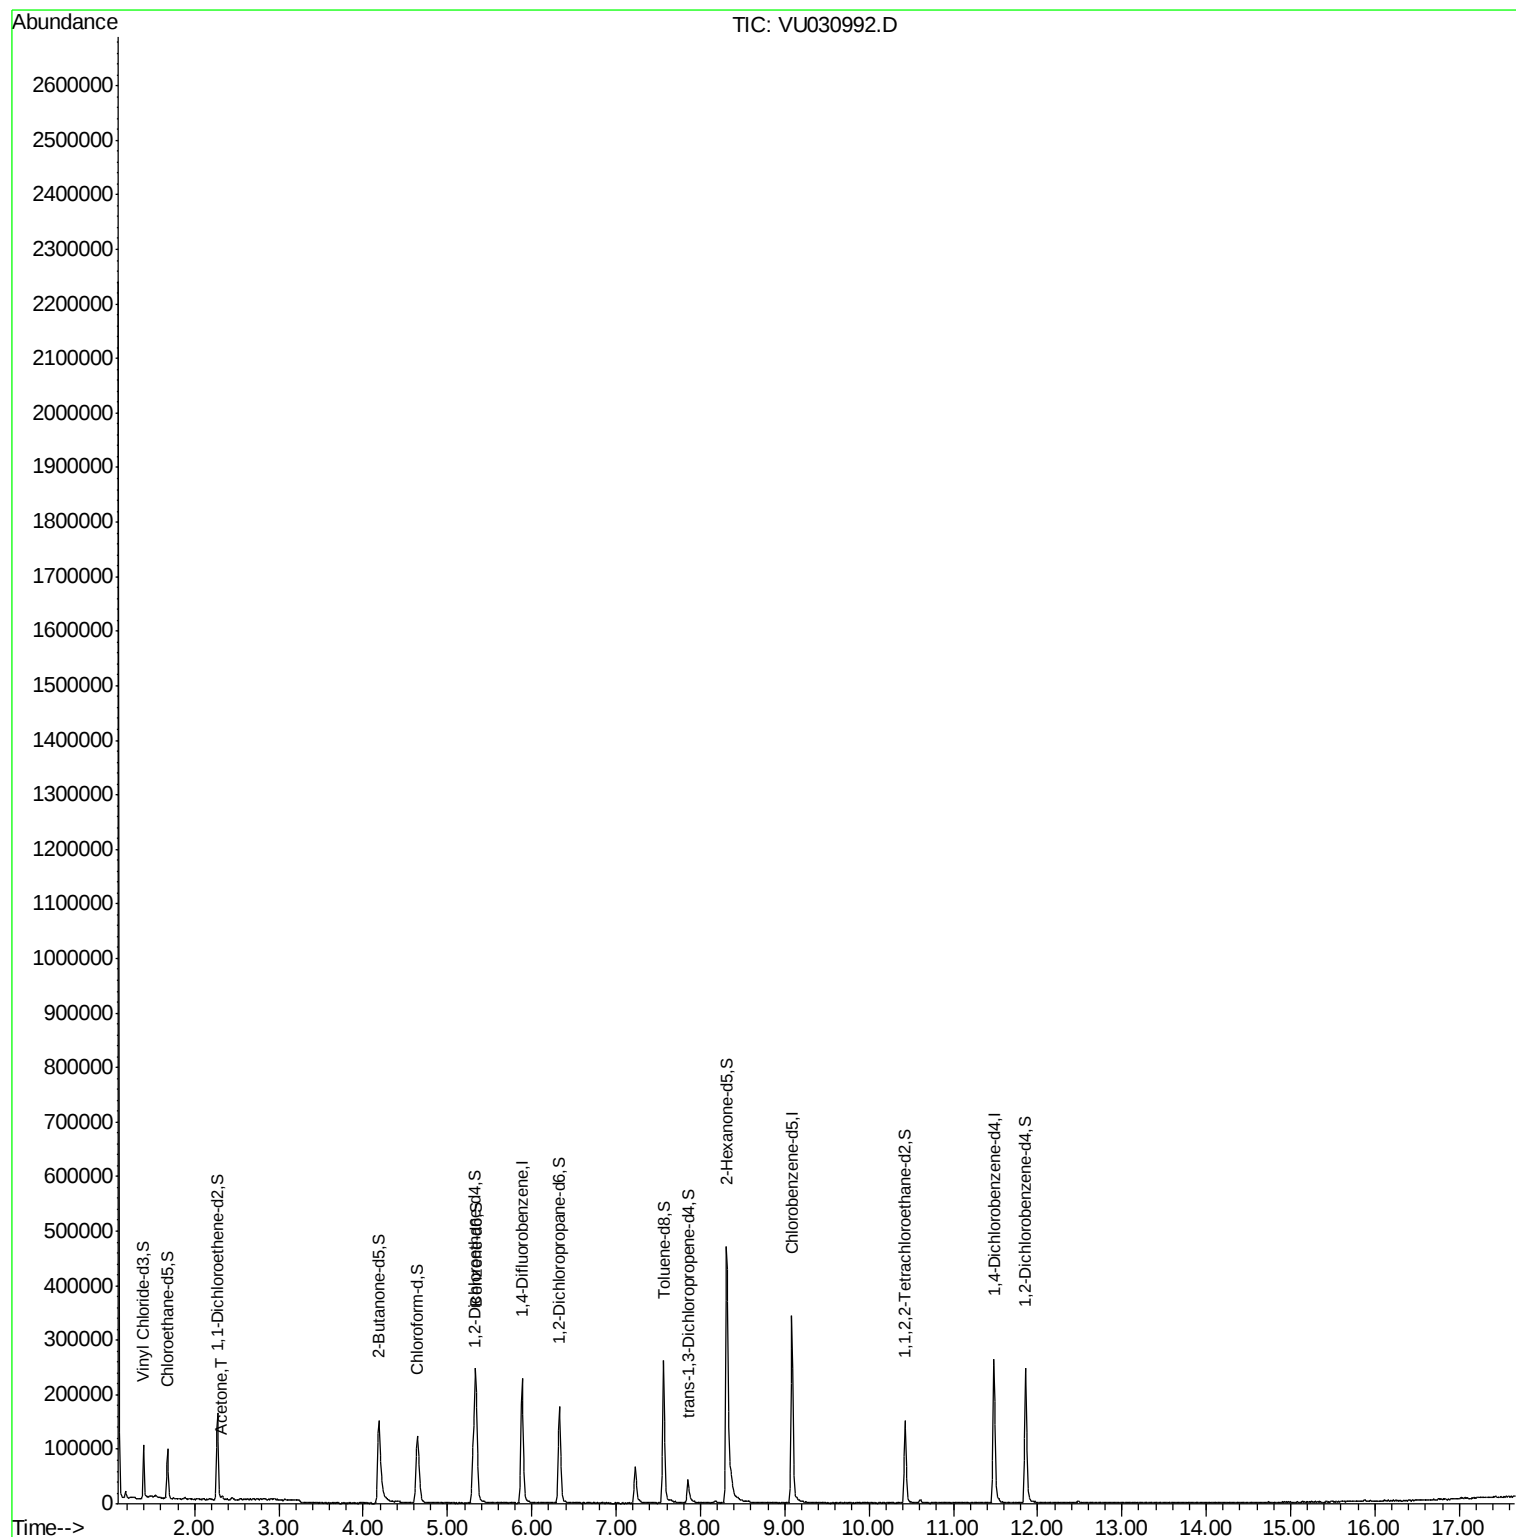

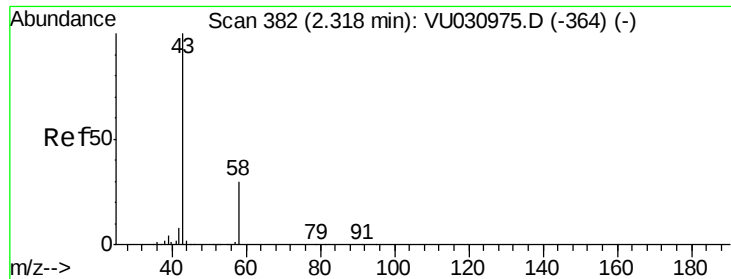

#13

Acetone

Concen: 1.763 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU030992.D

Acq: 10 Apr 2019 06:21

Instrument :
MSVOA_U
ClientSampleId :
BEZH5

Tot Ion: 43 Resp: 5022

Ion Ratio Lower Upper

43 100

58 16.2 0.0 62.8

