

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030915.D
 Acq On : 08 Apr 2019 19:19
 Operator : JC/SP
 Sample : K2284-02DL 4X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZA0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	22	28	35	rBV2	22131	21946	1.81%	0.239%
2	1.392	87	94	107	rBV	158846	170141	14.05%	1.856%
3	1.675	174	182	195	rVB	130720	161364	13.33%	1.760%
4	2.267	355	366	378	rBV	262324	397777	32.86%	4.339%
5	2.691	491	498	507	rVB2	20879	31732	2.62%	0.346%
6	4.193	953	965	1008	rBV	172230	502540	41.51%	5.481%
7	4.402	1022	1030	1040	rBV2	7502	14083	1.16%	0.154%
8	4.643	1089	1105	1131	rBV2	170375	433703	35.82%	4.730%
9	5.331	1296	1319	1346	rBV2	379561	1044039	86.24%	11.387%
10	5.881	1477	1490	1518	rBV	310602	637022	52.62%	6.948%
11	6.180	1567	1583	1604	rBV	282788	558088	46.10%	6.087%
12	6.328	1614	1629	1651	rBV2	241607	496010	40.97%	5.410%
13	7.228	1895	1909	1930	rBV	110964	209232	17.28%	2.282%
14	7.562	2000	2013	2034	rBV	422677	763312	63.05%	8.325%
15	7.852	2093	2103	2118	rBV	64986	117253	9.69%	1.279%
16	8.315	2233	2247	2281	rBV	610379	1210645	100.00%	13.204%
17	9.086	2474	2487	2513	rBV	466680	810441	66.94%	8.839%
18	10.431	2892	2905	2935	rBV3	176343	302765	25.01%	3.302%
19	11.482	3221	3232	3262	rBV	381125	657498	54.31%	7.171%
20	11.858	3332	3349	3376	rBV	361049	628946	51.95%	6.860%


Sum of corrected areas: 9168537

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030915.D
Acq On : 08 Apr 2019 19:19
Operator : JC/SP
Sample : K2284-02DL 4X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZA0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

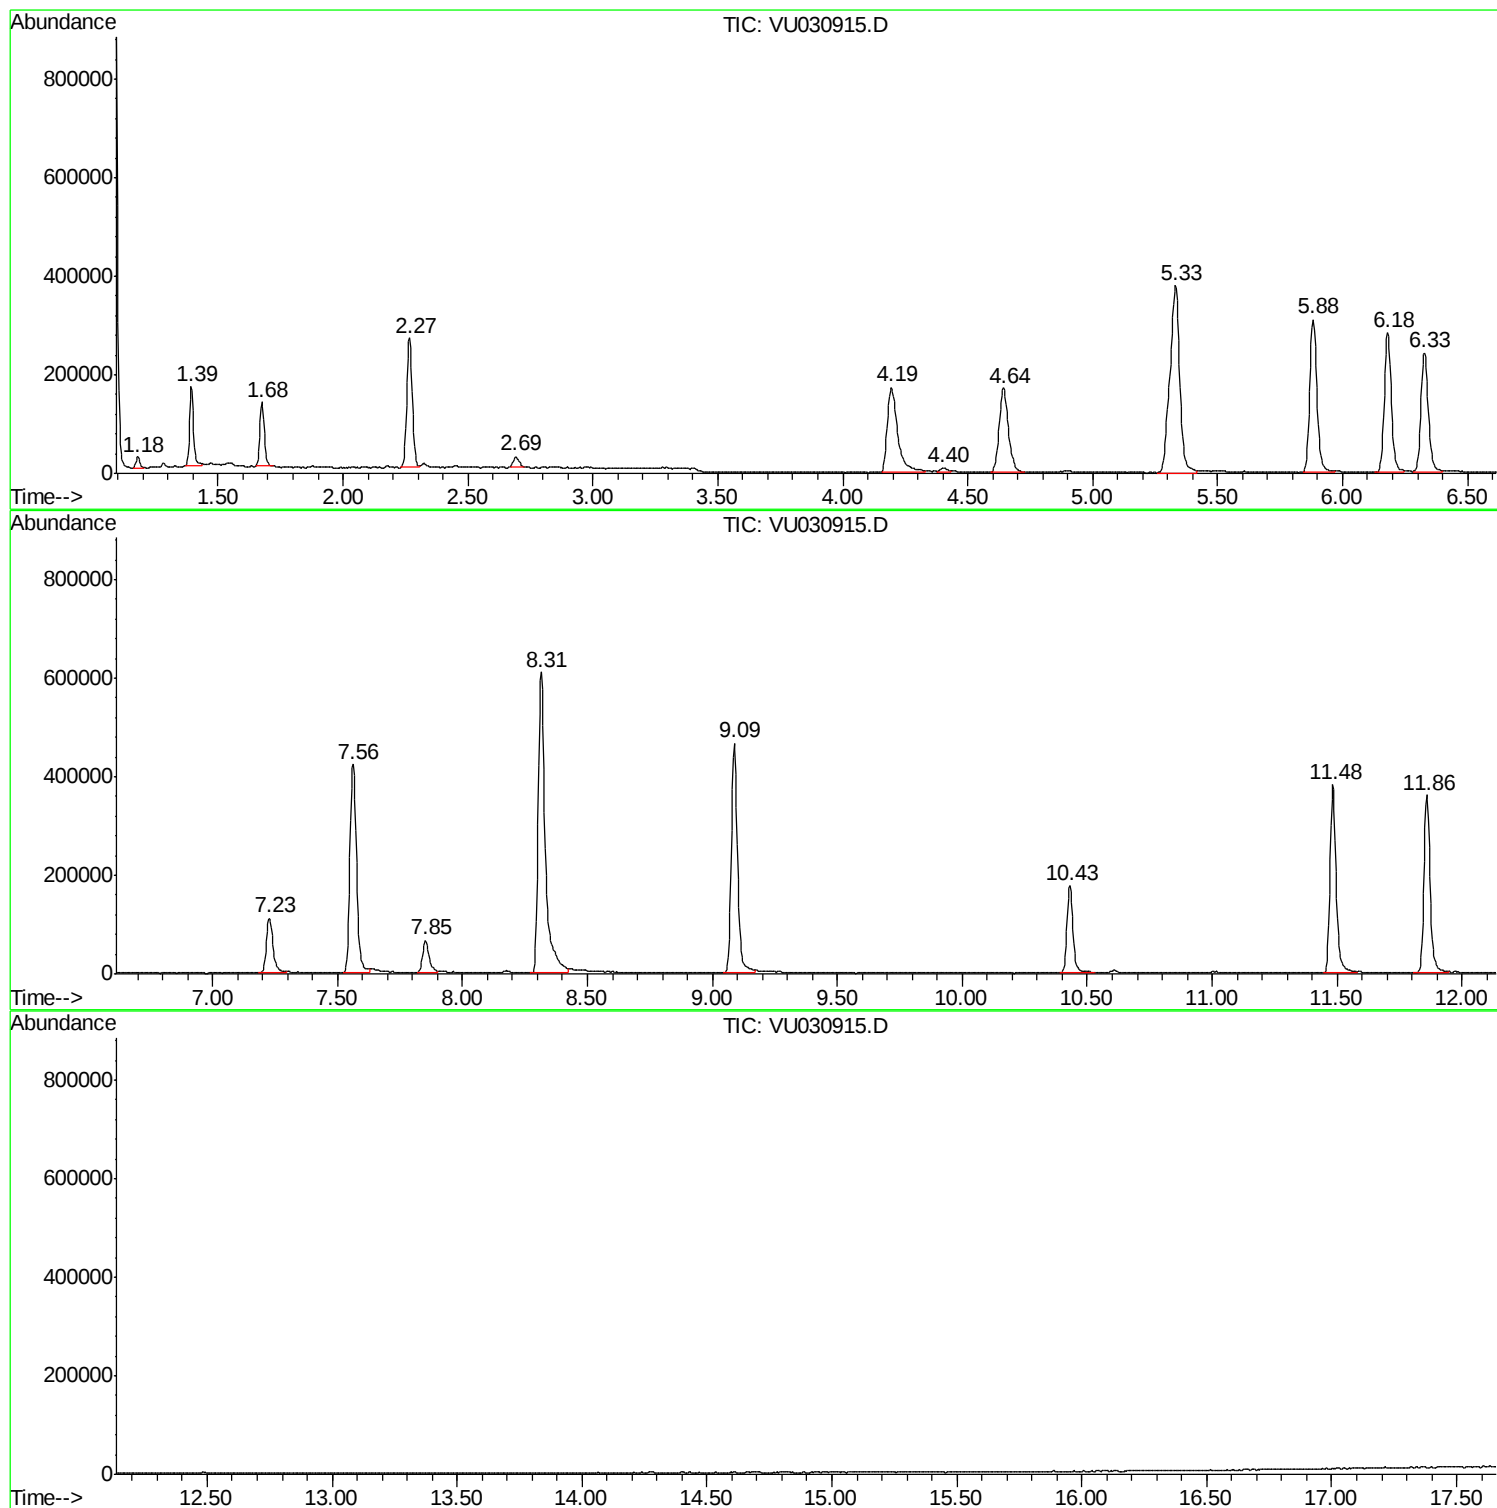

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041019\
Data File : VU030915.D
Acq On : 08 Apr 2019 19:19
Operator : JC/SP
Sample : K2284-02DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZA0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041019\
Data File : VU030915.D
Acq On : 08 Apr 2019 19:19
Operator : JC/SP
Sample : K2284-02DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZA0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc