

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU030946.D
 Acq On : 09 Apr 2019 10:05
 Operator : JC/SP
 Sample : K2286-10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BEZE8

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	88	95	105	rBV	129556	135450	12.88%	1.570%
2	1.678	175	183	197	rBV	116387	145555	13.84%	1.687%
3	2.270	357	367	377	rBV	230749	348568	33.14%	4.040%
4	2.444	411	421	437	rBV	112282	206444	19.63%	2.393%
5	4.190	948	964	996	rBV2	153786	499160	47.46%	5.785%
6	4.392	1017	1027	1047	rVB2	34185	80346	7.64%	0.931%
7	4.643	1088	1105	1126	rBV2	156224	383425	36.46%	4.444%
8	4.907	1172	1187	1201	rVB4	15562	37638	3.58%	0.436%
9	5.334	1295	1320	1337	rBV3	308637	876671	83.35%	10.160%
10	5.881	1478	1490	1512	rBV2	279090	570641	54.26%	6.613%
11	6.180	1569	1583	1607	rBV	449100	888262	84.45%	10.294%
12	6.328	1615	1629	1650	rVB	209552	420809	40.01%	4.877%
13	7.228	1895	1909	1924	rBV2	89443	168225	15.99%	1.950%
14	7.562	1998	2013	2029	rBV	354314	625508	59.47%	7.249%
15	7.852	2092	2103	2124	rBV	52534	101934	9.69%	1.181%
16	8.315	2235	2247	2280	rBV2	464491	1051760	100.00%	12.189%
17	9.086	2471	2487	2516	rBV	422760	735863	69.96%	8.528%
18	10.430	2892	2905	2924	rBV	154967	262873	24.99%	3.046%
19	11.482	3219	3232	3255	rBV	330292	570943	54.28%	6.617%
20	11.858	3335	3349	3375	rBV	293258	518650	49.31%	6.011%


Sum of corrected areas: 8628725

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030946.D
Acq On : 09 Apr 2019 10:05
Operator : JC/SP
Sample : K2286-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZE8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

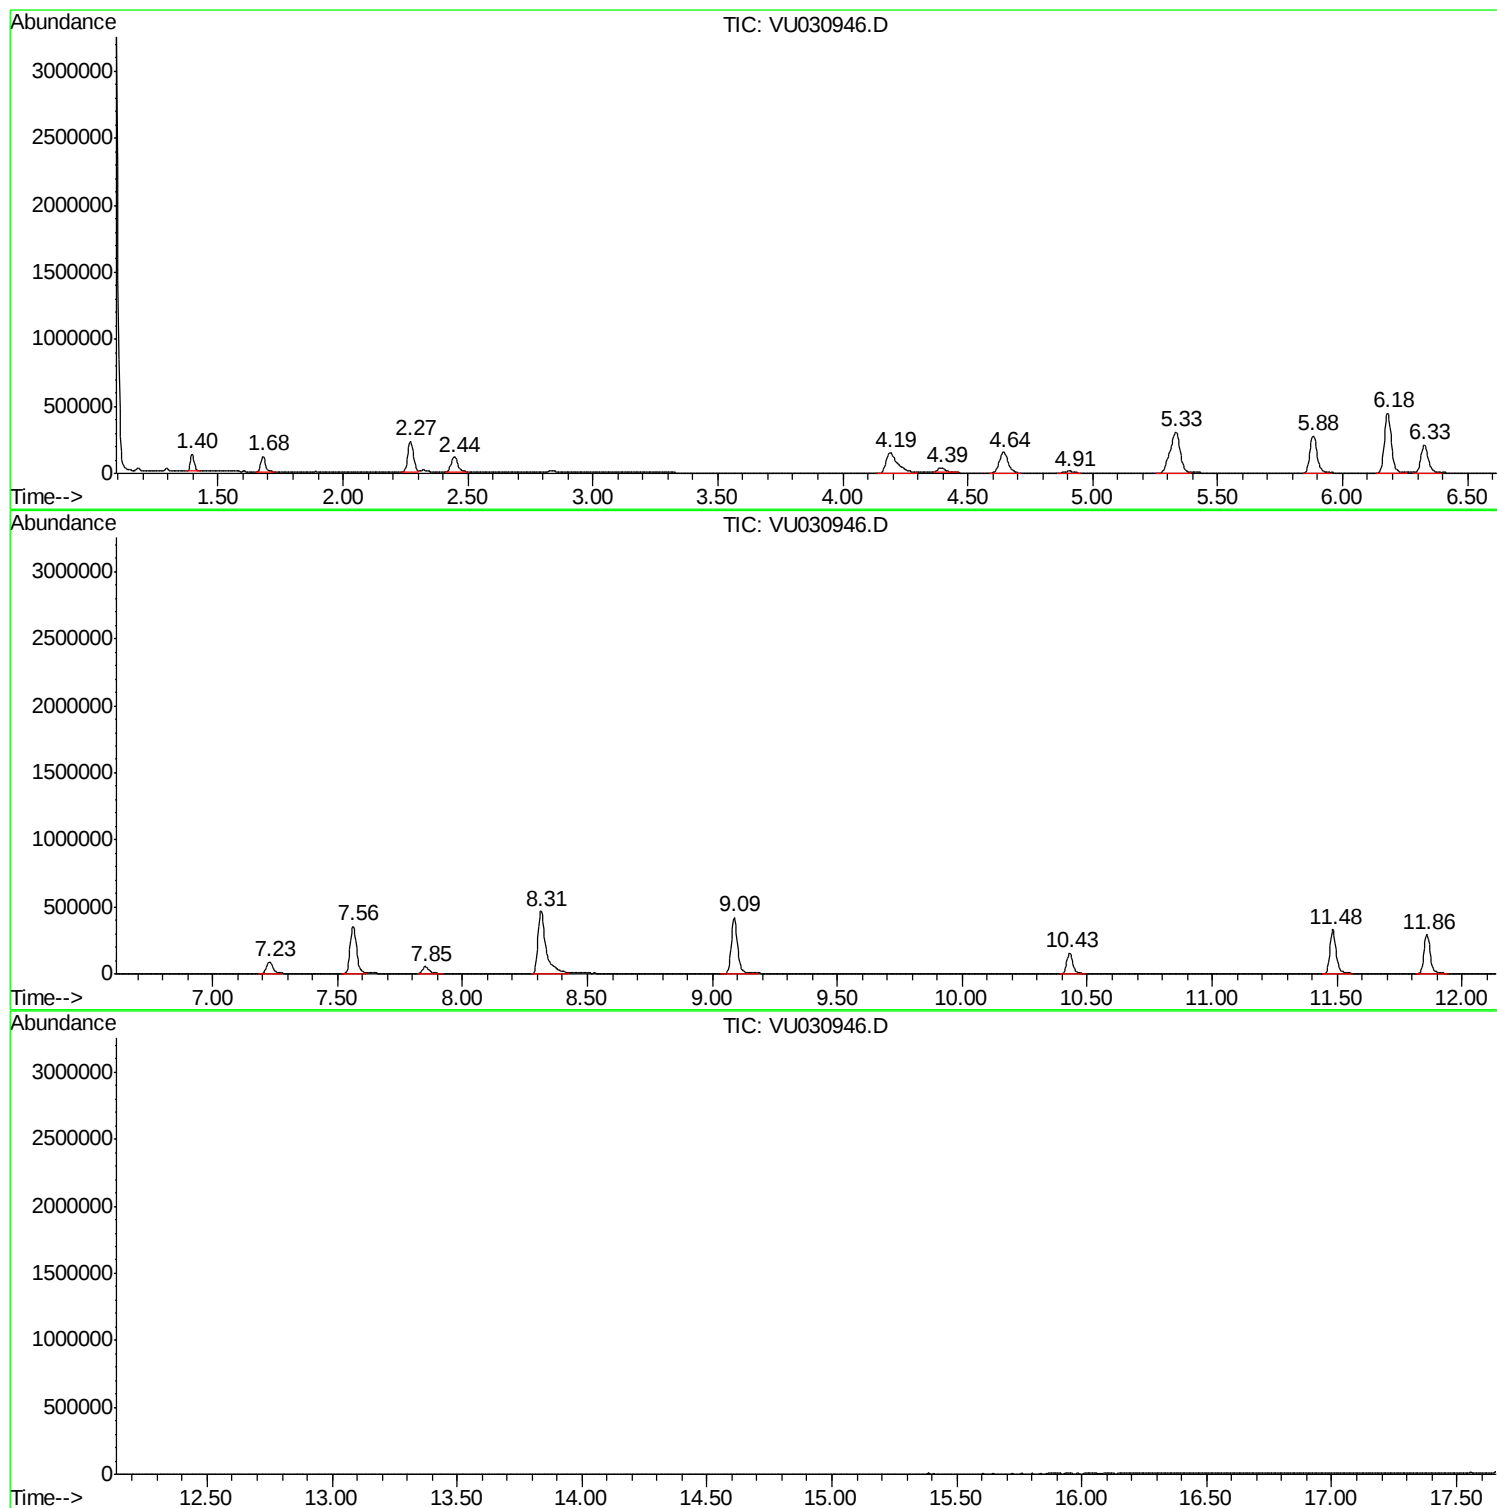

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030946.D
Acq On : 09 Apr 2019 10:05
Operator : JC/SP
Sample : K2286-10
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZE8










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.44	1.81 ug/L	206444	1,4-Difluorobenzene	5.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	90
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	83
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	78
4		Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

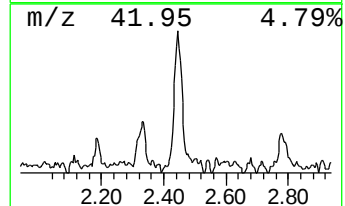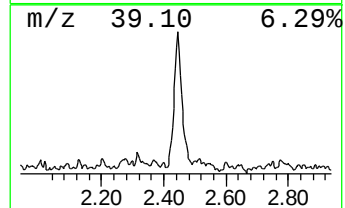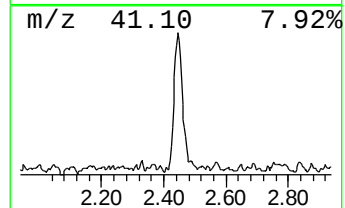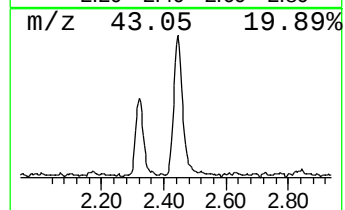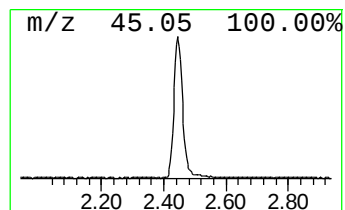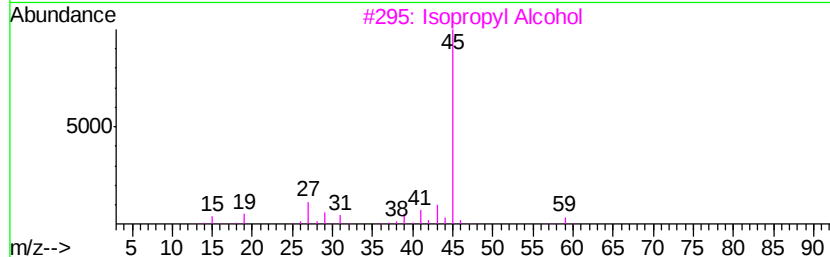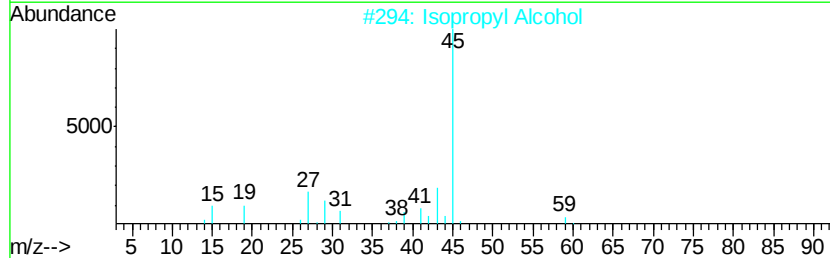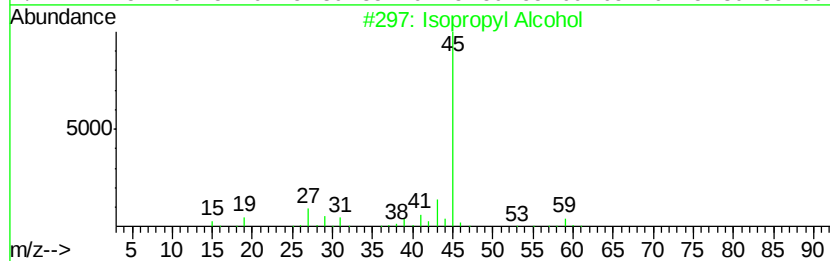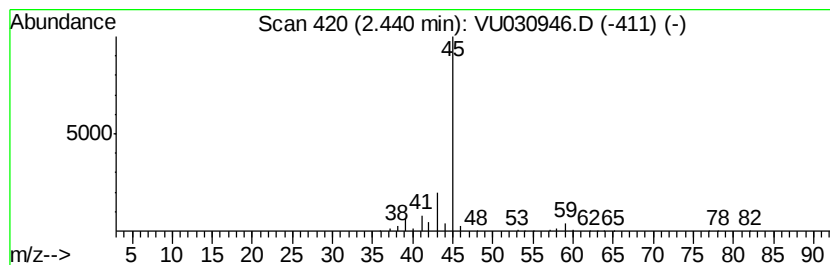

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041019\
Data File : VU030946.D
Acq On : 09 Apr 2019 10:05
Operator : JC/SP
Sample : K2286-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BEZE8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.44	1.8	ug/L	206444	1	5.88	570641	5.0