


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041019\
 Data File : VU030910.D
 Acq On : 08 Apr 2019 17:07
 Operator : JC/SP
 Sample : BFB03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 11 02:07:02 2019

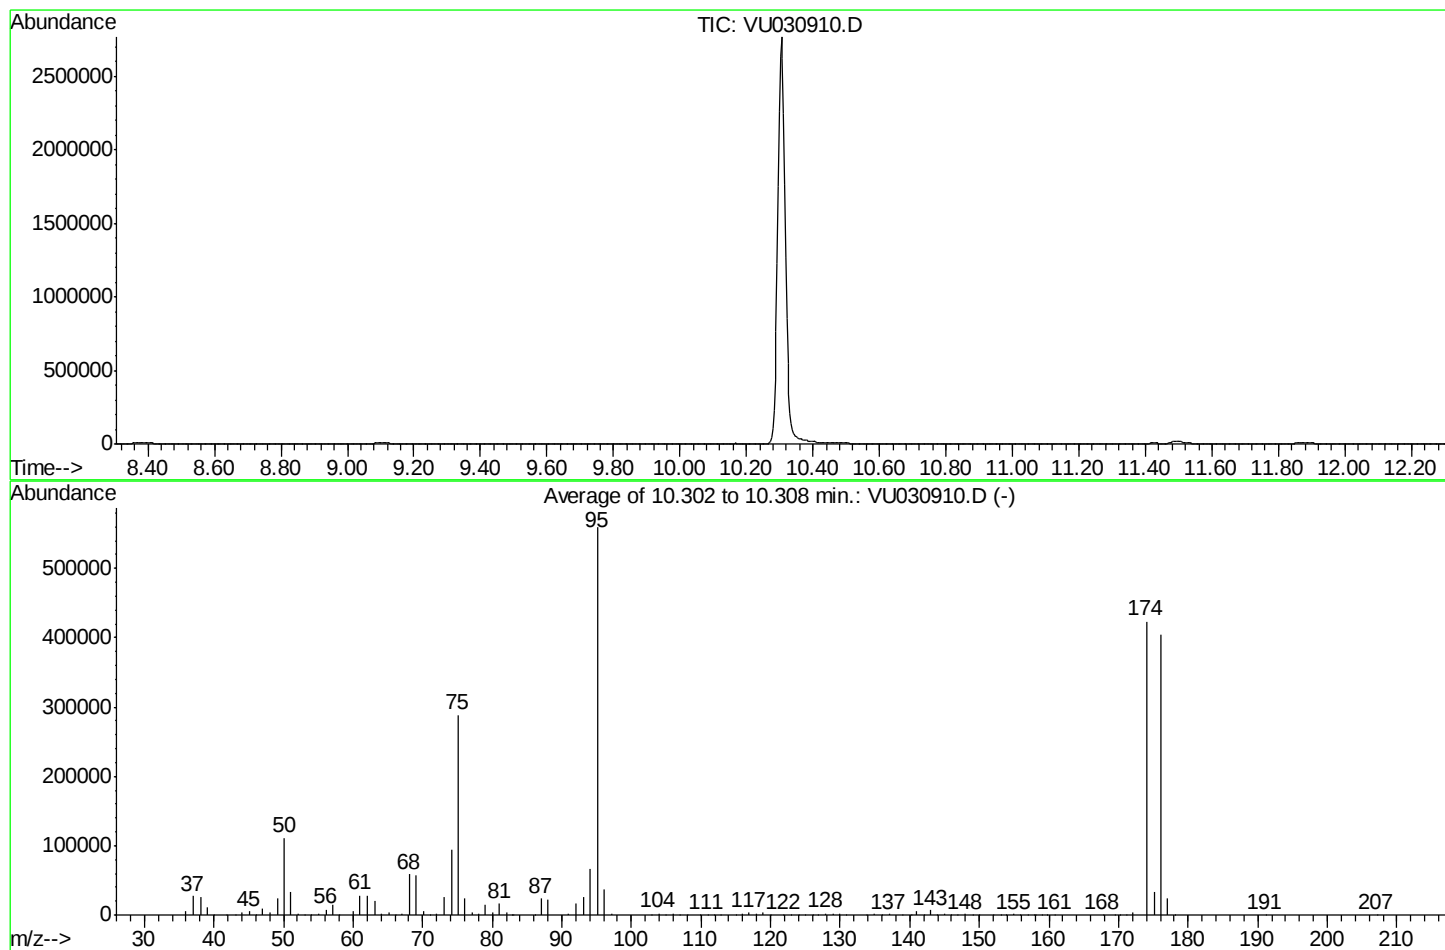

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	111672	PASS
75	95	30	80	51.6	288661	PASS
95	95	100	100	100.0	559338	PASS
96	95	5	9	6.7	37469	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.7	423466	PASS
175	174	5	9	7.7	32504	PASS
176	174	95	101	95.4	403904	PASS
177	176	5	9	6.1	24736	PASS

Scan 2850 (10.254 min): VU030910.D
BFB03

m/z	Abundance
39.80	466.0
44.00	1381.0
77.10	108.0
207.10	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	4833.0
37.00	25352.0
38.00	24608.0
39.10	9866.0
40.00	767.0
41.90	104.0
43.10	206.0
44.10	4283.0
45.10	4810.0
46.00	595.0
47.00	8588.0
48.00	3477.0
49.10	22384.0
50.10	107200.0
51.10	33432.0
52.10	1859.0
53.00	382.0
55.10	1315.0
56.10	8282.0
57.10	13990.0
58.00	598.0
60.00	5362.0
61.00	26768.0
62.10	25592.0
63.10	20240.0
64.00	2289.0
65.10	2929.0
66.00	387.0
66.90	1196.0
68.10	56952.0
69.10	55440.0
70.10	4402.0
71.10	260.0
72.10	2655.0
73.10	24232.0
74.10	90568.0
75.10	280448.0
76.10	22880.0
77.10	3516.0
78.10	2506.0
79.00	15382.0
80.00	4084.0
81.00	15331.0
82.00	3201.0
83.10	235.0
87.00	23592.0
88.00	21688.0
91.00	2062.0
92.10	15023.0
93.10	24664.0
94.10	64304.0
95.10	549696.0
96.10	34768.0
97.20	1073.0
102.90	195.0
103.90	2618.0
104.90	880.0
106.00	2267.0
106.90	733.0
108.10	101.0
109.90	402.0
110.90	353.0
111.90	292.0
112.90	425.0
115.00	665.0
116.00	1771.0
116.90	3550.0
118.00	1774.0
119.00	2552.0
120.00	259.0
122.90	118.0
123.90	458.0
124.90	179.0
126.00	301.0
126.90	252.0
127.90	1989.0
129.00	903.0
130.00	1708.0
130.80	687.0
133.90	112.0
134.90	987.0
135.80	176.0
137.00	1170.0
139.00	246.0
140.20	408.0
141.00	5243.0
142.00	917.0
143.00	6740.0
143.90	394.0
145.00	1479.0
146.00	960.0
146.90	279.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

147.90	1124.0
149.10	260.0
150.00	674.0
151.90	240.0
153.10	611.0
153.80	300.0
155.00	1481.0
155.80	242.0
157.00	599.0
158.10	149.0
159.00	803.0
160.90	531.0
167.70	140.0
169.40	113.0
170.20	187.0
171.10	785.0
172.10	4457.0
174.00	419072.0
175.10	32544.0
176.00	405888.0
177.00	24104.0
178.10	465.0
207.10	348.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	4906.0
37.00	27632.0
38.10	25336.0
39.10	10804.0
40.10	785.0
43.20	203.0
44.10	4190.0
45.10	5291.0
46.10	771.0
47.00	8709.0
48.00	3697.0
49.10	23664.0
50.10	112048.0
51.10	33392.0
52.10	1818.0
53.10	612.0
53.90	148.0
55.00	1531.0
56.10	8018.0
57.10	15427.0
58.00	567.0
60.00	5291.0
61.00	27984.0
62.10	27904.0
63.10	20320.0
64.00	2977.0
65.10	3664.0
66.00	470.0
67.00	1259.0
68.10	58984.0
69.10	56456.0
70.00	5079.0
70.90	330.0
72.00	2765.0
73.10	25696.0
74.10	93384.0
75.10	286720.0
76.10	25920.0
77.00	3328.0
78.10	2116.0
78.90	15472.0
80.00	4484.0
81.00	16125.0
82.00	3457.0
82.90	341.0
86.10	875.0
87.00	22168.0
88.00	21992.0
91.00	2072.0
92.10	16123.0
93.10	24480.0
94.10	66728.0
95.10	550272.0
96.10	38720.0
97.10	1047.0
102.90	183.0
103.90	2442.0
104.90	773.0
105.90	2293.0
107.00	701.0
110.00	308.0
110.90	475.0
111.80	284.0
112.80	374.0
115.10	535.0
116.00	1692.0
116.90	3560.0
118.00	2158.0
119.00	3234.0
121.90	144.0
124.00	368.0
124.90	247.0
126.00	255.0
126.90	282.0
128.00	1765.0
129.00	1088.0
129.90	1734.0
130.90	675.0
133.80	124.0
134.90	1077.0
136.00	205.0
137.00	964.0
138.90	203.0
140.10	377.0
141.00	5967.0
142.00	888.0
143.00	6957.0
143.80	327.0
145.00	1663.0
145.90	811.0
146.90	291.0
148.00	1037.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

149.10	244.0
150.00	508.0
152.00	281.0
153.00	561.0
154.00	453.0
155.00	1026.0
155.80	257.0
156.90	713.0
157.90	158.0
159.00	614.0
159.70	112.0
160.90	641.0
170.30	181.0
171.00	728.0
172.10	4585.0
174.00	411968.0
175.10	31504.0
176.00	388736.0
177.00	24840.0
178.10	589.0
207.10	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	5061.0
37.00	27784.0
38.00	26312.0
39.10	10969.0
40.10	740.0
43.20	212.0
44.10	4531.0
45.10	5426.0
46.00	720.0
47.00	9336.0
48.00	3690.0
49.10	24232.0
50.10	115768.0
51.10	35072.0
52.10	2066.0
53.00	483.0
53.90	135.0
55.00	1548.0
56.10	8799.0
57.10	15455.0
58.00	617.0
60.00	5687.0
61.00	28896.0
62.10	27800.0
63.10	21256.0
64.00	2719.0
65.10	3404.0
66.00	442.0
66.90	1280.0
68.10	61136.0
69.10	58664.0
70.10	5198.0
71.00	323.0
72.00	2850.0
73.10	26376.0
74.10	96456.0
75.10	298816.0
76.10	25760.0
77.10	3570.0
78.10	2426.0
79.00	16194.0
80.00	4345.0
81.00	16488.0
82.00	3457.0
82.90	243.0
87.00	24112.0
88.00	22648.0
91.00	2218.0
92.10	16552.0
93.10	26264.0
94.10	69320.0
95.10	578048.0
96.10	38920.0
97.10	1122.0
102.90	192.0
103.90	2731.0
104.90	910.0
106.00	2483.0
106.90	748.0
109.90	401.0
110.90	438.0
111.80	309.0
112.90	382.0
115.00	639.0
116.00	1852.0
116.90	3756.0
118.00	2027.0
118.90	3066.0
120.00	174.0
121.90	121.0
122.90	120.0
124.00	459.0
124.90	252.0
126.00	318.0
126.80	274.0
128.00	1883.0
129.00	1054.0
130.00	1736.0
130.90	764.0
133.80	105.0
134.90	1191.0
135.90	185.0
137.00	1171.0
139.00	183.0
140.20	397.0
141.00	5946.0
142.00	1050.0
143.00	7417.0
143.80	381.0
145.00	1652.0
145.90	877.0
146.90	280.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

147.90	1088.0
149.10	243.0
150.00	669.0
152.00	277.0
153.10	676.0
153.90	391.0
155.00	1287.0
155.80	253.0
156.90	708.0
157.90	123.0
159.00	769.0
159.70	108.0
160.90	617.0
167.80	125.0
169.40	130.0
171.00	847.0
172.10	4791.0
174.00	439360.0
175.10	33464.0
176.00	417088.0
177.00	25264.0
178.20	522.0
191.10	100.0
207.10	310.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03