


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
Data File : VU030948.D
Acq On : 09 Apr 2019 11:05
Operator : JC/SP
Sample : BFB04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Apr 11 02:07:02 2019

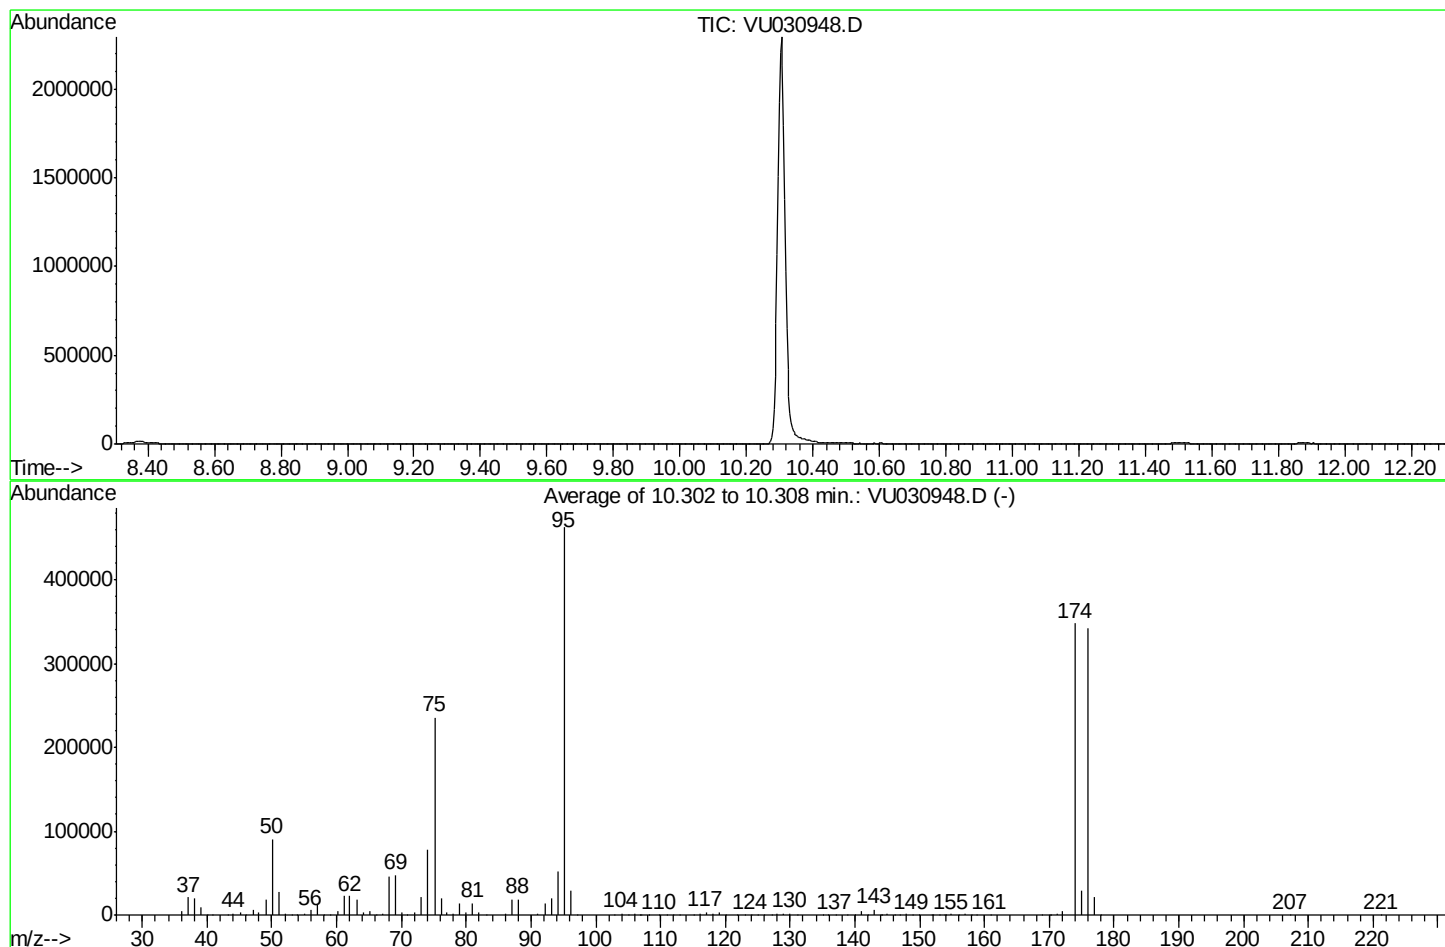

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	90226	PASS
75	95	30	80	50.9	235498	PASS
95	95	100	100	100.0	462613	PASS
96	95	5	9	6.4	29384	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.2	347840	PASS
175	174	5	9	8.2	28624	PASS
176	174	95	101	98.3	341930	PASS
177	176	5	9	6.4	21770	PASS

m/z	Abundance
36.00	4221.0
37.10	21408.0
38.10	19912.0
39.10	9091.0
40.00	939.0
40.80	186.0
43.10	216.0
44.00	3047.0
45.10	3417.0
46.00	711.0
47.10	6697.0
47.90	2789.0
49.10	19584.0
50.10	93664.0
51.10	28696.0
52.00	1012.0
53.00	381.0
54.00	210.0
55.10	1081.0
56.00	6101.0
57.10	12727.0
58.00	387.0
60.10	4398.0
61.10	23664.0
62.10	23712.0
63.10	19184.0
64.10	2978.0
65.10	4366.0
66.10	273.0
67.00	1499.0
68.10	48368.0
69.10	49736.0
70.10	3734.0
70.90	112.0
72.10	2569.0
73.10	21744.0
74.10	81448.0
75.10	243904.0
76.10	21336.0
77.00	2765.0
78.00	1767.0
79.00	14616.0
80.00	3499.0
81.00	14975.0
82.00	2986.0
83.00	233.0
86.10	957.0
87.00	19128.0
88.00	19808.0
91.00	1706.0
92.10	13851.0
93.10	20592.0
94.10	53360.0
95.10	480128.0
96.10	30448.0
97.10	659.0
103.00	272.0
104.00	1911.0
104.90	533.0
106.00	1841.0
106.80	361.0
108.20	154.0
109.90	314.0
111.00	278.0
111.90	248.0
113.00	500.0
115.10	717.0
116.00	1263.0
117.00	3655.0
118.00	2149.0
119.00	2755.0
123.00	151.0
124.00	299.0
125.00	132.0
125.90	247.0
127.10	119.0
127.90	1633.0
129.00	1025.0
130.00	2007.0
131.10	531.0
135.00	848.0
135.90	249.0
137.00	773.0
138.90	274.0
140.10	511.0
141.00	5055.0
142.00	579.0
143.00	6601.0
143.90	172.0
145.00	1865.0
146.10	662.0
147.00	228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

148.00	1170.0
148.90	157.0
150.00	618.0
151.80	342.0
152.90	358.0
153.70	335.0
154.10	305.0
154.90	1145.0
156.10	184.0
157.00	1058.0
158.10	194.0
158.90	411.0
160.90	517.0
168.90	207.0
170.20	289.0
171.20	944.0
172.10	4424.0
174.00	361024.0
175.10	29584.0
176.00	354368.0
177.00	22552.0
178.00	405.0
207.20	149.0
221.30	144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	3811.0
37.10	19464.0
38.10	17696.0
39.10	8140.0
40.00	866.0
40.80	168.0
43.10	238.0
44.00	2791.0
45.10	3313.0
46.00	638.0
47.10	6113.0
47.90	2817.0
49.10	17344.0
50.10	86128.0
51.10	26072.0
52.10	1083.0
52.90	420.0
53.90	212.0
55.10	950.0
56.00	5645.0
57.10	11617.0
58.10	351.0
58.90	127.0
60.10	3863.0
61.10	21400.0
62.00	21544.0
63.10	16824.0
64.00	2755.0
65.10	3974.0
66.00	225.0
67.00	1289.0
68.10	44304.0
69.10	46520.0
70.10	3306.0
72.10	2281.0
73.10	19736.0
74.10	74664.0
75.10	226112.0
76.10	18704.0
77.00	2629.0
77.90	1571.0
79.00	13399.0
80.00	3479.0
81.00	13445.0
82.00	2692.0
83.00	350.0
86.10	879.0
87.00	17536.0
88.00	17808.0
91.00	1624.0
92.10	12768.0
93.10	18536.0
94.10	49704.0
95.10	448512.0
96.10	28616.0
97.00	621.0
102.90	244.0
104.00	1928.0
105.00	466.0
105.90	1587.0
106.80	413.0
109.90	321.0
111.00	235.0
112.00	294.0
113.00	507.0
115.10	588.0
116.10	1369.0
117.00	3409.0
118.00	1715.0
119.00	2412.0
123.10	143.0
124.00	241.0
125.00	100.0
125.90	154.0
128.00	1292.0
129.00	975.0
130.00	1849.0
131.00	427.0
135.00	688.0
136.00	258.0
137.00	815.0
138.90	214.0
140.10	550.0
141.00	4612.0
142.00	531.0
143.00	6259.0
144.20	166.0
145.00	1437.0
146.10	561.0
147.00	249.0
147.90	1070.0
149.00	219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

149.90	670.0
151.80	205.0
152.00	212.0
152.90	350.0
153.70	235.0
154.10	267.0
154.90	1166.0
156.10	132.0
157.00	1001.0
157.90	157.0
158.90	414.0
161.00	429.0
168.90	179.0
170.30	354.0
171.20	725.0
172.00	4068.0
174.00	342144.0
175.00	28216.0
176.00	336640.0
177.00	20832.0
178.00	530.0
207.20	152.0
221.30	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Scan 2851 (10.257 min): VU030948.D
BFB04

m/z	Abundance
40.00	390.0
41.10	108.0
44.00	806.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	4090.0
37.10	21312.0
38.10	20368.0
39.10	9263.0
40.00	949.0
40.80	164.0
43.10	211.0
44.00	3282.0
45.10	3351.0
46.00	625.0
47.10	6490.0
47.90	2736.0
49.10	19632.0
50.10	90888.0
51.10	28872.0
52.00	989.0
53.10	353.0
54.00	228.0
55.10	1172.0
56.00	6333.0
57.10	12367.0
57.90	385.0
60.10	4658.0
61.10	23336.0
62.10	23216.0
63.10	19368.0
64.10	3093.0
65.10	4457.0
66.10	395.0
67.00	1329.0
68.10	46984.0
69.10	47848.0
70.10	3857.0
70.90	149.0
72.00	2570.0
73.10	21192.0
74.10	79160.0
75.10	236480.0
76.10	21656.0
77.00	2725.0
78.00	1916.0
79.00	14353.0
80.00	3515.0
81.00	15161.0
82.00	2983.0
83.10	190.0
86.10	965.0
87.00	19112.0
88.00	19408.0
91.00	1598.0
92.10	13625.0
93.10	20512.0
94.10	52704.0
95.10	459200.0
96.10	29088.0
97.10	691.0
103.00	286.0
104.00	1750.0
104.90	575.0
106.00	1928.0
107.10	326.0
108.10	181.0
109.80	274.0
110.90	319.0
112.00	209.0
112.90	446.0
115.10	633.0
115.90	1215.0
117.00	3558.0
118.00	2116.0
119.00	2903.0
120.00	127.0
121.90	102.0
123.00	133.0
124.00	278.0
125.00	159.0
125.90	270.0
127.10	141.0
127.90	1752.0
129.00	829.0
130.00	1968.0
131.10	609.0
135.00	900.0
135.90	214.0
137.00	667.0
138.80	244.0
141.00	4980.0
142.00	530.0
143.00	6190.0
143.90	253.0
145.00	2128.0
146.00	778.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

146.90	227.0
148.00	1155.0
148.80	183.0
150.00	527.0
151.80	397.0
153.00	273.0
153.80	288.0
154.10	259.0
154.90	947.0
156.10	186.0
157.00	931.0
158.10	258.0
158.80	393.0
160.90	570.0
168.90	175.0
170.00	216.0
171.10	1020.0
172.10	4502.0
174.00	340352.0
175.10	28072.0
176.00	334784.0
177.00	21928.0
178.00	369.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04