


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041019\
 Data File : VU031003.D
 Acq On : 10 Apr 2019 10:55
 Operator : JC/SP
 Sample : BFB05
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 11 02:07:02 2019

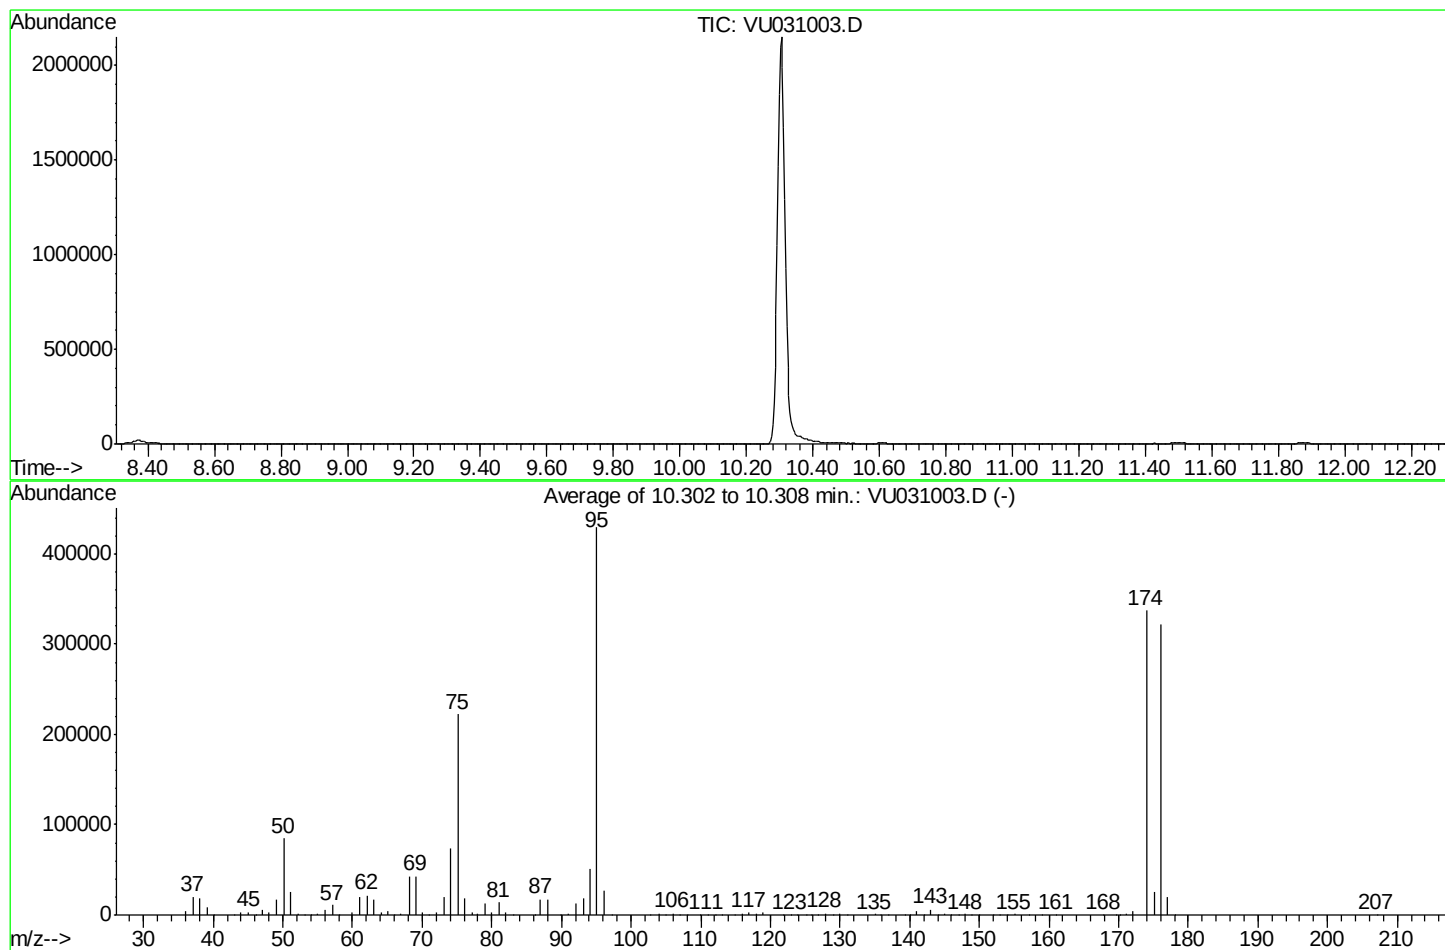

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	84712	PASS
75	95	30	80	51.7	221930	PASS
95	95	100	100	100.0	429333	PASS
96	95	5	9	6.3	27130	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.6	337280	PASS
175	174	5	9	7.5	25208	PASS
176	174	95	101	95.4	321792	PASS
177	176	5	9	6.3	20389	PASS

m/z	Abundance
36.10	3408.0
37.10	19280.0
38.10	16808.0
39.10	7125.0
40.10	658.0
43.10	243.0
44.00	2948.0
45.10	3130.0
46.10	532.0
47.00	4951.0
48.00	2705.0
49.10	17032.0
50.10	80112.0
51.10	24144.0
52.10	939.0
53.10	440.0
54.10	315.0
55.00	1045.0
56.00	5530.0
57.10	10236.0
58.00	401.0
60.00	3377.0
61.10	19416.0
62.10	20264.0
63.10	15681.0
64.10	2614.0
65.10	3377.0
66.00	257.0
66.90	1002.0
68.10	40792.0
69.10	40288.0
70.10	2827.0
72.00	2514.0
73.10	19128.0
74.10	69792.0
75.10	210688.0
76.10	17680.0
77.10	2907.0
77.90	1426.0
79.00	12506.0
79.90	3297.0
81.00	13060.0
82.00	2913.0
83.10	265.0
86.10	645.0
87.00	16392.0
88.00	15660.0
89.80	101.0
91.00	1571.0
92.10	12488.0
93.10	17624.0
94.10	48584.0
95.10	409664.0
96.10	25816.0
97.10	470.0
102.80	121.0
103.90	1774.0
104.90	727.0
106.00	1899.0
107.00	407.0
108.10	172.0
109.90	312.0
111.00	495.0
112.10	347.0
113.00	178.0
114.90	340.0
116.00	1492.0
116.90	2696.0
117.90	1232.0
119.00	2441.0
121.80	200.0
122.90	130.0
123.80	208.0
125.10	104.0
125.90	102.0
126.80	108.0
127.90	1629.0
129.10	634.0
129.90	1452.0
131.00	601.0
135.00	801.0
135.90	121.0
136.90	531.0
139.30	132.0
139.90	427.0
141.00	4587.0
142.10	528.0
143.00	6019.0
144.10	472.0
145.00	1737.0
145.90	845.0
147.00	345.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

148.00	789.0
148.80	174.0
150.00	538.0
151.90	275.0
152.90	458.0
154.00	310.0
155.10	1212.0
157.00	686.0
158.90	508.0
161.10	420.0
167.80	101.0
170.20	141.0
171.10	826.0
172.10	3890.0
174.00	330048.0
175.10	24024.0
176.10	313344.0
177.00	19304.0
178.00	512.0
207.00	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

Scan 2851 (10.257 min): VU031003.D
BFB05

m/z	Abundance
39.90	334.0
44.00	791.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.10	3768.0
37.10	20496.0
38.10	18880.0
39.10	8497.0
40.10	685.0
43.00	297.0
44.00	2918.0
45.10	3462.0
46.20	425.0
47.10	5199.0
48.00	2228.0
49.10	17688.0
50.10	86232.0
51.10	25632.0
52.10	1306.0
53.10	413.0
54.10	177.0
54.90	1166.0
56.10	5853.0
57.10	10992.0
58.10	316.0
60.00	3671.0
61.10	20712.0
62.00	22528.0
63.10	17904.0
64.10	3105.0
65.10	3730.0
66.00	329.0
67.00	1092.0
68.10	43976.0
69.10	44464.0
70.10	2784.0
71.00	136.0
72.10	2595.0
73.10	19296.0
74.10	75336.0
75.10	224704.0
76.10	19656.0
77.10	3051.0
78.00	2265.0
79.00	13892.0
80.00	3792.0
81.00	13639.0
81.90	3190.0
83.20	371.0
86.10	851.0
87.00	18000.0
88.00	17872.0
91.00	1518.0
92.10	12069.0
93.10	19704.0
94.10	52120.0
95.10	433536.0
96.10	27672.0
97.20	704.0
102.70	220.0
104.00	1911.0
104.80	617.0
105.90	2253.0
106.90	432.0
108.00	231.0
109.90	283.0
110.90	559.0
112.10	334.0
112.90	206.0
114.80	414.0
115.90	1564.0
117.00	2759.0
118.00	1156.0
118.90	2695.0
121.90	141.0
123.00	122.0
123.80	239.0
125.80	140.0
126.80	111.0
127.90	1633.0
129.10	626.0
129.90	1685.0
131.00	643.0
135.00	780.0
136.90	715.0
139.90	278.0
141.00	4615.0
142.10	851.0
143.00	6303.0
144.00	464.0
145.00	2059.0
145.90	539.0
146.90	274.0
148.00	1103.0
148.80	302.0
150.00	342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

151.90	338.0
153.00	434.0
153.90	278.0
155.10	1165.0
157.10	617.0
158.90	693.0
161.00	462.0
169.70	138.0
171.10	1043.0
172.10	4272.0
174.00	333440.0
175.10	25792.0
176.00	319552.0
177.00	20720.0
178.00	438.0
207.10	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.10	3895.0
37.10	21040.0
38.10	18632.0
39.10	8054.0
40.10	662.0
43.00	254.0
44.00	3107.0
45.10	3492.0
46.10	473.0
47.00	5362.0
48.00	2508.0
49.10	18280.0
50.10	87792.0
51.10	26072.0
52.10	1176.0
53.10	419.0
54.10	300.0
55.00	1072.0
56.10	5823.0
57.10	11005.0
58.00	364.0
60.00	3599.0
61.10	20688.0
62.10	22464.0
63.10	17768.0
64.10	3039.0
65.10	3770.0
66.00	321.0
66.90	1125.0
68.10	44032.0
69.10	44368.0
70.10	2902.0
71.00	127.0
72.10	2773.0
73.10	20320.0
74.10	76552.0
75.10	230400.0
76.10	19520.0
77.10	3320.0
78.00	1901.0
79.00	13824.0
79.90	3638.0
81.00	14051.0
82.00	3190.0
83.10	368.0
86.10	787.0
87.00	18080.0
88.00	17944.0
91.00	1638.0
92.10	12743.0
93.10	19560.0
94.10	52816.0
95.10	444800.0
96.10	27904.0
97.10	551.0
102.80	172.0
103.90	1993.0
104.80	706.0
106.00	2063.0
106.90	444.0
108.10	225.0
109.90	373.0
111.00	601.0
112.10	417.0
112.90	198.0
114.80	371.0
116.00	1598.0
116.90	2808.0
117.90	1219.0
118.90	2660.0
121.80	171.0
122.90	126.0
123.80	226.0
125.10	112.0
125.80	137.0
126.80	137.0
127.90	1838.0
129.10	700.0
129.90	1708.0
131.00	673.0
135.00	819.0
136.90	648.0
139.30	147.0
140.00	406.0
141.00	4934.0
142.10	767.0
143.00	6641.0
144.10	508.0
145.00	1991.0
145.90	729.0
146.90	331.0
148.00	962.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

148.80	273.0
150.00	528.0
151.90	338.0
152.90	477.0
154.00	297.0
155.10	1320.0
157.00	728.0
158.90	613.0
161.10	500.0
169.70	140.0
170.20	124.0
171.10	992.0
172.10	4401.0
174.00	348352.0
175.10	25808.0
176.00	332480.0
177.00	21144.0
178.00	494.0
207.10	219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05