




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053610.D
 Acq On : 10 Apr 2023 11:16
 Operator : JC/MD
 Sample : 02251-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0MC5

Manual IntegrationsAPPROVED

Quant Time: Apr 11 02:21:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 11 02:19:45 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
 Supervised By :Mahesh Dadoda 04/11/2023

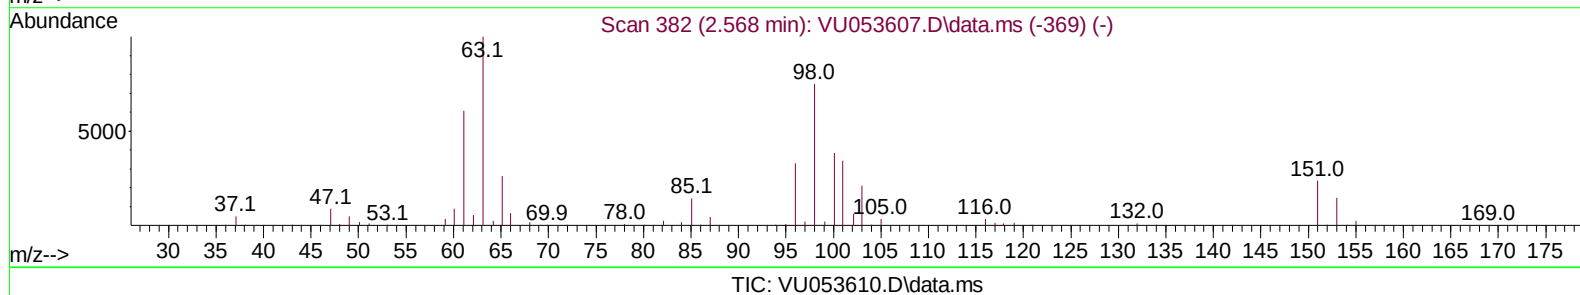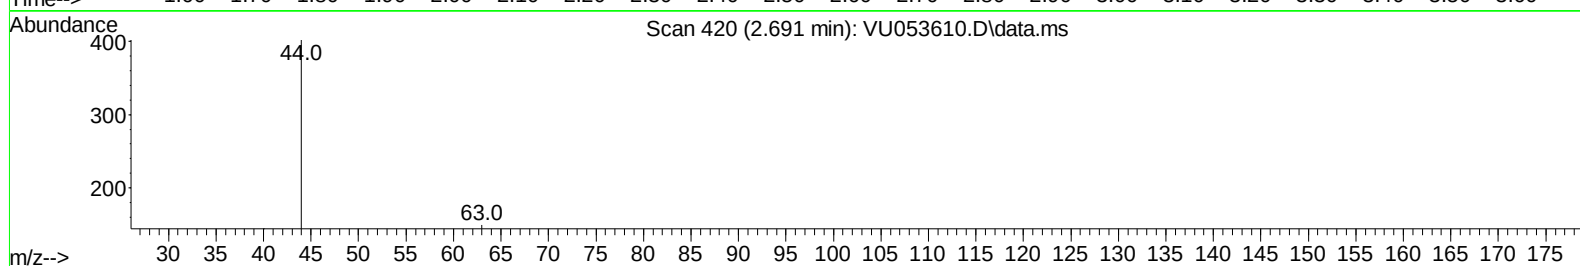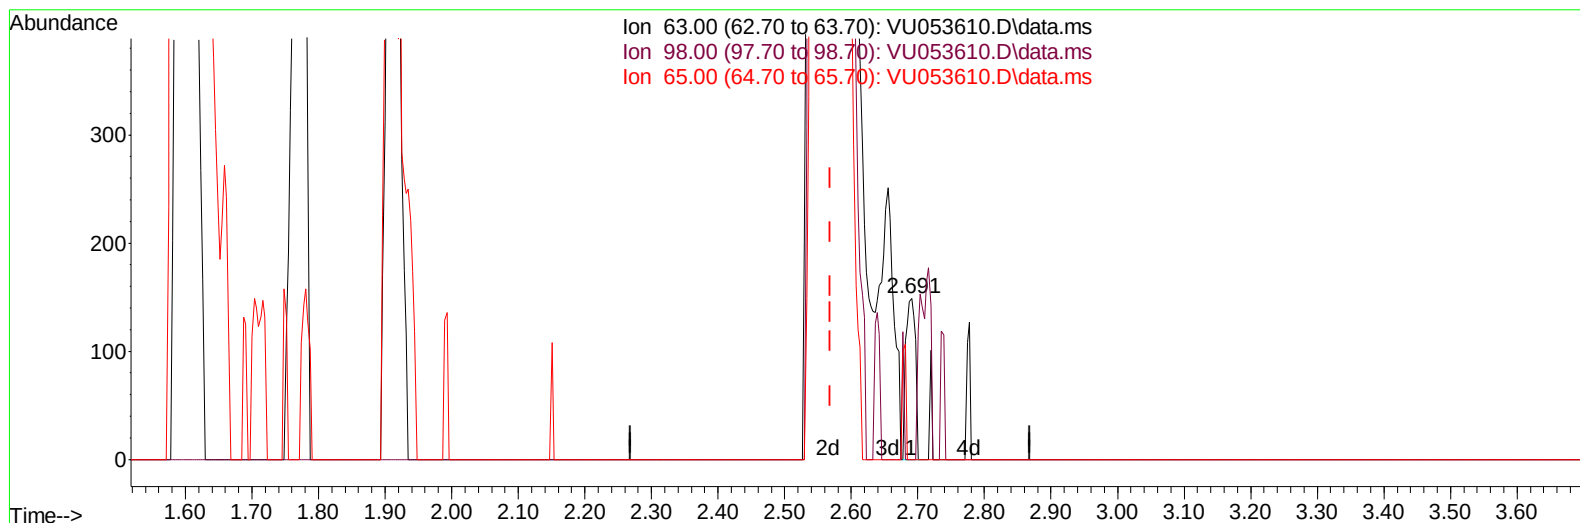

(11) 1,1-Dichloroethene-d2 (S)

2.691min (+ 0.122) 0.05 ug/L

response 149

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	85.20	70.47
65.00	24.60	26.85
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053610.D
 Acq On : 10 Apr 2023 11:16
 Operator : JC/MD
 Sample : 02251-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0MC5

Manual IntegrationsAPPROVED

Quant Time: Apr 11 02:21:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 11 02:19:45 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
 Supervised By :Mahesh Dadoda 04/11/2023

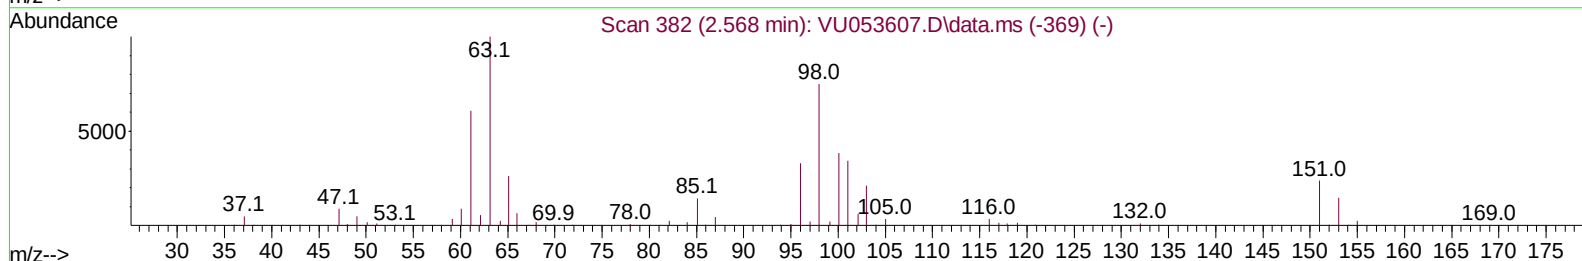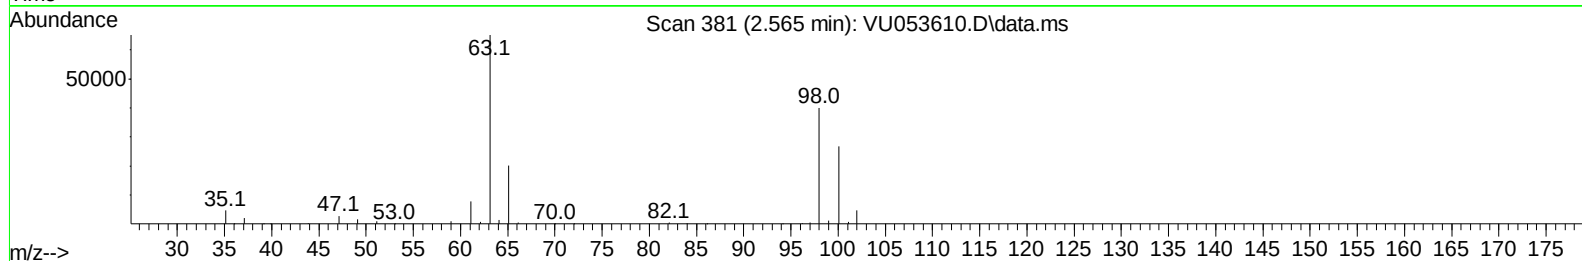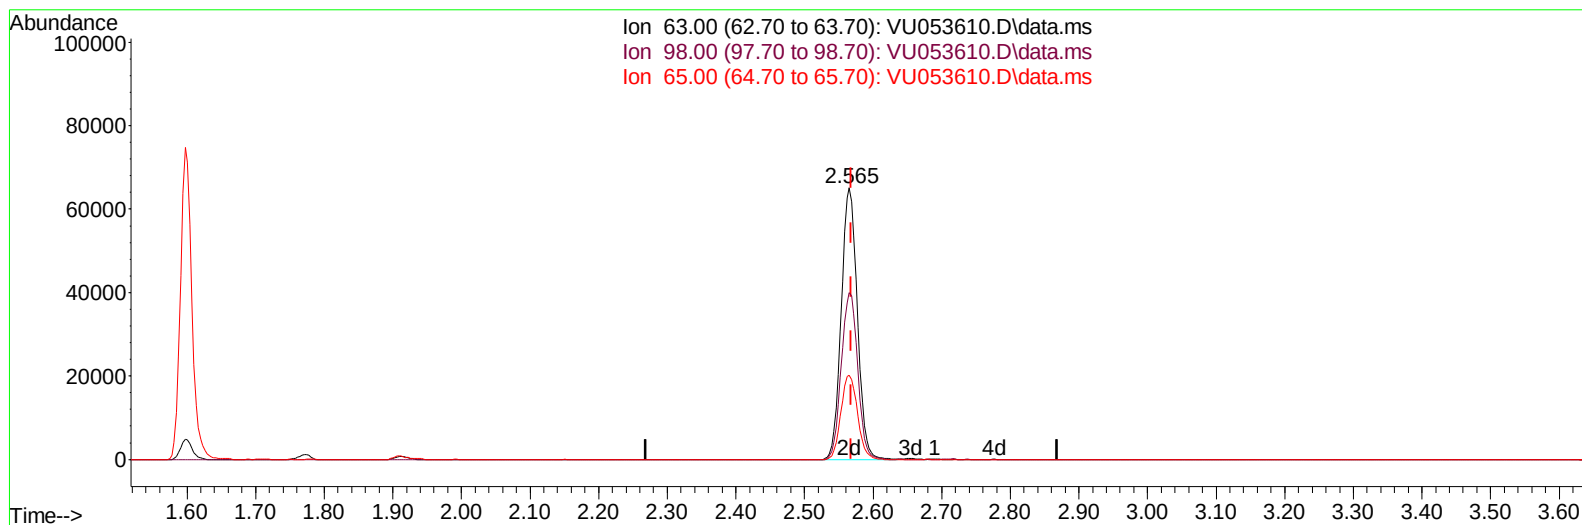

TIC: VU053610.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.565min (-0.003) 34.38 ug/L m

response 105563

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	85.20	0.10#
65.00	24.60	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053610.D
 Acq On : 10 Apr 2023 11:16
 Operator : JC/MD
 Sample : 02251-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC5

Manual IntegrationsAPPROVED

Quant Time: Apr 11 02:21:07 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 11 02:19:45 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
 Supervised By :Mahesh Dadoda 04/11/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	254776	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	236814	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	118871	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	86387	43.545	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	87.100%	
7) Chloroethane-d5	1.909	69	73626	48.134	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	96.260%	
11) 1,1-Dichloroethene-d2	2.565	63	105563m	34.375	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	68.760%	
21) 2-Butanone-d5	4.613	46	98026	109.136	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	109.140%	
24) Chloroform-d	5.057	84	149197	45.474	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.940%	
26) 1,2-Dichloroethane-d4	5.694	65	94943	48.972	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.940%	
32) Benzene-d6	5.723	84	310813	48.623	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.240%	
36) 1,2-Dichloropropane-d6	6.684	67	96825	49.557	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	99.120%	
41) Toluene-d8	7.893	98	284196	44.732	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.460%	
43) trans-1,3-Dichloroprop...	8.173	79	46209	45.817	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	91.640%	
47) 2-Hexanone-d5	8.626	63	72099	108.125	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	108.120%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	134365	48.792	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	97.580%	
66) 1,2-Dichlorobenzene-d4	12.189	152	110276	44.443	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	88.880%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053610.D
Acq On : 10 Apr 2023 11:16
Operator : JC/MD
Sample : 02251-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC5

Manual IntegrationsAPPROVED

Quant Time: Apr 11 02:21:07 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 11 02:19:45 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
Supervised By :Mahesh Dadoda 04/11/2023

