

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053608.D
 Acq On : 10 Apr 2023 10:22
 Operator : JC/MD
 Sample : VU0410WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK075

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	125690	144883	16.43%	2.090%
2	1.912	170	178	195	rVB	102332	138906	15.75%	2.004%
3	2.565	369	381	404	rBV	187026	309983	35.15%	4.471%
4	2.793	444	452	459	rVB2	1072	1500	0.17%	0.022%
5	3.044	522	530	541	rVB4	5508	9185	1.04%	0.132%
6	3.263	594	598	601	rBV2	362	348	0.04%	0.005%
7	3.555	686	689	692	rBV	250	157	0.02%	0.002%
8	3.745	744	748	751	rBV	317	209	0.02%	0.003%
9	3.874	786	788	790	rBV	228	130	0.01%	0.002%
10	3.890	790	793	796	rVV2	255	177	0.02%	0.003%
11	3.906	796	798	802	rVB	192	111	0.01%	0.002%
12	3.957	812	814	817	rBV	250	173	0.02%	0.002%
13	4.079	849	852	854	rBV2	277	205	0.02%	0.003%
14	4.369	937	942	946	rBV	248	267	0.03%	0.004%
15	4.533	991	993	994	rBV	225	76	0.01%	0.001%
16	4.616	1007	1019	1048	rBV	67990	169468	19.22%	2.444%
17	4.954	1121	1124	1127	rVB	284	176	0.02%	0.003%
18	4.986	1129	1134	1139	rBV2	198	224	0.03%	0.003%
19	5.057	1139	1156	1178	rBV	165392	367455	41.67%	5.300%
20	5.372	1250	1254	1255	rBV	281	139	0.02%	0.002%
21	5.485	1286	1289	1292	rBV	260	173	0.02%	0.002%
22	5.584	1317	1320	1322	rBV	153	82	0.01%	0.001%
23	5.600	1323	1325	1330	rVB2	269	176	0.02%	0.003%
24	5.719	1341	1362	1384	rBV2	321210	881781	100.00%	12.719%
25	5.964	1434	1438	1440	rBV2	311	215	0.02%	0.003%
26	6.018	1452	1455	1459	rBV	285	273	0.03%	0.004%
27	6.086	1473	1476	1479	rBV	159	118	0.01%	0.002%
28	6.102	1479	1481	1482	rBV	189	79	0.01%	0.001%
29	6.137	1490	1492	1494	rBV	179	105	0.01%	0.002%
30	6.166	1498	1501	1504	rVB	225	136	0.02%	0.002%
31	6.192	1507	1509	1512	rBV	205	145	0.02%	0.002%
32	6.243	1512	1525	1545	rBV	286248	544171	61.71%	7.849%
33	6.491	1598	1602	1604	rBV2	334	282	0.03%	0.004%
34	6.526	1605	1613	1626	rVB6	4695	8749	0.99%	0.126%
35	6.587	1629	1632	1634	rBV	272	163	0.02%	0.002%
36	6.687	1648	1663	1683	rBV	204790	397089	45.03%	5.728%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053608.D
 Acq On : 10 Apr 2023 10:22
 Operator : JC/MD
 Sample : VU0410WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK075

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.845	1711	1712	1718	rVB2	228	142	0.02%	0.002%
38	6.899	1726	1729	1735	rVB	356	321	0.04%	0.005%
39	6.970	1748	1751	1754	rBV2	230	151	0.02%	0.002%
40	7.083	1783	1786	1790	rVB	207	122	0.01%	0.002%
41	7.111	1790	1795	1800	rBV	313	289	0.03%	0.004%
42	7.243	1834	1836	1837	rBV	197	82	0.01%	0.001%
43	7.269	1842	1844	1847	rVB	302	163	0.02%	0.002%
44	7.298	1851	1853	1857	rVB2	180	134	0.02%	0.002%
45	7.365	1871	1874	1879	rBV2	284	240	0.03%	0.003%
46	7.459	1900	1903	1909	rVB2	303	285	0.03%	0.004%
47	7.562	1923	1935	1953	rBV	115824	207265	23.51%	2.990%
48	7.697	1969	1977	1984	rBV3	964	1447	0.16%	0.021%
49	7.726	1984	1986	1990	rVB	343	127	0.01%	0.002%
50	7.790	2003	2006	2009	rBV	545	363	0.04%	0.005%
51	7.893	2025	2038	2068	rBV	413150	724617	82.18%	10.452%
52	8.105	2102	2104	2111	rVB	264	183	0.02%	0.003%
53	8.176	2115	2126	2149	rVV	79459	136952	15.53%	1.975%
54	8.295	2161	2163	2164	rBV	228	69	0.01%	0.001%
55	8.330	2170	2174	2177	rBV	426	388	0.04%	0.006%
56	8.378	2185	2189	2191	rBV	297	219	0.02%	0.003%
57	8.552	2238	2243	2250	rVB6	1053	1307	0.15%	0.019%
58	8.629	2255	2267	2299	rBV	201151	380697	43.17%	5.491%
59	8.848	2333	2335	2341	rVB3	279	195	0.02%	0.003%
60	8.938	2359	2363	2365	rBV	248	197	0.02%	0.003%
61	9.066	2401	2403	2406	rBV	166	92	0.01%	0.001%
62	9.095	2409	2412	2415	rBV	259	176	0.02%	0.003%
63	9.240	2454	2457	2458	rBV	174	83	0.01%	0.001%
64	9.327	2482	2484	2486	rBV2	115	62	0.01%	0.001%
65	9.414	2497	2511	2539	rBV	388868	652587	74.01%	9.413%
66	9.536	2547	2549	2553	rBV3	324	197	0.02%	0.003%
67	9.603	2568	2570	2573	rBV	226	131	0.01%	0.002%
68	9.639	2578	2581	2583	rBV	172	100	0.01%	0.001%
69	9.938	2669	2674	2677	rBV2	296	333	0.04%	0.005%
70	10.012	2694	2697	2702	rVB2	347	300	0.03%	0.004%
71	10.031	2702	2703	2704	rBV	264	65	0.01%	0.001%
72	10.063	2710	2713	2716	rBV	284	207	0.02%	0.003%
73	10.092	2719	2722	2724	rBV2	424	309	0.04%	0.004%
74	10.243	2766	2769	2770	rBV2	163	73	0.01%	0.001%
75	10.635	2883	2891	2901	rVB4	4756	7317	0.83%	0.106%
76	10.693	2907	2909	2912	rVB	239	115	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053608.D
 Acq On : 10 Apr 2023 10:22
 Operator : JC/MD
 Sample : VU0410WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK075

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.751	2914	2927	2945	rBV	282877	455687	51.68%	6.573%
78	10.864	2959	2962	2965	rBV2	359	235	0.03%	0.003%
79	11.134	3044	3046	3048	rBV2	245	121	0.01%	0.002%
80	11.188	3060	3063	3069	rBV	330	268	0.03%	0.004%
81	11.227	3072	3075	3077	rBV	199	103	0.01%	0.001%
82	11.269	3085	3088	3091	rBV	239	164	0.02%	0.002%
83	11.414	3130	3133	3135	rBV2	321	239	0.03%	0.003%
84	11.680	3212	3216	3217	rBV	255	168	0.02%	0.002%
85	11.748	3230	3237	3243	rVB4	1938	2761	0.31%	0.040%
86	11.809	3244	3256	3274	rBV	418243	668678	75.83%	9.645%
87	11.999	3313	3315	3317	rBV	354	201	0.02%	0.003%
88	12.131	3354	3356	3361	rBV	250	203	0.02%	0.003%
89	12.188	3361	3374	3395	rBV	415879	676850	76.76%	9.763%
90	12.385	3434	3435	3438	rBV	202	101	0.01%	0.001%
91	12.584	3493	3497	3502	rBV2	283	360	0.04%	0.005%
92	12.822	3569	3571	3573	rBV	165	91	0.01%	0.001%
93	13.221	3691	3695	3702	rBV4	1637	1905	0.22%	0.027%
94	13.413	3753	3755	3759	rBV2	328	238	0.03%	0.003%
95	13.719	3847	3850	3852	rBV2	314	239	0.03%	0.003%
96	13.809	3875	3878	3879	rBV	303	163	0.02%	0.002%
97	13.838	3880	3887	3899	rVB5	5591	8980	1.02%	0.130%
98	14.089	3957	3965	3981	rBV2	7383	12622	1.43%	0.182%
99	14.198	3996	3999	4001	rBV2	456	305	0.03%	0.004%
100	14.327	4034	4039	4051	rVB5	4358	6621	0.75%	0.096%


Sum of corrected areas: 6932914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053608.D
Acq On : 10 Apr 2023 10:22
Operator : JC/MD
Sample : VU0410WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

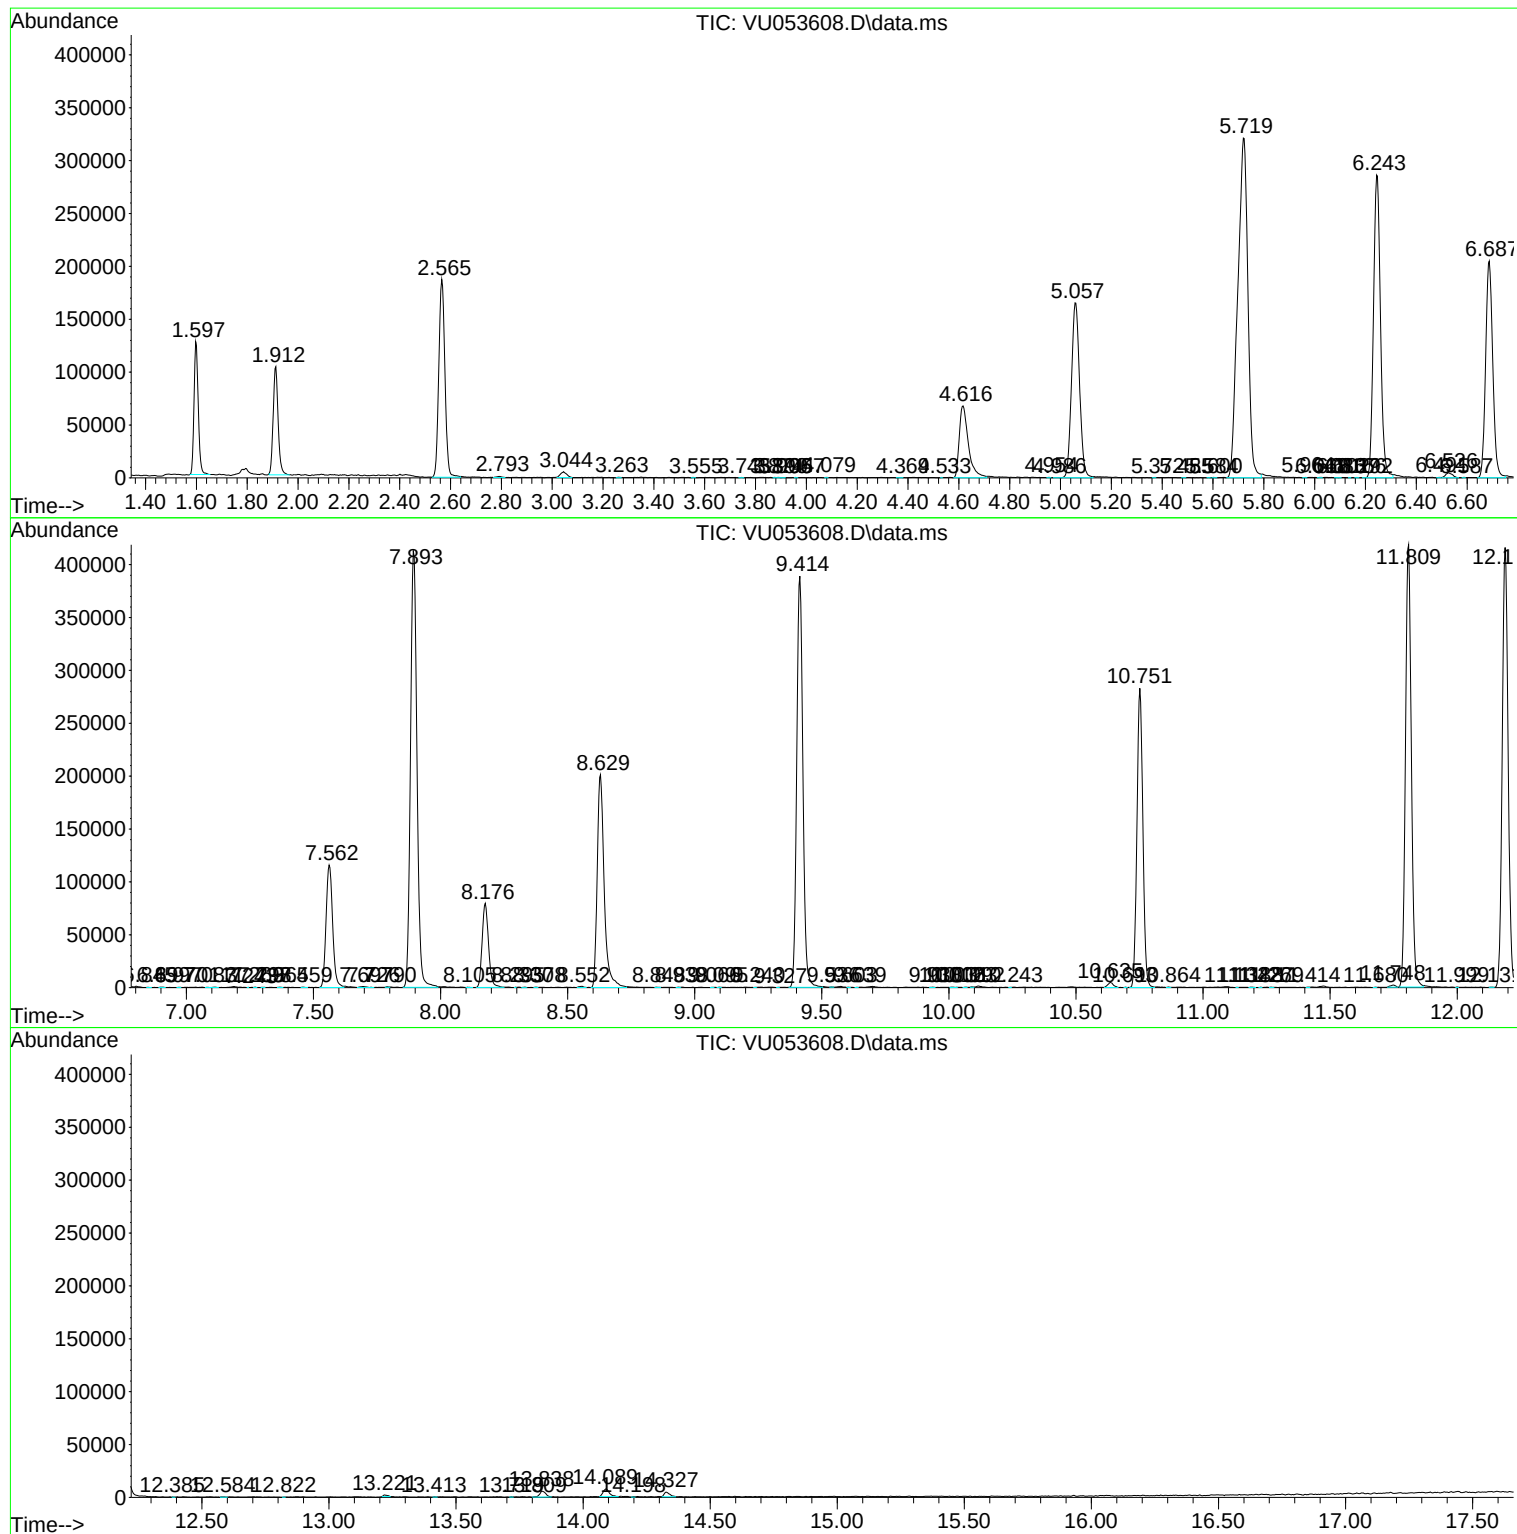

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053608.D
Acq On : 10 Apr 2023 10:22
Operator : JC/MD
Sample : VU0410WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053608.D
Acq On : 10 Apr 2023 10:22
Operator : JC/MD
Sample : VU0410WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------