

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053609.D
 Acq On : 10 Apr 2023 10:52
 Operator : JC/MD
 Sample : 02251-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	124068	142278	16.59%	2.041%
2	1.912	169	178	195	rVB	98817	135285	15.77%	1.941%
3	2.565	369	381	398	rBV	186434	304160	35.46%	4.364%
4	2.707	422	425	429	rBV2	503	304	0.04%	0.004%
5	2.752	436	439	440	rBV2	605	387	0.05%	0.006%
6	3.038	524	528	538	rVB3	1277	1894	0.22%	0.027%
7	3.176	568	571	572	rBV	442	273	0.03%	0.004%
8	3.401	639	641	645	rVB	255	136	0.02%	0.002%
9	3.424	645	648	651	rBV	234	199	0.02%	0.003%
10	3.642	713	716	717	rBV	196	85	0.01%	0.001%
11	3.681	725	728	730	rBV	216	132	0.02%	0.002%
12	3.703	733	735	737	rBV2	166	80	0.01%	0.001%
13	3.880	787	790	791	rBV2	244	126	0.01%	0.002%
14	4.031	834	837	839	rBV	177	143	0.02%	0.002%
15	4.125	862	866	870	rBV2	258	237	0.03%	0.003%
16	4.208	889	892	895	rBV	218	157	0.02%	0.002%
17	4.247	901	904	907	rBV	235	158	0.02%	0.002%
18	4.414	953	956	959	rVB	220	118	0.01%	0.002%
19	4.475	972	975	977	rBV	164	106	0.01%	0.002%
20	4.530	989	992	995	rBV2	240	171	0.02%	0.002%
21	4.617	1008	1019	1046	rBV2	63047	157333	18.34%	2.257%
22	4.941	1117	1120	1123	rBV2	201	158	0.02%	0.002%
23	4.996	1135	1137	1139	rBV	212	92	0.01%	0.001%
24	5.060	1140	1157	1177	rBV	154557	356190	41.52%	5.111%
25	5.379	1254	1256	1258	rBV	189	76	0.01%	0.001%
26	5.456	1279	1280	1281	rBV	135	41	0.00%	0.001%
27	5.507	1291	1296	1302	rBV2	265	400	0.05%	0.006%
28	5.565	1311	1314	1317	rBV2	240	169	0.02%	0.002%
29	5.584	1317	1320	1322	rVB	139	58	0.01%	0.001%
30	5.594	1322	1323	1325	rBV2	256	99	0.01%	0.001%
31	5.633	1330	1335	1338	rBV2	393	405	0.05%	0.006%
32	5.719	1342	1362	1384	rBV2	310941	857832	100.00%	12.308%
33	6.086	1474	1476	1478	rBV	173	87	0.01%	0.001%
34	6.115	1483	1485	1489	rBV	324	271	0.03%	0.004%
35	6.247	1512	1526	1543	rBV	316122	601896	70.16%	8.636%
36	6.523	1605	1612	1616	rBV5	3273	4627	0.54%	0.066%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053609.D
 Acq On : 10 Apr 2023 10:52
 Operator : JC/MD
 Sample : 02251-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.568	1623	1626	1628	rBV	318	137	0.02%	0.002%
38	6.626	1641	1644	1649	rVB2	308	278	0.03%	0.004%
39	6.687	1649	1663	1682	rBV	193268	382829	44.63%	5.493%
40	6.842	1709	1711	1715	rVB	254	151	0.02%	0.002%
41	6.874	1718	1721	1724	rBV	182	85	0.01%	0.001%
42	7.141	1801	1804	1806	rBV2	356	240	0.03%	0.003%
43	7.272	1838	1845	1848	rBV2	235	299	0.03%	0.004%
44	7.327	1860	1862	1864	rBV	195	106	0.01%	0.002%
45	7.359	1870	1872	1875	rBV	137	81	0.01%	0.001%
46	7.520	1919	1922	1923	rBV	164	75	0.01%	0.001%
47	7.562	1923	1935	1959	rBV	111328	199751	23.29%	2.866%
48	7.896	2025	2039	2069	rBV	410670	721856	84.15%	10.357%
49	8.176	2114	2126	2142	rBV	80607	135402	15.78%	1.943%
50	8.343	2175	2178	2181	rBV2	374	232	0.03%	0.003%
51	8.436	2199	2207	2209	rBV	225	326	0.04%	0.005%
52	8.542	2237	2240	2241	rBV2	486	284	0.03%	0.004%
53	8.629	2255	2267	2296	rBV2	192906	360203	41.99%	5.168%
54	8.813	2322	2324	2329	rBV	312	256	0.03%	0.004%
55	8.835	2329	2331	2332	rBV	321	106	0.01%	0.002%
56	9.076	2402	2406	2408	rBV	311	267	0.03%	0.004%
57	9.247	2457	2459	2461	rVB	162	63	0.01%	0.001%
58	9.285	2469	2471	2476	rBV	201	101	0.01%	0.001%
59	9.349	2487	2491	2494	rBV2	188	130	0.02%	0.002%
60	9.414	2497	2511	2535	rBV	429795	715561	83.42%	10.267%
61	9.694	2593	2598	2606	rVV2	682	831	0.10%	0.012%
62	9.732	2608	2610	2612	rVB	234	91	0.01%	0.001%
63	9.780	2622	2625	2627	rVB	223	98	0.01%	0.001%
64	9.877	2652	2655	2657	rBV	223	156	0.02%	0.002%
65	10.012	2696	2697	2698	rBV	121	34	0.00%	0.000%
66	10.108	2723	2727	2728	rBV2	684	531	0.06%	0.008%
67	10.337	2795	2798	2800	rBV	175	118	0.01%	0.002%
68	10.411	2817	2821	2824	rBV	295	264	0.03%	0.004%
69	10.751	2916	2927	2942	rBV	269644	433069	50.48%	6.214%
70	10.890	2962	2970	2980	rVB4	1106	1596	0.19%	0.023%
71	11.253	3080	3083	3086	rVB	294	151	0.02%	0.002%
72	11.266	3086	3087	3090	rBV	169	69	0.01%	0.001%
73	11.497	3155	3159	3162	rBV2	296	258	0.03%	0.004%
74	11.748	3230	3237	3242	rVB3	1317	1803	0.21%	0.026%
75	11.809	3244	3256	3273	rBV	468724	747292	87.11%	10.722%
76	12.189	3362	3374	3393	rBV	417443	684184	79.76%	9.817%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053609.D
 Acq On : 10 Apr 2023 10:52
 Operator : JC/MD
 Sample : 02251-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0MC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	12.398	3438	3439	3443	rVB2	332	166	0.02%	0.002%
78	12.420	3443	3446	3448	rBV	284	168	0.02%	0.002%
79	12.796	3560	3563	3566	rBV	264	186	0.02%	0.003%
80	12.938	3605	3607	3610	rVB	359	129	0.02%	0.002%
81	13.063	3643	3646	3648	rBV	458	224	0.03%	0.003%
82	13.217	3691	3694	3700	rBV4	974	1055	0.12%	0.015%
83	13.324	3724	3727	3728	rBV2	356	198	0.02%	0.003%
84	13.558	3799	3800	3804	rVB2	390	154	0.02%	0.002%
85	13.652	3827	3829	3832	rBV	303	165	0.02%	0.002%
86	13.764	3861	3864	3867	rBV2	412	352	0.04%	0.005%
87	13.844	3882	3889	3899	rVB4	4078	5744	0.67%	0.082%
88	14.031	3944	3947	3948	rBV	387	218	0.03%	0.003%
89	14.092	3960	3966	3975	rBV2	3504	5022	0.59%	0.072%
90	14.465	4079	4082	4084	rBV	441	316	0.04%	0.005%




Sum of corrected areas: 6969624

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053609.D
Acq On : 10 Apr 2023 10:52
Operator : JC/MD
Sample : 02251-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

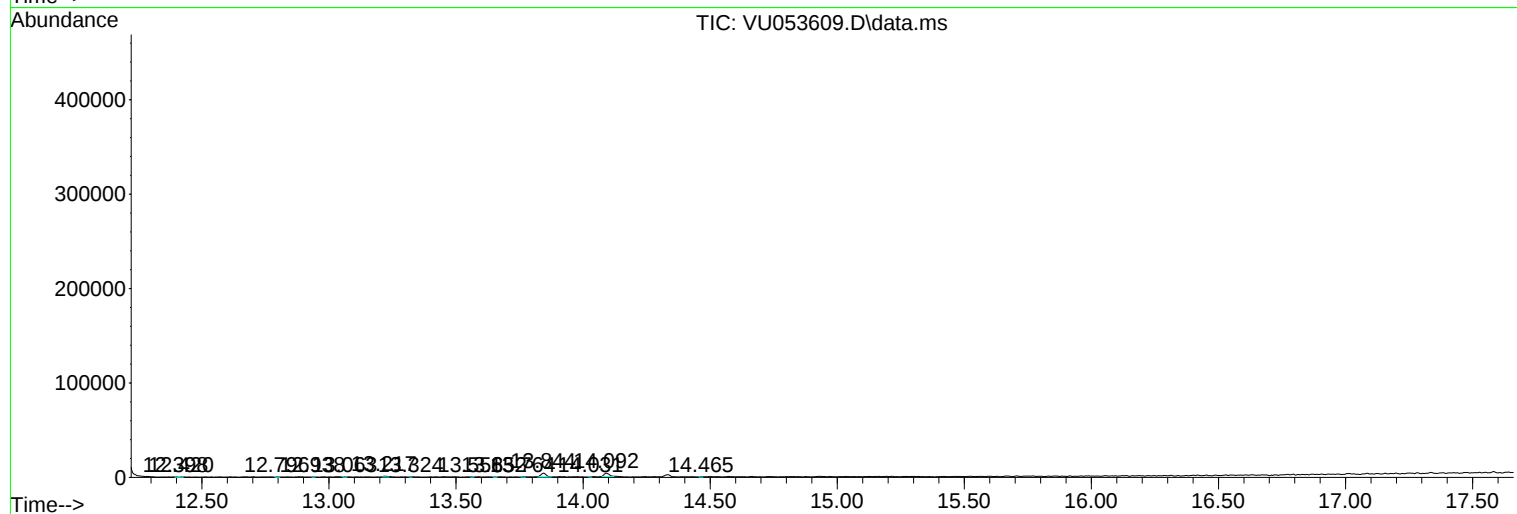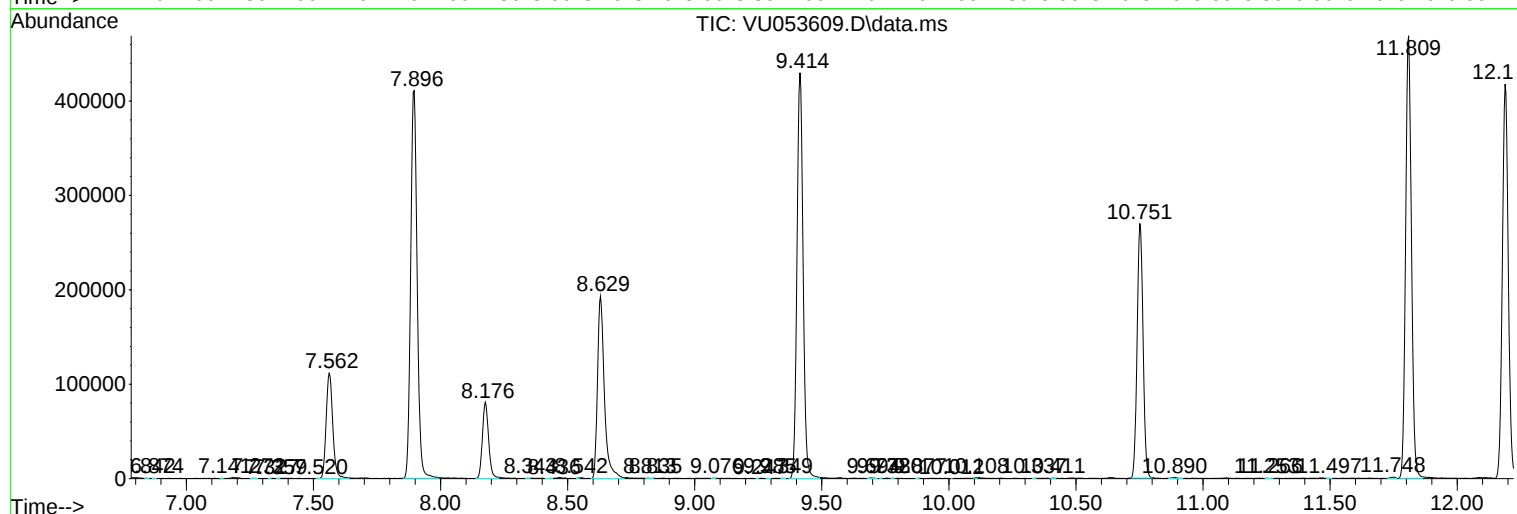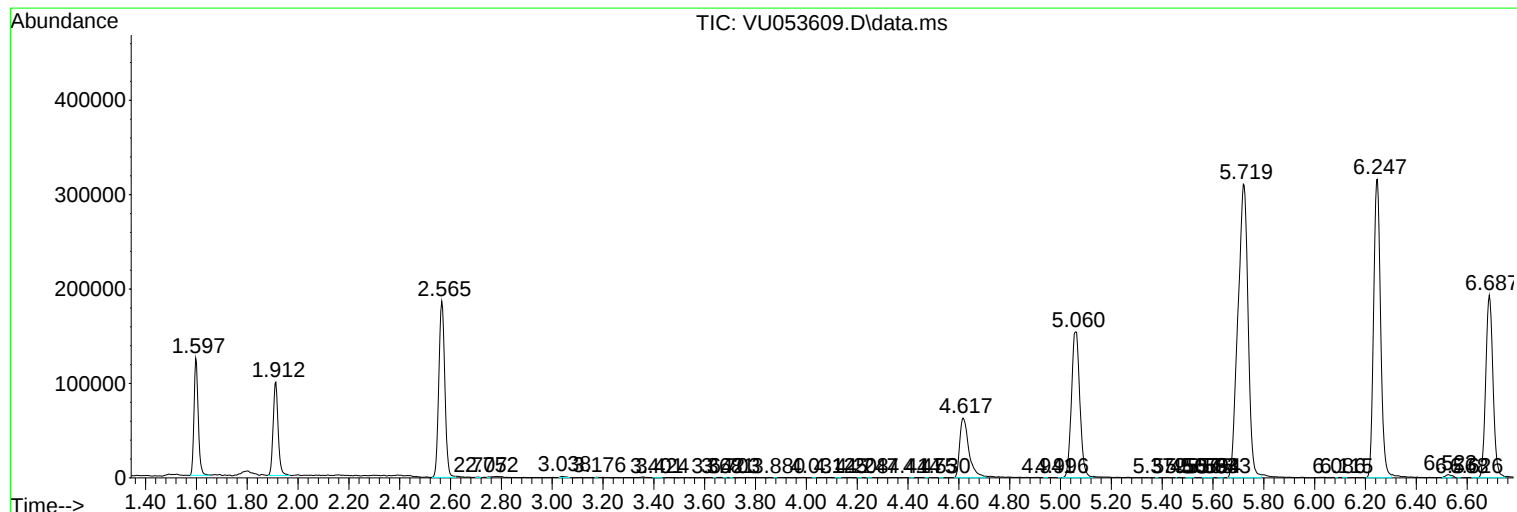

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053609.D
Acq On : 10 Apr 2023 10:52
Operator : JC/MD
Sample : 02251-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053609.D
Acq On : 10 Apr 2023 10:52
Operator : JC/MD
Sample : 02251-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------