

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053610.D
 Acq On : 10 Apr 2023 11:16
 Operator : JC/MD
 Sample : 02251-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	119814	136082	15.73%	1.989%
2	1.909	169	177	193	rVB	94722	133021	15.37%	1.945%
3	2.565	369	381	397	rBV	185251	302208	34.93%	4.418%
4	2.777	444	447	448	rBV	367	217	0.03%	0.003%
5	2.928	491	494	497	rVV2	326	225	0.03%	0.003%
6	2.945	497	499	503	rVB3	365	195	0.02%	0.003%
7	2.980	506	510	518	rBV2	426	653	0.08%	0.010%
8	3.041	523	529	537	rVB3	1547	2518	0.29%	0.037%
9	3.092	537	545	548	rBV2	355	425	0.05%	0.006%
10	3.163	564	567	569	rBV	324	219	0.03%	0.003%
11	3.240	587	591	594	rBV	227	195	0.02%	0.003%
12	3.356	624	627	630	rBV2	279	163	0.02%	0.002%
13	3.411	639	644	647	rBV2	264	250	0.03%	0.004%
14	3.572	691	694	698	rVB	186	158	0.02%	0.002%
15	3.639	712	715	719	rVB	285	171	0.02%	0.002%
16	3.703	730	735	740	rBV2	254	328	0.04%	0.005%
17	3.761	749	753	758	rBV	254	258	0.03%	0.004%
18	3.928	800	805	807	rBV	253	213	0.02%	0.003%
19	4.018	828	833	839	rVB	296	265	0.03%	0.004%
20	4.076	846	851	853	rBV2	210	150	0.02%	0.002%
21	4.163	874	878	881	rBV	246	185	0.02%	0.003%
22	4.507	981	985	988	rBV2	223	157	0.02%	0.002%
23	4.526	988	991	993	rBV	241	198	0.02%	0.003%
24	4.613	1006	1018	1046	rBV	69784	166886	19.29%	2.440%
25	4.928	1113	1116	1118	rBV2	386	246	0.03%	0.004%
26	5.057	1139	1156	1181	rBV	160614	351420	40.62%	5.138%
27	5.237	1210	1212	1217	rVB2	462	278	0.03%	0.004%
28	5.311	1231	1235	1237	rBV2	393	265	0.03%	0.004%
29	5.488	1285	1290	1295	rVB2	286	362	0.04%	0.005%
30	5.539	1295	1306	1309	rBV2	307	462	0.05%	0.007%
31	5.719	1341	1362	1397	rBV2	313841	865216	100.00%	12.649%
32	6.038	1455	1461	1465	rVV4	568	511	0.06%	0.007%
33	6.057	1465	1467	1470	rVB2	305	179	0.02%	0.003%
34	6.134	1489	1491	1494	rVB	314	167	0.02%	0.002%
35	6.243	1512	1525	1544	rBV	295693	565155	65.32%	8.262%
36	6.526	1603	1613	1614	rBV4	3471	4162	0.48%	0.061%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053610.D
 Acq On : 10 Apr 2023 11:16
 Operator : JC/MD
 Sample : 02251-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.626	1641	1644	1648	rBV2	251	208	0.02%	0.003%
38	6.687	1648	1663	1683	rBV	194174	383961	44.38%	5.613%
39	6.935	1738	1740	1744	rBV2	244	160	0.02%	0.002%
40	6.996	1753	1759	1763	rBV2	276	336	0.04%	0.005%
41	7.041	1769	1773	1777	rBV2	206	146	0.02%	0.002%
42	7.121	1795	1798	1801	rBV	200	145	0.02%	0.002%
43	7.189	1809	1819	1825	rBV6	1310	1905	0.22%	0.028%
44	7.237	1831	1834	1838	rBV2	244	152	0.02%	0.002%
45	7.420	1887	1891	1893	rVB2	246	162	0.02%	0.002%
46	7.436	1893	1896	1899	rBV2	241	162	0.02%	0.002%
47	7.562	1922	1935	1951	rBV	111830	196434	22.70%	2.872%
48	7.784	1999	2004	2006	rBB2	361	277	0.03%	0.004%
49	7.893	2025	2038	2072	rBV	409167	711408	82.22%	10.401%
50	8.067	2089	2092	2097	rVB2	369	284	0.03%	0.004%
51	8.121	2105	2109	2113	rBV	271	216	0.02%	0.003%
52	8.173	2113	2125	2141	rBV	77743	133474	15.43%	1.951%
53	8.298	2160	2164	2167	rVB2	326	239	0.03%	0.003%
54	8.404	2195	2197	2203	rBV	124	156	0.02%	0.002%
55	8.433	2203	2206	2210	rBV	218	211	0.02%	0.003%
56	8.510	2226	2230	2235	rBB2	187	151	0.02%	0.002%
57	8.626	2253	2266	2296	rBV2	200787	373727	43.19%	5.464%
58	8.777	2310	2313	2317	rVB3	432	278	0.03%	0.004%
59	8.857	2335	2338	2342	rBV	190	190	0.02%	0.003%
60	9.031	2389	2392	2394	rBV	276	182	0.02%	0.003%
61	9.240	2452	2457	2459	rBV	214	214	0.02%	0.003%
62	9.414	2498	2511	2531	rBV	408188	677615	78.32%	9.907%
63	9.661	2585	2588	2591	rBV2	286	231	0.03%	0.003%
64	9.684	2591	2595	2597	rBV2	319	245	0.03%	0.004%
65	9.732	2607	2610	2613	rBV2	302	189	0.02%	0.003%
66	9.774	2619	2623	2626	rBV	242	175	0.02%	0.003%
67	9.793	2627	2629	2634	rVV	269	231	0.03%	0.003%
68	9.857	2645	2649	2652	rVB	242	192	0.02%	0.003%
69	9.928	2668	2671	2677	rVB	361	256	0.03%	0.004%
70	10.044	2702	2707	2708	rBV	267	231	0.03%	0.003%
71	10.070	2713	2715	2720	rVB	298	185	0.02%	0.003%
72	10.144	2736	2738	2745	rBB2	255	252	0.03%	0.004%
73	10.311	2787	2790	2798	rBV2	264	353	0.04%	0.005%
74	10.411	2817	2821	2824	rBV2	264	250	0.03%	0.004%
75	10.446	2827	2832	2836	rVB2	333	312	0.04%	0.005%
76	10.475	2838	2841	2842	rBV2	430	234	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053610.D
 Acq On : 10 Apr 2023 11:16
 Operator : JC/MD
 Sample : 02251-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.533	2855	2859	2860	rBV2	257	153	0.02%	0.002%
78	10.636	2888	2891	2898	rBV3	915	908	0.10%	0.013%
79	10.751	2915	2927	2948	rBV	275632	441307	51.01%	6.452%
80	10.890	2964	2970	2974	rVV4	736	1018	0.12%	0.015%
81	10.919	2977	2979	2983	rVB2	257	187	0.02%	0.003%
82	11.015	3004	3009	3012	rBV	286	296	0.03%	0.004%
83	11.224	3071	3074	3079	rVB2	185	211	0.02%	0.003%
84	11.465	3145	3149	3152	rBV3	352	305	0.04%	0.004%
85	11.738	3229	3234	3238	rBV3	642	758	0.09%	0.011%
86	11.806	3243	3255	3273	rBV	434568	697866	80.66%	10.203%
87	12.070	3333	3337	3339	rBV3	385	326	0.04%	0.005%
88	12.189	3361	3374	3397	rBV	408352	670236	77.46%	9.799%
89	12.330	3415	3418	3421	rVB	363	235	0.03%	0.003%
90	12.468	3459	3461	3464	rVB	252	146	0.02%	0.002%
91	12.529	3478	3480	3483	rBV2	246	167	0.02%	0.002%
92	12.729	3539	3542	3544	rBV	248	167	0.02%	0.002%
93	12.835	3572	3575	3580	rBV2	213	183	0.02%	0.003%
94	12.986	3619	3622	3626	rBV2	296	298	0.03%	0.004%
95	13.356	3735	3737	3740	rBV	286	204	0.02%	0.003%
96	13.523	3786	3789	3794	rBV2	266	263	0.03%	0.004%
97	13.600	3810	3813	3817	rBV2	310	273	0.03%	0.004%
98	13.745	3855	3858	3860	rBV	362	225	0.03%	0.003%
99	13.812	3876	3879	3881	rBV	260	143	0.02%	0.002%
100	13.844	3881	3889	3899	rVV5	2962	4679	0.54%	0.068%




Sum of corrected areas: 6840046

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053610.D
Acq On : 10 Apr 2023 11:16
Operator : JC/MD
Sample : 02251-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

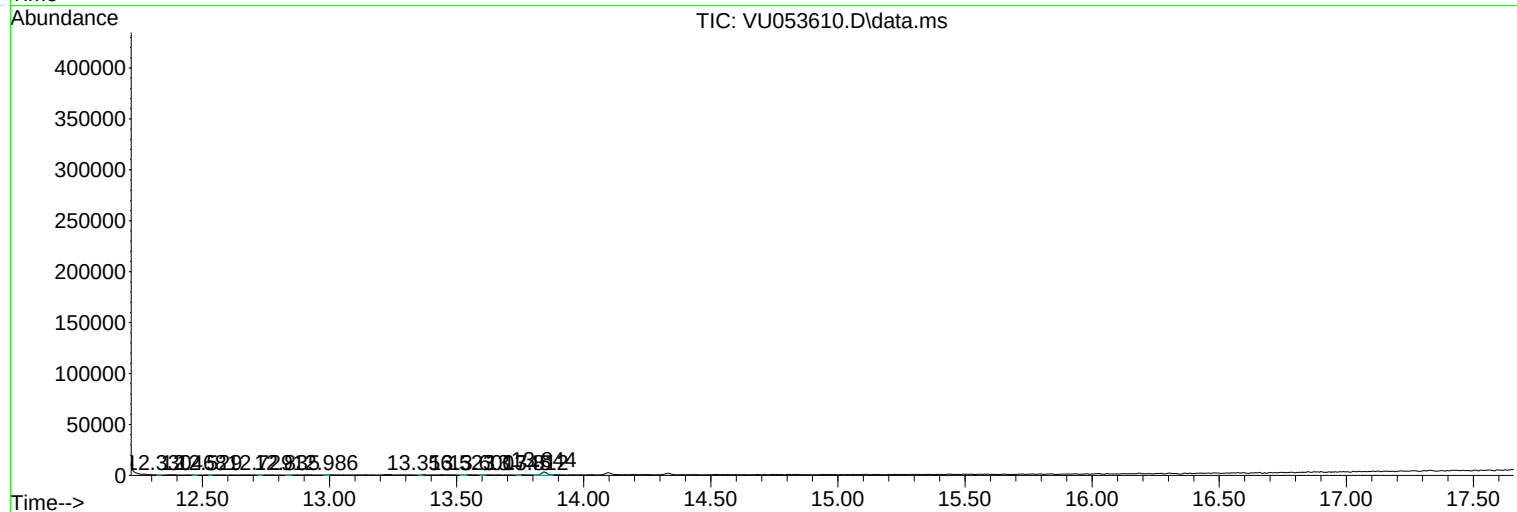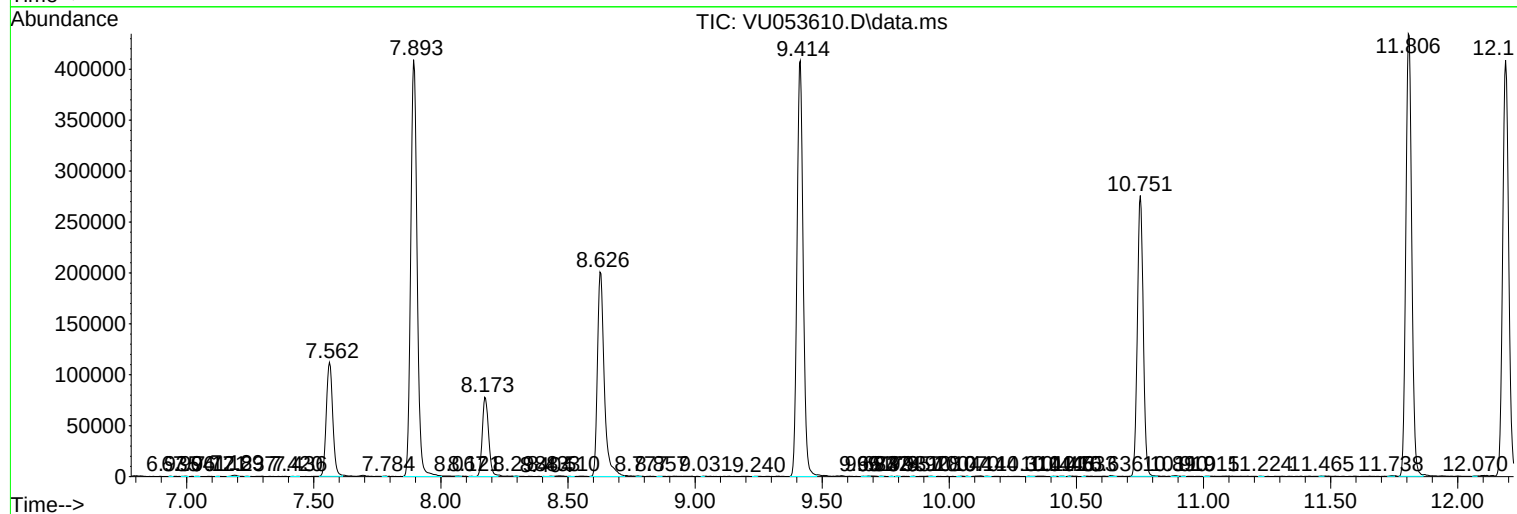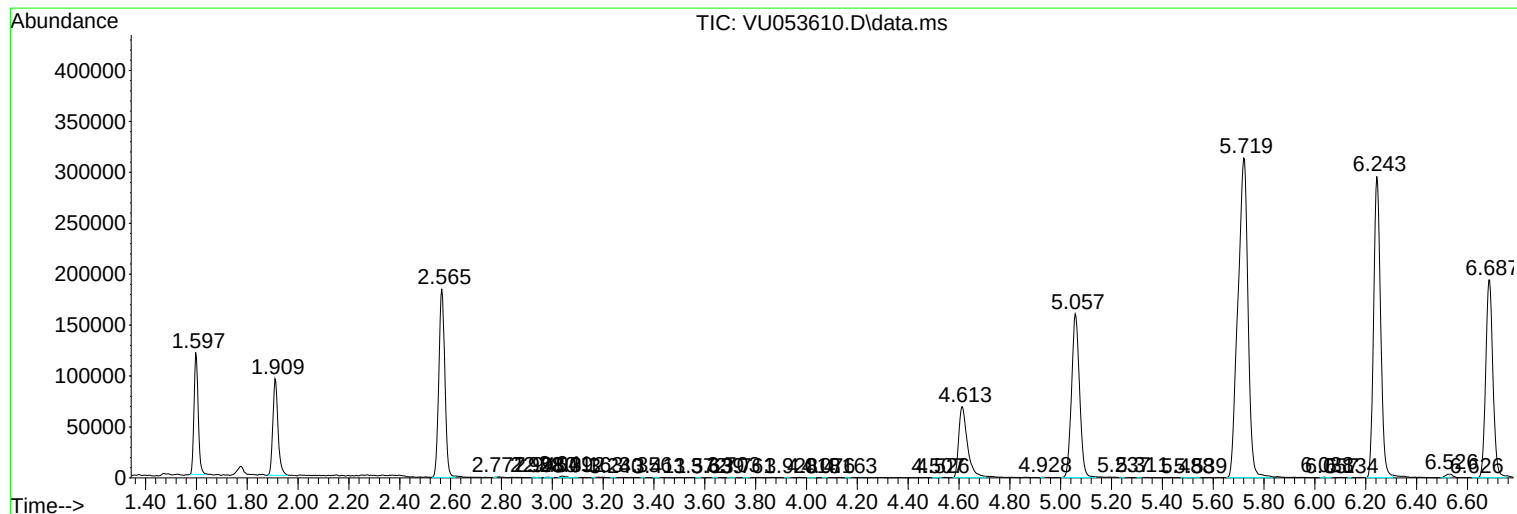

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053610.D
Acq On : 10 Apr 2023 11:16
Operator : JC/MD
Sample : 02251-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053610.D
Acq On : 10 Apr 2023 11:16
Operator : JC/MD
Sample : 02251-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------