

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053612.D
 Acq On : 10 Apr 2023 12:03
 Operator : JC/MD
 Sample : 02251-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	111417	132719	4.17%	0.853%
2	1.909	170	177	191	rVB	95596	128002	4.02%	0.823%
3	2.565	370	381	401	rVB	176929	288155	9.05%	1.853%
4	3.244	590	592	594	rVB2	688	219	0.01%	0.001%
5	3.282	601	604	608	rBV3	372	386	0.01%	0.002%
6	3.639	713	715	716	rBV3	327	164	0.01%	0.001%
7	3.883	789	791	793	rBV	181	105	0.00%	0.001%
8	3.919	800	802	807	rVB2	216	187	0.01%	0.001%
9	3.944	807	810	814	rBV	415	324	0.01%	0.002%
10	4.009	827	830	833	rBV	291	216	0.01%	0.001%
11	4.063	842	847	850	rBV2	282	267	0.01%	0.002%
12	4.398	947	951	954	rBV2	235	203	0.01%	0.001%
13	4.491	977	980	983	rBV2	316	171	0.01%	0.001%
14	4.613	1006	1018	1049	rBV	67690	164597	5.17%	1.058%
15	4.784	1068	1071	1073	rBV2	619	432	0.01%	0.003%
16	4.938	1117	1119	1124	rVB2	279	192	0.01%	0.001%
17	5.057	1140	1156	1176	rBV	158873	357804	11.23%	2.301%
18	5.285	1224	1227	1232	rBV3	452	439	0.01%	0.003%
19	5.378	1254	1256	1258	rBV	305	170	0.01%	0.001%
20	5.398	1259	1262	1264	rBV2	427	260	0.01%	0.002%
21	5.469	1281	1284	1286	rBV	156	111	0.00%	0.001%
22	5.597	1321	1324	1325	rBV	211	98	0.00%	0.001%
23	5.629	1330	1334	1338	rVB2	344	279	0.01%	0.002%
24	5.719	1341	1362	1370	rBV2	310249	839026	26.34%	5.395%
25	6.038	1456	1461	1464	rBV3	621	623	0.02%	0.004%
26	6.086	1474	1476	1480	rVB2	240	169	0.01%	0.001%
27	6.186	1505	1507	1511	rBV2	345	213	0.01%	0.001%
28	6.243	1511	1525	1548	rBV	277615	527237	16.55%	3.390%
29	6.436	1583	1585	1588	rBV2	346	192	0.01%	0.001%
30	6.456	1588	1591	1593	rBV2	256	164	0.01%	0.001%
31	6.523	1602	1612	1623	rBV6	4264	7876	0.25%	0.051%
32	6.607	1636	1638	1639	rBV6	225	92	0.00%	0.001%
33	6.632	1643	1646	1648	rBB	242	118	0.00%	0.001%
34	6.687	1648	1663	1679	rBV	190431	374856	11.77%	2.410%
35	6.903	1727	1730	1731	rBV	221	119	0.00%	0.001%
36	6.941	1740	1742	1745	rVB	368	188	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053612.D
 Acq On : 10 Apr 2023 12:03
 Operator : JC/MD
 Sample : 02251-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.970	1745	1751	1755	rBV2	304	311	0.01%	0.002%
38	7.022	1764	1767	1772	rVB2	377	295	0.01%	0.002%
39	7.047	1772	1775	1777	rBV	199	130	0.00%	0.001%
40	7.247	1835	1837	1841	rBV	169	101	0.00%	0.001%
41	7.288	1847	1850	1852	rBV	188	110	0.00%	0.001%
42	7.353	1866	1870	1873	rBV2	213	172	0.01%	0.001%
43	7.407	1885	1887	1895	rVB	328	263	0.01%	0.002%
44	7.562	1922	1935	1957	rBV	110987	199894	6.28%	1.285%
45	7.800	2006	2009	2010	rBV	235	128	0.00%	0.001%
46	7.825	2013	2017	2019	rBV2	180	124	0.00%	0.001%
47	7.838	2019	2021	2025	rBV2	245	145	0.00%	0.001%
48	7.893	2025	2038	2063	rBV	402267	703840	22.10%	4.525%
49	8.108	2103	2105	2107	rBV	335	157	0.00%	0.001%
50	8.176	2113	2126	2145	rBV	81242	135720	4.26%	0.873%
51	8.292	2160	2162	2167	rVB	313	149	0.00%	0.001%
52	8.324	2170	2172	2175	rVV2	369	159	0.00%	0.001%
53	8.340	2175	2177	2183	rVB	441	308	0.01%	0.002%
54	8.372	2184	2187	2195	rVB	242	166	0.01%	0.001%
55	8.472	2212	2218	2227	rVB4	783	1079	0.03%	0.007%
56	8.626	2255	2266	2301	rBV	200532	374315	11.75%	2.407%
57	8.960	2368	2370	2375	rBV2	408	305	0.01%	0.002%
58	8.986	2375	2378	2383	rBV	304	321	0.01%	0.002%
59	9.105	2412	2415	2418	rBV2	214	178	0.01%	0.001%
60	9.176	2435	2437	2442	rBV2	171	120	0.00%	0.001%
61	9.256	2459	2462	2464	rBV	244	167	0.01%	0.001%
62	9.330	2483	2485	2488	rBV	188	111	0.00%	0.001%
63	9.443	2497	2520	2555	rBV2	1061484	2417562	75.90%	15.544%
64	9.816	2633	2636	2638	rBV	199	135	0.00%	0.001%
65	9.893	2658	2660	2664	rVB	359	197	0.01%	0.001%
66	9.915	2664	2667	2672	rBV3	199	240	0.01%	0.002%
67	9.964	2680	2682	2685	rVB2	270	161	0.01%	0.001%
68	9.983	2686	2688	2690	rBV2	220	132	0.00%	0.001%
69	10.028	2700	2702	2707	rVB2	395	202	0.01%	0.001%
70	10.089	2718	2721	2722	rBV	348	189	0.01%	0.001%
71	10.173	2743	2747	2751	rVB2	257	225	0.01%	0.001%
72	10.295	2782	2785	2786	rBV2	203	101	0.00%	0.001%
73	10.549	2861	2864	2866	rBV	240	125	0.00%	0.001%
74	10.562	2866	2868	2870	rVV	297	119	0.00%	0.001%
75	10.632	2887	2890	2896	rBV2	973	895	0.03%	0.006%
76	10.690	2905	2908	2910	rBV2	254	172	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053612.D
 Acq On : 10 Apr 2023 12:03
 Operator : JC/MD
 Sample : 02251-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0MC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.751	2915	2927	2949	rVB	261250	430637	13.52%	2.769%
78	10.886	2964	2969	2973	rBV4	664	880	0.03%	0.006%
79	11.176	3056	3059	3064	rBV2	241	232	0.01%	0.001%
80	11.465	3146	3149	3157	rBV4	590	758	0.02%	0.005%
81	11.558	3176	3178	3182	rBV	404	278	0.01%	0.002%
82	11.652	3202	3207	3211	rBV3	471	594	0.02%	0.004%
83	11.742	3223	3235	3245	rBV	300265	472708	14.84%	3.039%
84	11.832	3246	3263	3289	rVB2	1639880	3185048	100.00%	20.479%
85	12.208	3362	3380	3397	rBV2	1542646	3022903	94.91%	19.436%
86	12.484	3462	3466	3472	rBV4	662	891	0.03%	0.006%
87	12.642	3513	3515	3518	rBV2	387	237	0.01%	0.002%
88	12.684	3522	3528	3529	rBV3	491	440	0.01%	0.003%
89	12.770	3553	3555	3556	rBV3	289	149	0.00%	0.001%
90	13.201	3679	3689	3704	rBV2	29677	51903	1.63%	0.334%
91	13.324	3720	3727	3736	rBV6	2230	2965	0.09%	0.019%
92	13.388	3746	3747	3752	rVB2	318	173	0.01%	0.001%
93	13.558	3796	3800	3803	rBV	367	319	0.01%	0.002%
94	13.632	3819	3823	3826	rBV	554	400	0.01%	0.003%
95	13.742	3854	3857	3862	rBV2	421	349	0.01%	0.002%
96	13.835	3874	3886	3904	rBV	690012	1099934	34.53%	7.072%
97	14.282	4023	4025	4026	rBV	718	329	0.01%	0.002%
98	14.323	4027	4038	4057	rVB	312721	507236	15.93%	3.261%
99	14.725	4154	4163	4177	rBV3	15127	27002	0.85%	0.174%
100	15.992	4549	4557	4569	rVB3	49787	80954	2.54%	0.521%




Sum of corrected areas: 15552915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053612.D
Acq On : 10 Apr 2023 12:03
Operator : JC/MD
Sample : 02251-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

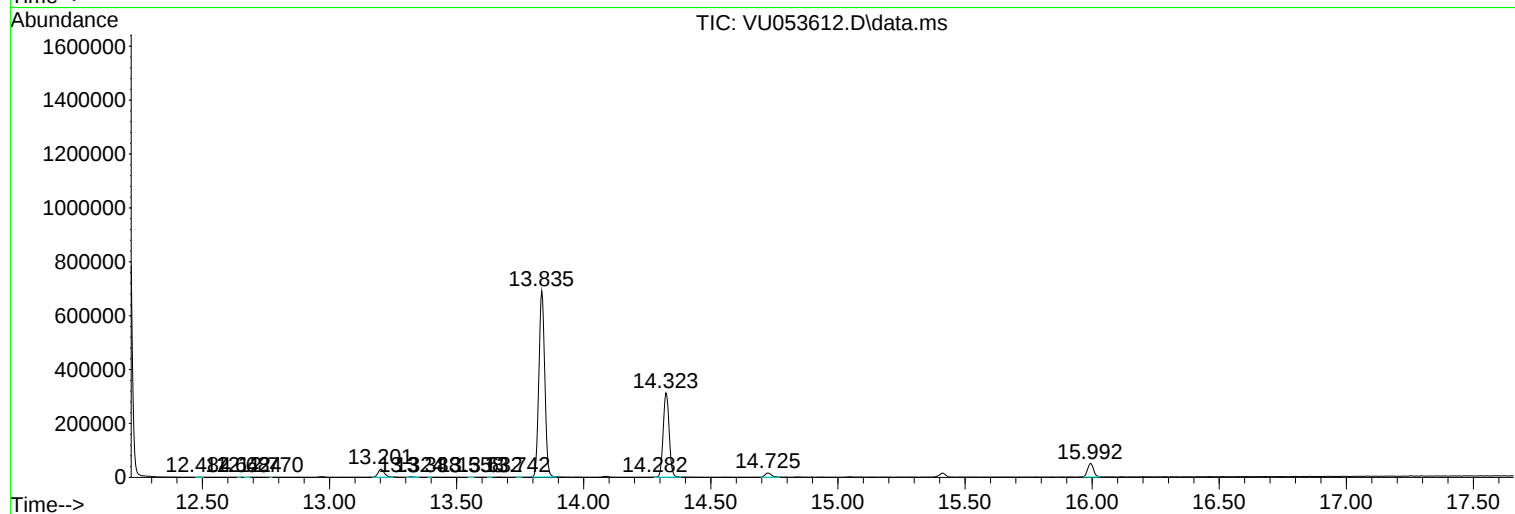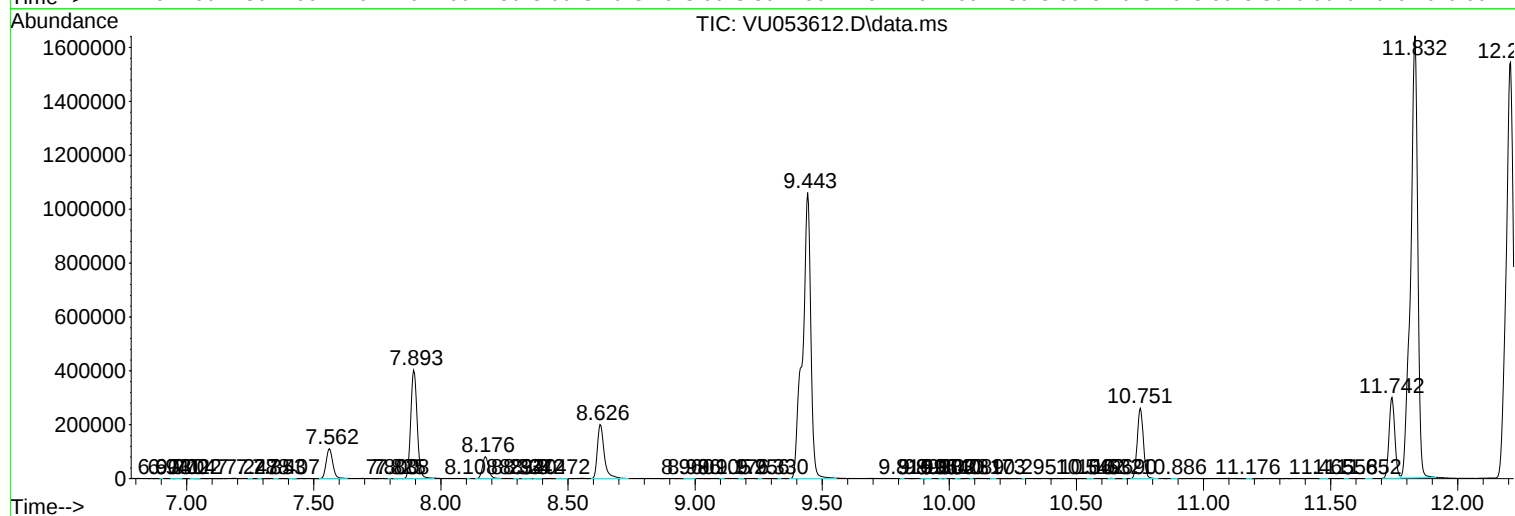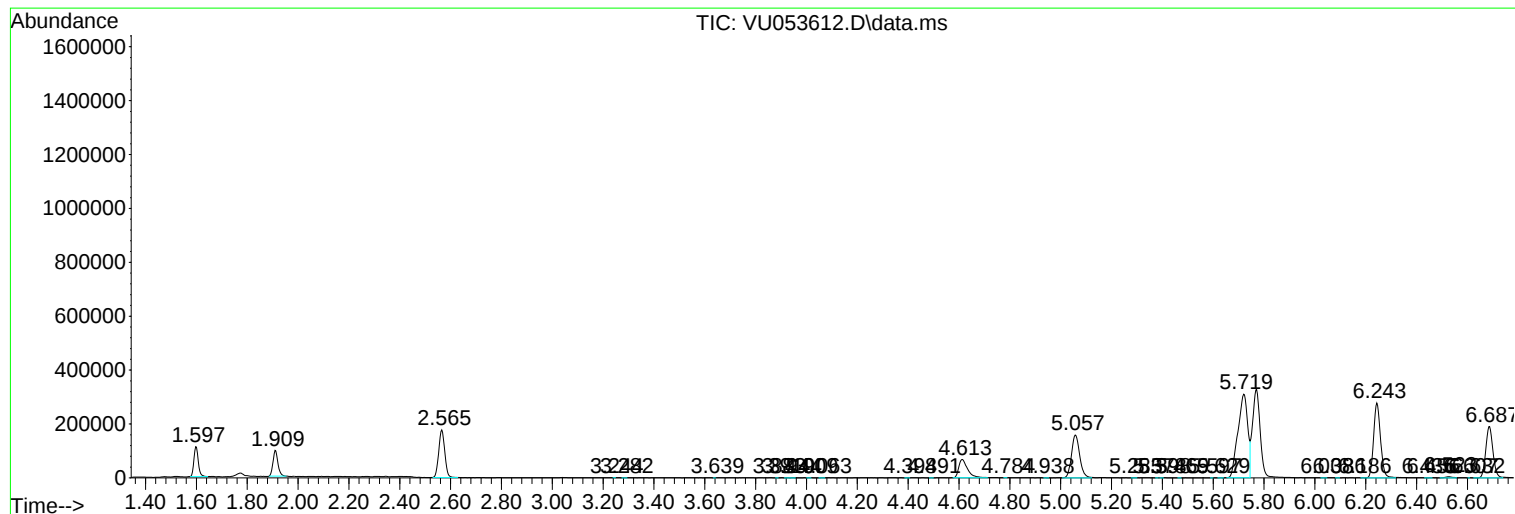

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053612.D
Acq On : 10 Apr 2023 12:03
Operator : JC/MD
Sample : 02251-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053612.D
Acq On : 10 Apr 2023 12:03
Operator : JC/MD
Sample : 02251-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------