

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053615.D
 Acq On : 10 Apr 2023 15:15
 Operator : JC/MD
 Sample : 02251-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	118203	134230	0.31%	0.130%
2	1.909	170	177	193	rVB	94250	132352	0.31%	0.128%
3	2.562	369	380	395	rBV	184302	300265	0.70%	0.291%
4	2.748	428	438	452	rVV2	13464	25134	0.06%	0.024%
5	2.870	473	476	479	rBV3	392	317	0.00%	0.000%
6	2.967	504	506	508	rBV	300	152	0.00%	0.000%
7	3.022	517	523	524	rBV	257	226	0.00%	0.000%
8	3.038	524	528	531	rVV3	804	723	0.00%	0.001%
9	3.134	551	558	563	rBV3	729	943	0.00%	0.001%
10	3.179	567	572	573	rBV2	662	519	0.00%	0.001%
11	3.584	692	698	701	rBV2	320	310	0.00%	0.000%
12	3.652	714	719	720	rBV	205	168	0.00%	0.000%
13	3.694	729	732	734	rVB3	323	172	0.00%	0.000%
14	3.745	745	748	751	rBV2	325	199	0.00%	0.000%
15	3.793	760	763	764	rBV	245	141	0.00%	0.000%
16	3.832	773	775	778	rBV2	302	182	0.00%	0.000%
17	3.993	823	825	828	rBV	211	141	0.00%	0.000%
18	4.012	829	831	836	rVB	338	173	0.00%	0.000%
19	4.038	836	839	843	rBV2	335	251	0.00%	0.000%
20	4.060	843	846	852	rVB2	332	318	0.00%	0.000%
21	4.086	852	854	858	rBV2	284	170	0.00%	0.000%
22	4.150	869	874	877	rBV	324	235	0.00%	0.000%
23	4.356	935	938	940	rBV	276	143	0.00%	0.000%
24	4.369	940	942	945	rVV	324	169	0.00%	0.000%
25	4.401	949	952	955	rBV2	251	167	0.00%	0.000%
26	4.462	968	971	978	rVB2	208	216	0.00%	0.000%
27	4.533	978	993	1002	rVB8	2107	4539	0.01%	0.004%
28	4.613	1006	1018	1045	rBV	74244	182462	0.42%	0.177%
29	4.986	1130	1134	1137	rVB3	202	152	0.00%	0.000%
30	5.057	1140	1156	1177	rBV	165314	363096	0.84%	0.351%
31	5.288	1225	1228	1229	rBV	220	158	0.00%	0.000%
32	5.382	1247	1257	1258	rBV3	1414	1481	0.00%	0.001%
33	5.523	1298	1301	1304	rVB2	237	162	0.00%	0.000%
34	5.600	1321	1325	1329	rVB2	211	220	0.00%	0.000%
35	5.626	1329	1333	1335	rBV2	191	171	0.00%	0.000%
36	5.774	1341	1379	1438	rBV2	18889518	38568711	89.36%	37.333%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053615.D
 Acq On : 10 Apr 2023 15:15
 Operator : JC/MD
 Sample : 02251-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.243	1513	1525	1548	rVB	311578	585002	1.36%	0.566%
38	6.526	1606	1613	1614	rBV5	3075	2864	0.01%	0.003%
39	6.594	1631	1634	1636	rBV3	360	276	0.00%	0.000%
40	6.684	1649	1662	1681	rBV2	202296	392313	0.91%	0.380%
41	6.867	1713	1719	1724	rBV2	282	359	0.00%	0.000%
42	6.941	1739	1742	1746	rVB	424	295	0.00%	0.000%
43	7.028	1766	1769	1772	rBV2	309	167	0.00%	0.000%
44	7.102	1788	1792	1795	rVV2	346	255	0.00%	0.000%
45	7.185	1812	1818	1825	rBV6	980	1442	0.00%	0.001%
46	7.237	1831	1834	1835	rBV	241	162	0.00%	0.000%
47	7.562	1923	1935	1960	rBV	116350	204278	0.47%	0.198%
48	7.700	1975	1978	1982	rVB2	749	517	0.00%	0.001%
49	7.745	1987	1992	1996	rBV	273	355	0.00%	0.000%
50	7.796	2005	2008	2009	rBV2	281	143	0.00%	0.000%
51	7.835	2017	2020	2024	rBV	343	304	0.00%	0.000%
52	7.893	2024	2038	2056	rBV	432650	740453	1.72%	0.717%
53	8.089	2097	2099	2102	rVB2	366	235	0.00%	0.000%
54	8.172	2114	2125	2143	rBV	81983	137166	0.32%	0.133%
55	8.356	2179	2182	2184	rBV	262	190	0.00%	0.000%
56	8.401	2192	2196	2200	rBV2	239	207	0.00%	0.000%
57	8.443	2203	2209	2211	rBV2	305	251	0.00%	0.000%
58	8.552	2235	2243	2250	rVB6	1747	2260	0.01%	0.002%
59	8.626	2254	2266	2294	rBV	224724	404194	0.94%	0.391%
60	8.857	2336	2338	2341	rVB	268	157	0.00%	0.000%
61	8.980	2372	2376	2379	rBV2	350	302	0.00%	0.000%
62	9.028	2388	2391	2396	rBV2	280	154	0.00%	0.000%
63	9.179	2435	2438	2440	rBV	235	152	0.00%	0.000%
64	9.311	2475	2479	2481	rBV2	267	175	0.00%	0.000%
65	9.446	2499	2521	2564	rBV	26495337	43159253	100.00%	41.776%
66	10.034	2701	2704	2707	rBV2	365	315	0.00%	0.000%
67	10.240	2764	2768	2770	rBV2	403	254	0.00%	0.000%
68	10.343	2796	2800	2801	rBV2	459	326	0.00%	0.000%
69	10.388	2809	2814	2817	rBV	342	184	0.00%	0.000%
70	10.414	2817	2822	2824	rBV2	399	317	0.00%	0.000%
71	10.484	2838	2844	2846	rVV3	496	499	0.00%	0.000%
72	10.597	2875	2879	2882	rBV	295	219	0.00%	0.000%
73	10.668	2897	2901	2904	rBV3	384	322	0.00%	0.000%
74	10.751	2914	2927	2952	rVB	290498	468116	1.08%	0.453%
75	10.860	2957	2961	2964	rBV	401	306	0.00%	0.000%
76	10.883	2964	2968	2969	rBV2	522	373	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053615.D
 Acq On : 10 Apr 2023 15:15
 Operator : JC/MD
 Sample : 02251-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.979	2995	2998	3003	rBV2	1046	912	0.00%	0.001%
78	11.098	3029	3035	3046	rBV4	934	1648	0.00%	0.002%
79	11.160	3052	3054	3056	rBV	313	162	0.00%	0.000%
80	11.246	3078	3081	3084	rBV	279	159	0.00%	0.000%
81	11.465	3146	3149	3152	rBV	576	418	0.00%	0.000%
82	11.539	3168	3172	3175	rBV	382	306	0.00%	0.000%
83	11.600	3186	3191	3193	rBV	237	183	0.00%	0.000%
84	11.632	3196	3201	3202	rBV	210	174	0.00%	0.000%
85	11.677	3214	3215	3218	rBV2	380	174	0.00%	0.000%
86	11.741	3218	3235	3245	rBV	194947	321913	0.75%	0.312%
87	11.831	3245	3263	3285	rVV	5607806	9256123	21.45%	8.959%
88	12.208	3362	3380	3418	rBV2	4520029	7692361	17.82%	7.446%
89	12.635	3510	3513	3514	rBV2	353	186	0.00%	0.000%
90	12.664	3518	3522	3525	rBV3	458	413	0.00%	0.000%
91	13.221	3691	3695	3701	rVB4	666	703	0.00%	0.001%
92	13.278	3710	3713	3716	rVB	321	160	0.00%	0.000%
93	13.304	3718	3721	3722	rBV	300	155	0.00%	0.000%
94	13.671	3832	3835	3837	rBV	237	168	0.00%	0.000%
95	13.696	3837	3843	3845	rBV2	503	509	0.00%	0.000%
96	13.764	3860	3864	3869	rBV2	620	623	0.00%	0.001%
97	13.790	3869	3872	3875	rVV2	306	250	0.00%	0.000%
98	13.835	3875	3886	3909	rVV	122317	198091	0.46%	0.192%
99	14.220	4003	4006	4009	rBV	398	327	0.00%	0.000%
100	14.327	4031	4039	4050	rVB5	6480	10357	0.02%	0.010%




Sum of corrected areas: 103310755

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053615.D
Acq On : 10 Apr 2023 15:15
Operator : JC/MD
Sample : 02251-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

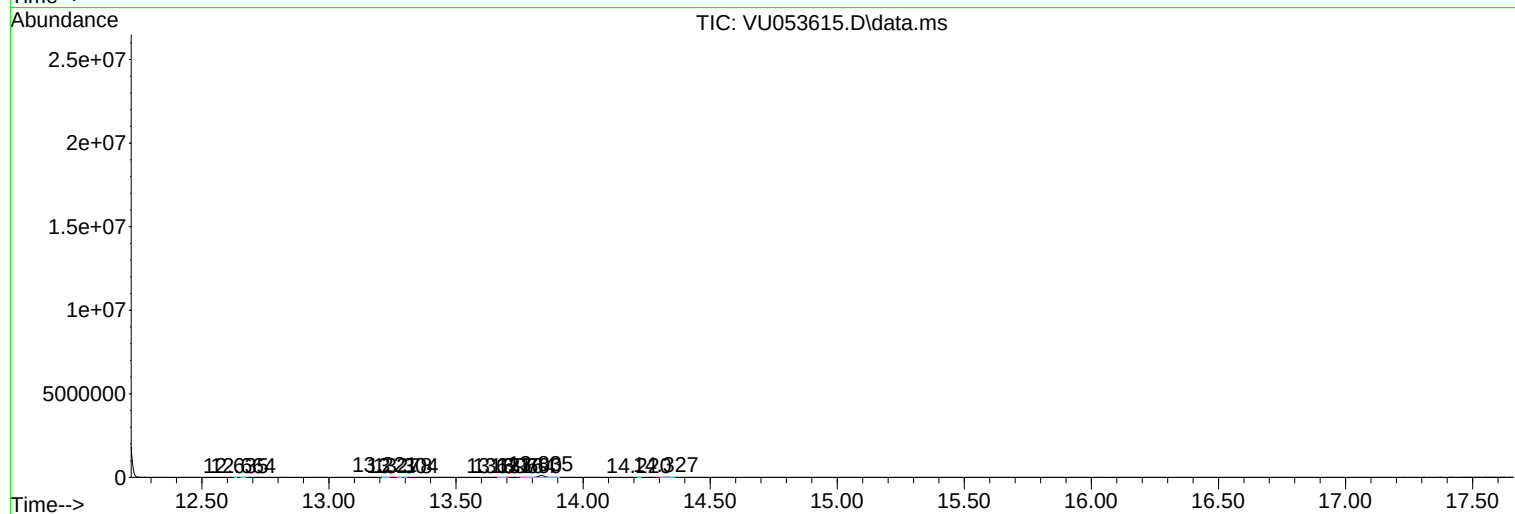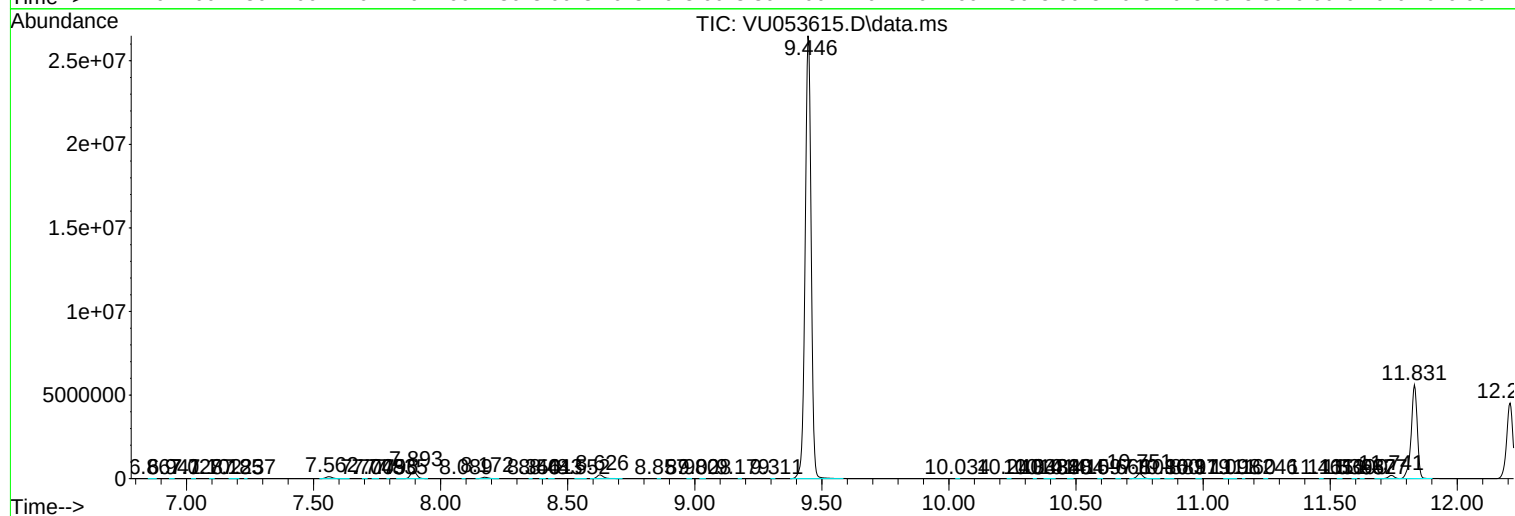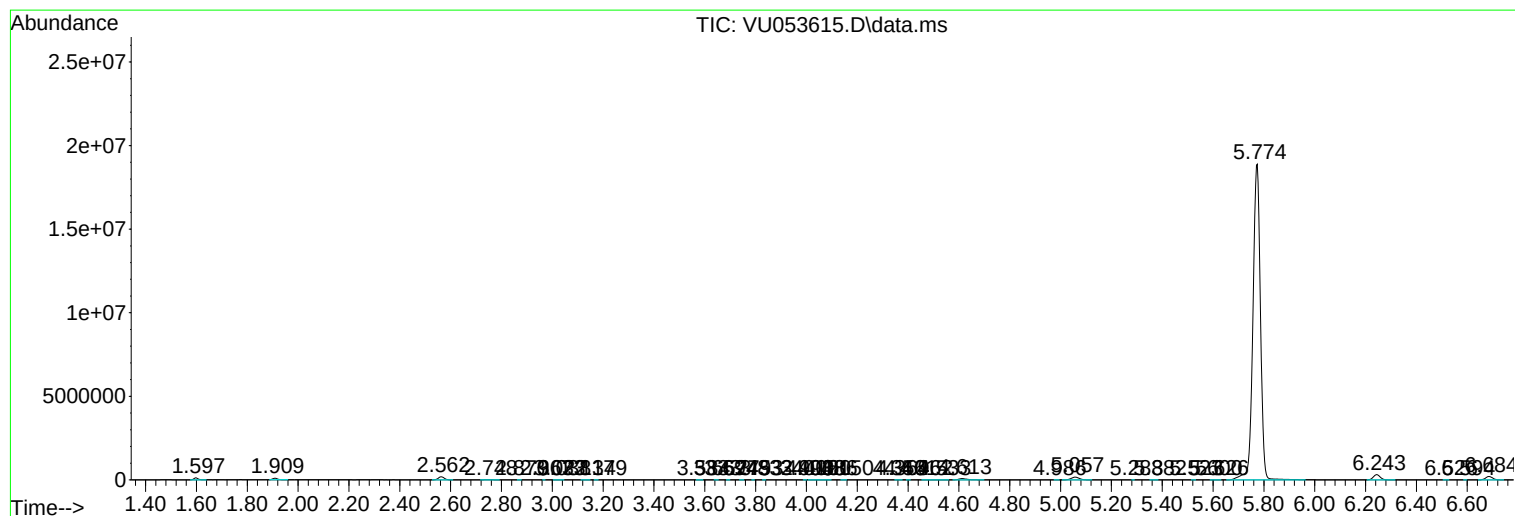

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053615.D
Acq On : 10 Apr 2023 15:15
Operator : JC/MD
Sample : 02251-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053615.D
Acq On : 10 Apr 2023 15:15
Operator : JC/MD
Sample : 02251-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------