

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053619.D
 Acq On : 10 Apr 2023 17:37
 Operator : JC/MD
 Sample : VIBLK124
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	110624	128984	15.65%	1.888%
2	1.909	170	177	191	rVB	92504	123340	14.97%	1.806%
3	2.565	369	381	396	rBV	170639	279840	33.96%	4.097%
4	3.041	518	529	544	rBV2	12558	24425	2.96%	0.358%
5	3.160	564	566	567	rBV2	189	86	0.01%	0.001%
6	3.424	646	648	649	rBV2	227	81	0.01%	0.001%
7	3.530	679	681	683	rBV2	234	134	0.02%	0.002%
8	3.896	792	795	799	rBV2	286	224	0.03%	0.003%
9	4.025	834	835	836	rBV	158	47	0.01%	0.001%
10	4.169	876	880	881	rBV2	245	168	0.02%	0.002%
11	4.263	903	909	911	rBV2	282	290	0.04%	0.004%
12	4.330	928	930	933	rBV2	180	113	0.01%	0.002%
13	4.616	1007	1019	1046	rBV	68121	166190	20.17%	2.433%
14	5.060	1140	1157	1175	rBV	152512	333822	40.51%	4.887%
15	5.250	1214	1216	1218	rBV2	359	158	0.02%	0.002%
16	5.507	1295	1296	1297	rBV2	130	41	0.00%	0.001%
17	5.575	1313	1317	1323	rBV	321	426	0.05%	0.006%
18	5.623	1330	1332	1333	rBV	158	66	0.01%	0.001%
19	5.719	1341	1362	1376	rBV2	299984	824123	100.00%	12.065%
20	5.954	1432	1435	1437	rBV	257	200	0.02%	0.003%
21	6.112	1481	1484	1485	rBV	175	80	0.01%	0.001%
22	6.121	1485	1487	1489	rVB	167	52	0.01%	0.001%
23	6.131	1489	1490	1491	rBV	191	54	0.01%	0.001%
24	6.243	1512	1525	1549	rBV	300115	569197	69.07%	8.333%
25	6.520	1604	1611	1612	rBV2	2634	1979	0.24%	0.029%
26	6.687	1648	1663	1692	rBV	187996	370959	45.01%	5.431%
27	6.861	1715	1717	1720	rBV	256	154	0.02%	0.002%
28	6.944	1740	1743	1744	rBV	245	135	0.02%	0.002%
29	7.009	1758	1763	1766	rVB2	328	313	0.04%	0.005%
30	7.108	1792	1794	1796	rBV	175	72	0.01%	0.001%
31	7.182	1806	1817	1827	rBV4	1270	2377	0.29%	0.035%
32	7.317	1858	1859	1860	rBV4	133	38	0.00%	0.001%
33	7.353	1866	1870	1873	rBV	233	251	0.03%	0.004%
34	7.462	1902	1904	1907	rVB	185	56	0.01%	0.001%
35	7.562	1922	1935	1959	rBV	101877	183674	22.29%	2.689%
36	7.664	1965	1967	1970	rVB	522	251	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053619.D
 Acq On : 10 Apr 2023 17:37
 Operator : JC/MD
 Sample : VIBLK124
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.690	1970	1975	1982	rBV5	727	1119	0.14%	0.016%
38	7.841	2021	2022	2023	rBV	150	32	0.00%	0.000%
39	7.893	2024	2038	2062	rBV	381699	667888	81.04%	9.778%
40	8.092	2098	2100	2103	rBV2	188	108	0.01%	0.002%
41	8.176	2115	2126	2147	rBV	71914	123843	15.03%	1.813%
42	8.336	2174	2176	2179	rVB	192	84	0.01%	0.001%
43	8.433	2204	2206	2209	rBV	175	92	0.01%	0.001%
44	8.452	2210	2212	2216	rVV2	299	169	0.02%	0.002%
45	8.500	2224	2227	2230	rBV	350	287	0.03%	0.004%
46	8.552	2241	2243	2248	rVB	253	132	0.02%	0.002%
47	8.629	2255	2267	2292	rBV	203385	368280	44.69%	5.391%
48	8.809	2321	2323	2325	rVB	201	62	0.01%	0.001%
49	8.825	2325	2328	2330	rBV	393	245	0.03%	0.004%
50	8.877	2341	2344	2346	rBV	213	97	0.01%	0.001%
51	8.954	2365	2368	2370	rBV2	388	208	0.03%	0.003%
52	9.343	2487	2489	2493	rBV2	192	126	0.02%	0.002%
53	9.414	2498	2511	2534	rBV2	404361	775810	94.14%	11.358%
54	9.600	2566	2569	2572	rVB	308	168	0.02%	0.002%
55	9.632	2576	2579	2580	rBV	195	95	0.01%	0.001%
56	9.742	2611	2613	2616	rVB	445	187	0.02%	0.003%
57	9.761	2616	2619	2621	rBV	192	121	0.01%	0.002%
58	9.938	2670	2674	2679	rBV2	303	330	0.04%	0.005%
59	9.973	2683	2685	2692	rBV	209	242	0.03%	0.004%
60	10.105	2722	2726	2731	rBV2	418	446	0.05%	0.007%
61	10.205	2755	2757	2759	rBV	190	84	0.01%	0.001%
62	10.288	2778	2783	2785	rBV2	241	224	0.03%	0.003%
63	10.343	2795	2800	2805	rBV2	245	334	0.04%	0.005%
64	10.436	2827	2829	2830	rBV2	197	75	0.01%	0.001%
65	10.478	2840	2842	2843	rBV	228	69	0.01%	0.001%
66	10.658	2896	2898	2899	rBV	210	68	0.01%	0.001%
67	10.751	2915	2927	2949	rBV	271884	435657	52.86%	6.378%
68	10.861	2959	2961	2964	rBV	198	93	0.01%	0.001%
69	11.015	3007	3009	3011	rVB	194	78	0.01%	0.001%
70	11.188	3060	3063	3066	rBV2	339	205	0.02%	0.003%
71	11.410	3130	3132	3135	rBV	279	111	0.01%	0.002%
72	11.745	3229	3236	3244	rBV4	3955	6358	0.77%	0.093%
73	11.809	3244	3256	3280	rBV	436970	759126	92.11%	11.113%
74	12.012	3317	3319	3321	rBV	331	137	0.02%	0.002%
75	12.147	3359	3361	3362	rBV	262	121	0.01%	0.002%
76	12.188	3362	3374	3398	rVV	388906	662594	80.40%	9.700%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053619.D
Acq On : 10 Apr 2023 17:37
Operator : JC/MD
Sample : VIBLK124
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

77	12.356	3423	3426	3429	rBV	581	377	0.05%	0.006%
78	13.487	3776	3778	3783	rBV3	437	382	0.05%	0.006%
79	13.841	3882	3888	3900	rVB4	7161	10978	1.33%	0.161%
80	14.082	3960	3963	3967	rBV3	434	400	0.05%	0.006%
81	14.388	4056	4058	4060	rVB	355	134	0.02%	0.002%
82	14.565	4110	4113	4119	rBV3	543	637	0.08%	0.009%




Sum of corrected areas: 6830813

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053619.D
Acq On : 10 Apr 2023 17:37
Operator : JC/MD
Sample : VIBLK124
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

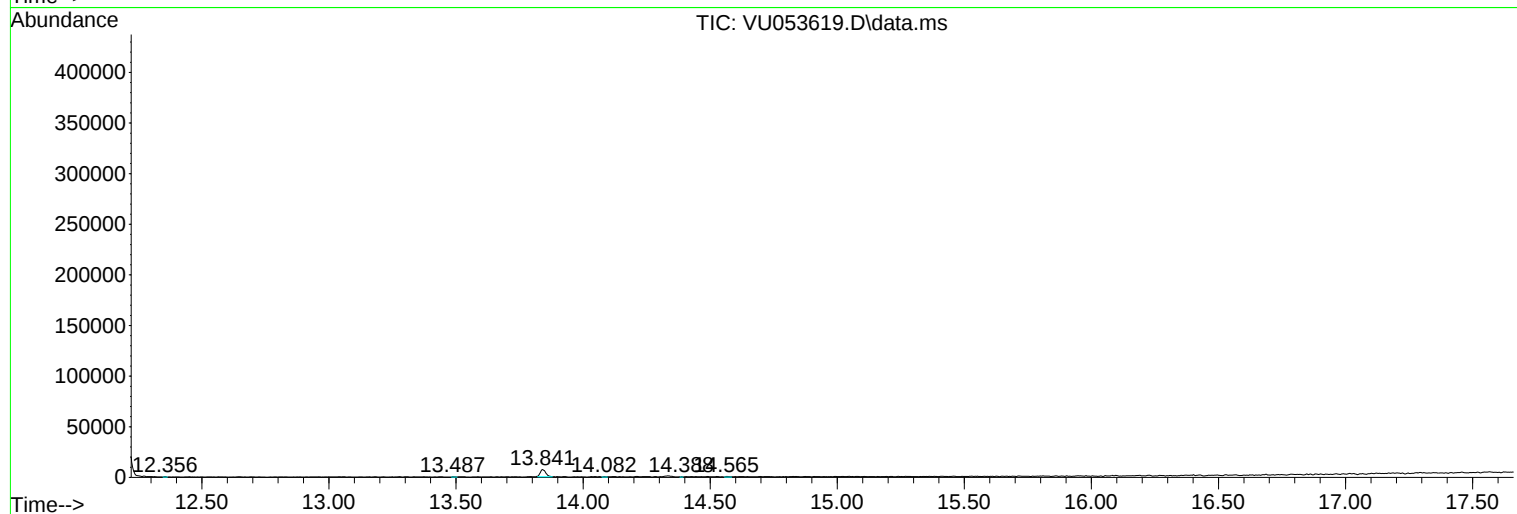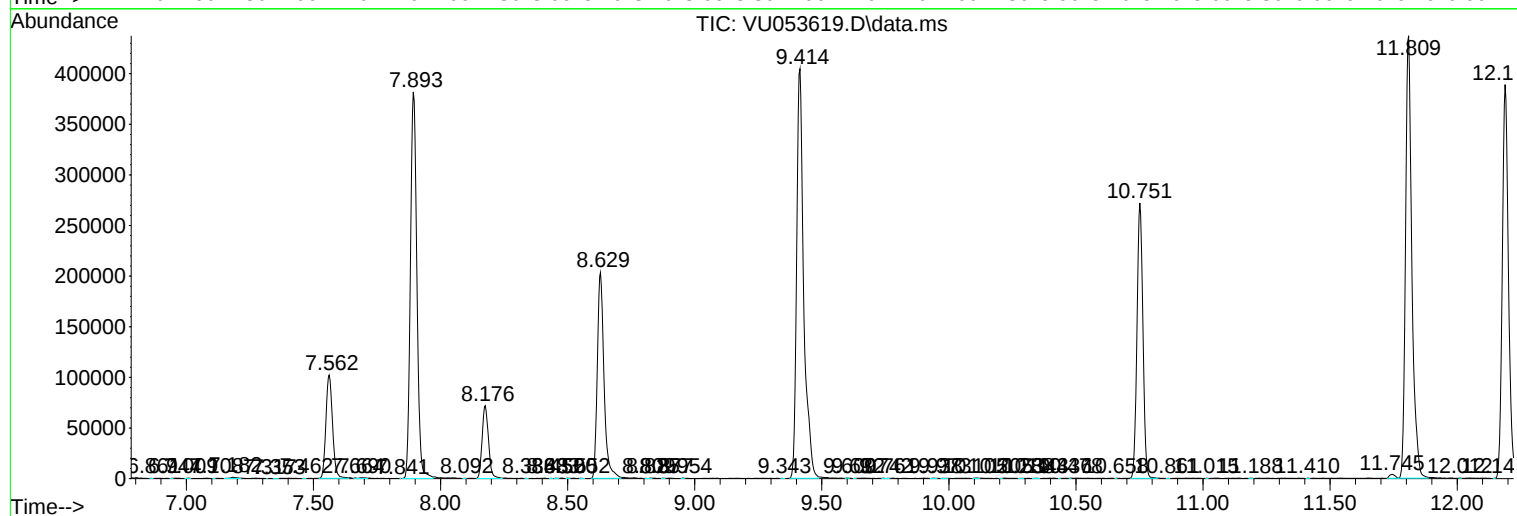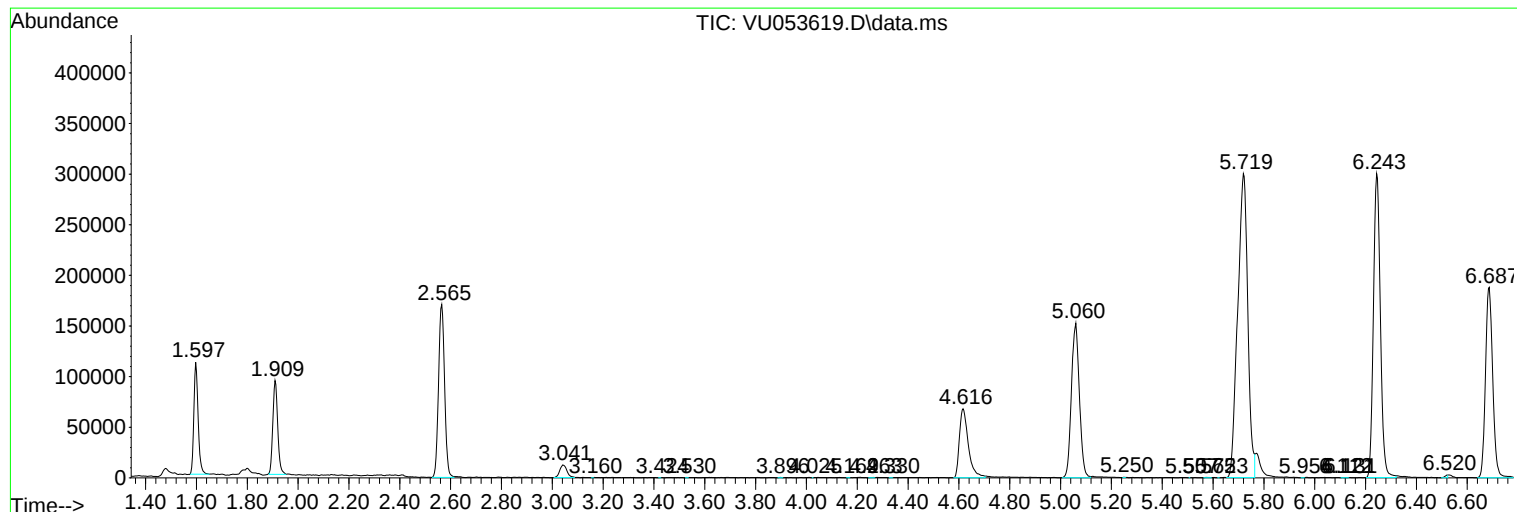

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053619.D
Acq On : 10 Apr 2023 17:37
Operator : JC/MD
Sample : VIBLK124
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053619.D
Acq On : 10 Apr 2023 17:37
Operator : JC/MD
Sample : VIBLK124
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------