

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053620.D
 Acq On : 10 Apr 2023 18:01
 Operator : JC/MD
 Sample : 02251-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	36	42	53	rBV2	8462	15663	1.72%	0.224%
2	1.597	73	80	97	rVB	101773	118533	13.01%	1.692%
3	1.909	170	177	193	rVB	87513	115932	12.73%	1.655%
4	2.565	369	381	397	rBV	161083	258704	28.40%	3.693%
5	3.121	551	554	559	rBV	262	243	0.03%	0.003%
6	3.453	655	657	661	rVB	197	87	0.01%	0.001%
7	3.617	705	708	710	rBV2	256	161	0.02%	0.002%
8	4.276	908	913	914	rBV	216	191	0.02%	0.003%
9	4.314	922	925	928	rBV2	198	175	0.02%	0.002%
10	4.427	956	960	963	rBV2	297	305	0.03%	0.004%
11	4.462	968	971	973	rBV	177	89	0.01%	0.001%
12	4.481	973	977	982	rVB	294	207	0.02%	0.003%
13	4.504	982	984	988	rBV	157	99	0.01%	0.001%
14	4.617	1007	1019	1044	rBV	65277	156504	17.18%	2.234%
15	4.903	1106	1108	1110	rBV	227	102	0.01%	0.001%
16	4.935	1115	1118	1122	rBV2	366	260	0.03%	0.004%
17	4.977	1129	1131	1135	rVB2	299	211	0.02%	0.003%
18	5.002	1137	1139	1141	rBV2	269	100	0.01%	0.001%
19	5.057	1141	1156	1179	rBV	145816	313429	34.41%	4.474%
20	5.282	1225	1226	1227	rVB	107	21	0.00%	0.000%
21	5.337	1241	1243	1246	rBV	344	169	0.02%	0.002%
22	5.424	1267	1270	1273	rBV	261	183	0.02%	0.003%
23	5.568	1311	1315	1316	rBV2	184	108	0.01%	0.002%
24	5.639	1335	1337	1338	rBV2	134	73	0.01%	0.001%
25	5.719	1341	1362	1394	rVV2	275774	813895	89.35%	11.618%
26	5.993	1444	1447	1453	rVB3	349	320	0.04%	0.005%
27	6.022	1454	1456	1457	rBV3	154	47	0.01%	0.001%
28	6.038	1458	1461	1466	rVB	312	287	0.03%	0.004%
29	6.105	1480	1482	1486	rVB2	341	160	0.02%	0.002%
30	6.166	1499	1501	1504	rBV	270	149	0.02%	0.002%
31	6.243	1511	1525	1550	rBV	287776	548791	60.24%	7.834%
32	6.478	1595	1598	1600	rBV2	196	107	0.01%	0.002%
33	6.687	1649	1663	1687	rBV	173404	347079	38.10%	4.954%
34	7.067	1778	1781	1784	rBV2	190	153	0.02%	0.002%
35	7.096	1788	1790	1791	rBV2	150	42	0.00%	0.001%
36	7.105	1791	1793	1796	rVB	167	57	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
 Data File : VU053620.D
 Acq On : 10 Apr 2023 18:01
 Operator : JC/MD
 Sample : 02251-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	7.189	1813	1819	1827	rBV5	1072	1736	0.19%	0.025%
38	7.234	1831	1833	1835	rBV	251	167	0.02%	0.002%
39	7.266	1841	1843	1844	rBV	175	75	0.01%	0.001%
40	7.472	1902	1907	1910	rBV2	334	410	0.05%	0.006%
41	7.562	1923	1935	1957	rBV	98622	174930	19.20%	2.497%
42	7.694	1970	1976	1984	rVV4	1076	1282	0.14%	0.018%
43	7.726	1984	1986	1989	rVB	231	104	0.01%	0.001%
44	7.893	2024	2038	2067	rBV	352211	622885	68.38%	8.891%
45	8.018	2075	2077	2079	rVB	301	121	0.01%	0.002%
46	8.176	2114	2126	2146	rBV	67569	116014	12.74%	1.656%
47	8.359	2178	2183	2186	rBV	244	279	0.03%	0.004%
48	8.401	2194	2196	2198	rBV	178	104	0.01%	0.001%
49	8.629	2256	2267	2298	rBV	196537	358304	39.33%	5.114%
50	8.845	2330	2334	2341	rBV3	434	524	0.06%	0.007%
51	8.912	2352	2355	2356	rBV	253	145	0.02%	0.002%
52	8.951	2364	2367	2370	rBV2	288	197	0.02%	0.003%
53	9.349	2488	2491	2494	rBV2	294	227	0.02%	0.003%
54	9.414	2498	2511	2546	rVV3	405021	834218	91.58%	11.908%
55	9.784	2624	2626	2630	rBV	200	121	0.01%	0.002%
56	9.867	2649	2652	2653	rBV	170	95	0.01%	0.001%
57	9.951	2675	2678	2679	rBV	172	93	0.01%	0.001%
58	10.060	2709	2712	2714	rVB	278	152	0.02%	0.002%
59	10.089	2718	2721	2726	rBV	226	166	0.02%	0.002%
60	10.340	2796	2799	2802	rBV2	354	280	0.03%	0.004%
61	10.375	2808	2810	2812	rBV	177	121	0.01%	0.002%
62	10.751	2914	2927	2945	rBV	262875	419115	46.01%	5.983%
63	10.880	2964	2967	2969	rBV	290	226	0.02%	0.003%
64	11.658	3206	3209	3212	rVB2	256	177	0.02%	0.003%
65	11.742	3223	3235	3244	rBV	23960	37517	4.12%	0.536%
66	11.809	3244	3256	3280	rVB2	431375	910945	100.00%	13.003%
67	11.954	3299	3301	3305	rVB2	310	172	0.02%	0.002%
68	12.073	3334	3338	3339	rBV2	768	628	0.07%	0.009%
69	12.189	3362	3374	3395	rBV2	399455	794102	87.17%	11.335%
70	12.320	3412	3415	3418	rBV3	424	338	0.04%	0.005%
71	12.362	3425	3428	3429	rBV	304	179	0.02%	0.003%
72	12.388	3435	3436	3439	rVB	324	137	0.02%	0.002%
73	12.433	3446	3450	3452	rBV2	302	214	0.02%	0.003%
74	13.838	3879	3887	3901	rBV3	17818	27358	3.00%	0.391%
75	14.102	3963	3969	3971	rBV2	708	780	0.09%	0.011%
76	14.182	3993	3994	3997	rBV2	520	221	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053620.D
Acq On : 10 Apr 2023 18:01
Operator : JC/MD
Sample : 02251-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis

77	14.330	4034	4040	4050	rVB3	5279	8159	0.90%	0.116%
----	--------	------	------	------	------	------	------	-------	--------




Sum of corrected areas: 7005654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053620.D
Acq On : 10 Apr 2023 18:01
Operator : JC/MD
Sample : 02251-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

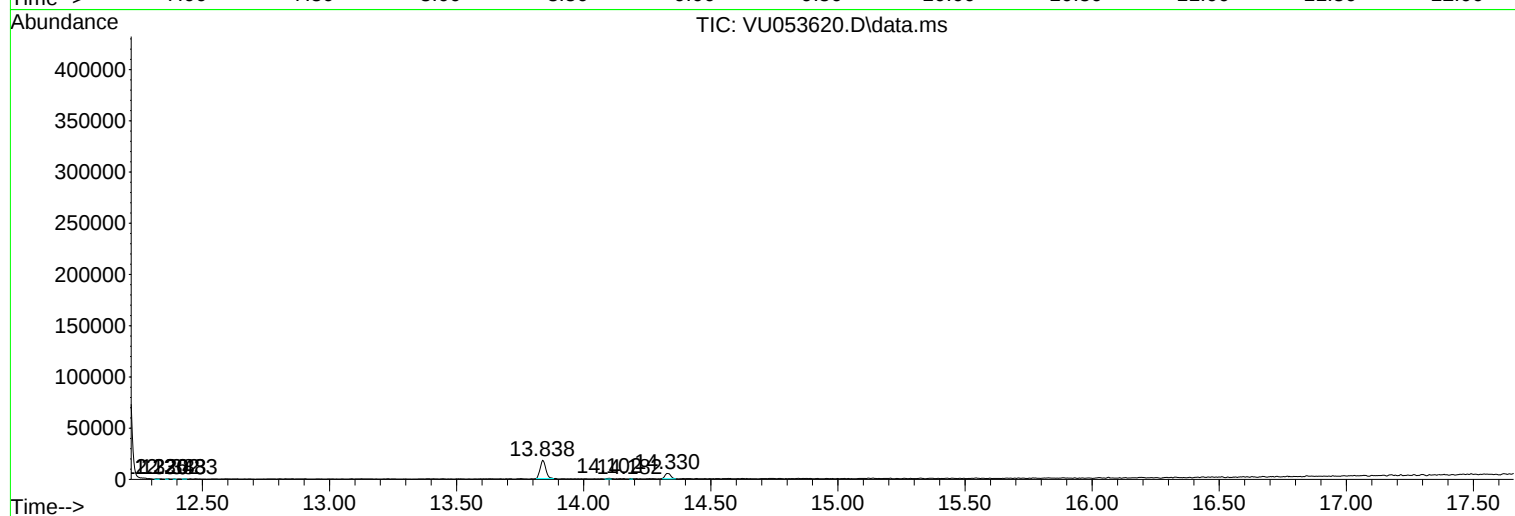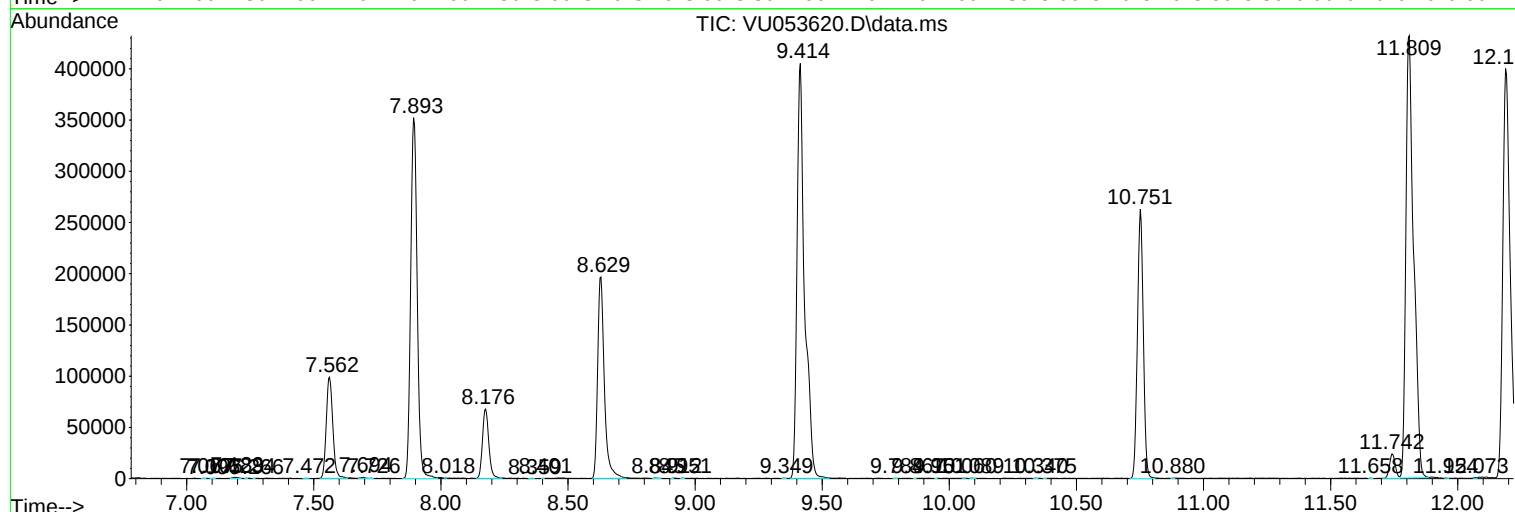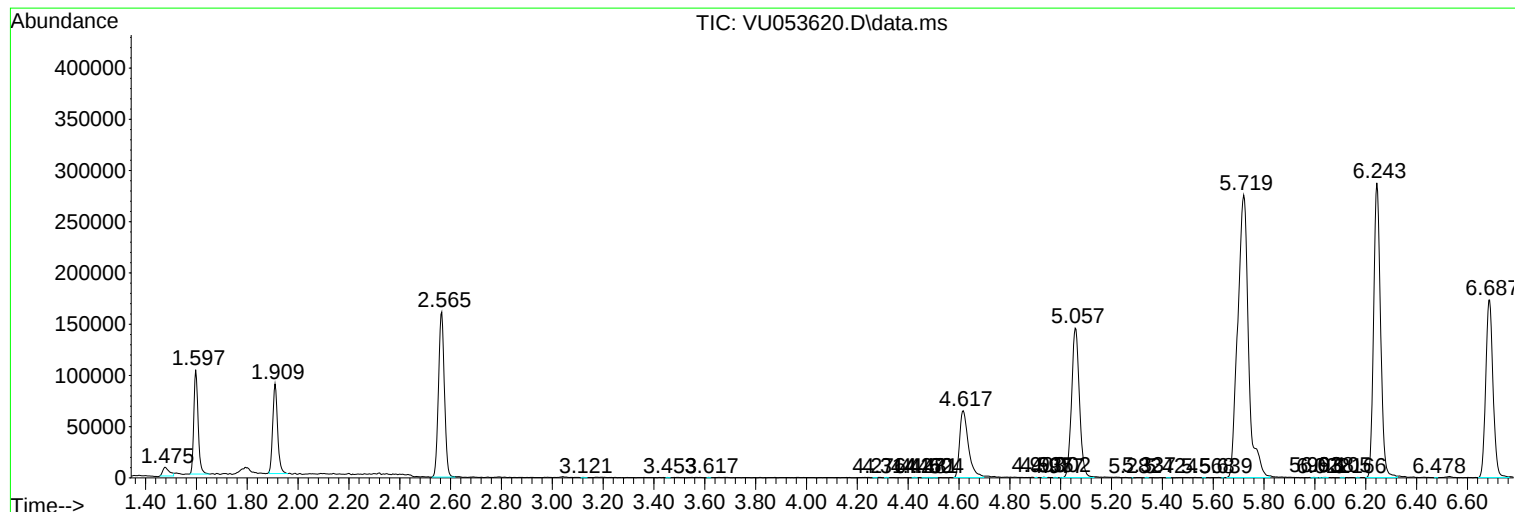

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053620.D
Acq On : 10 Apr 2023 18:01
Operator : JC/MD
Sample : 02251-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053620.D
Acq On : 10 Apr 2023 18:01
Operator : JC/MD
Sample : 02251-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------