
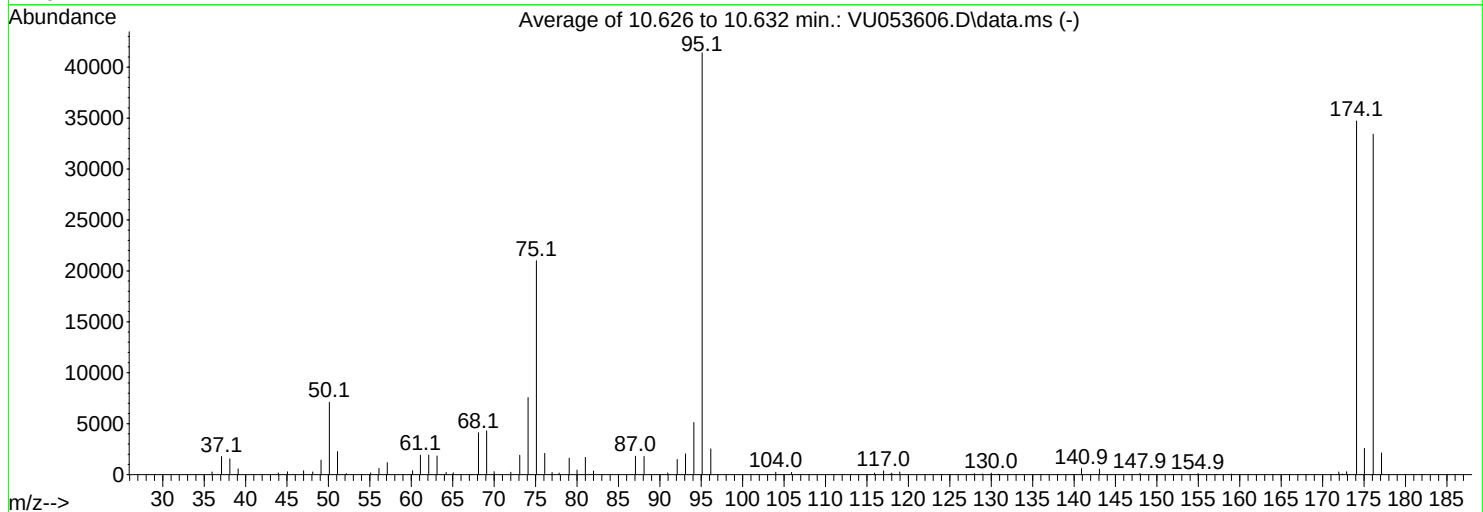


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041023\
Data File : VU053606.D
Acq On : 10 Apr 2023 09:02
Operator : JC/MD
Sample : BFB177
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB177

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Title : VOC Analysis
Last Update : Tue Apr 11 02:19:45 2023

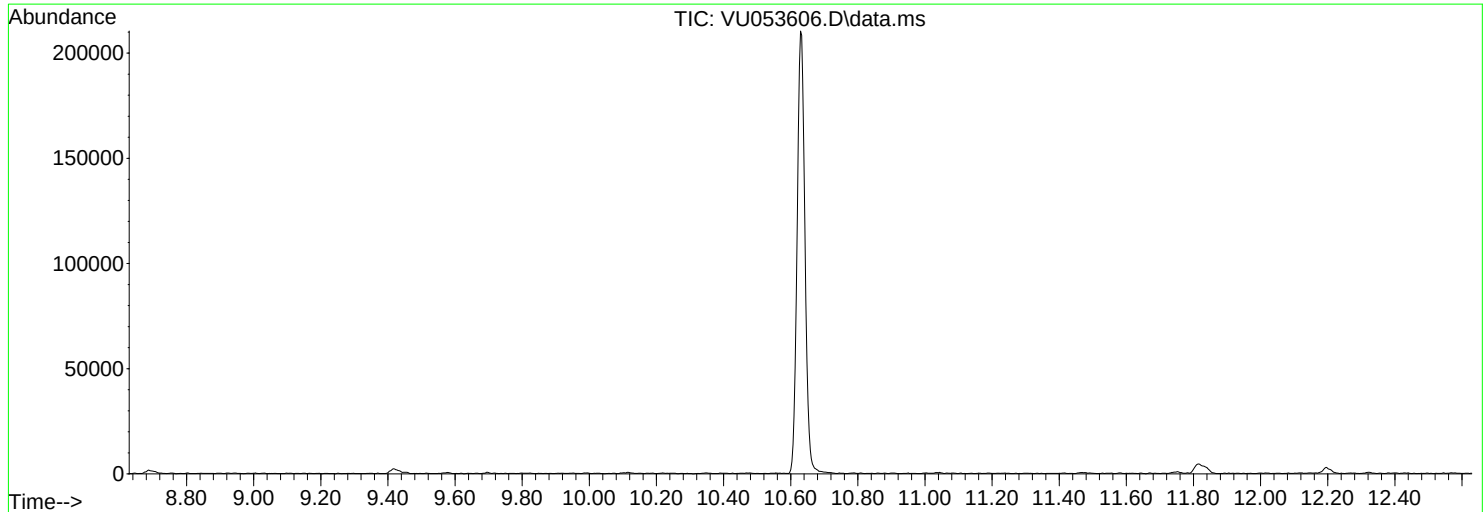

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	7105	PASS
75	95	30	80	50.7	21005	PASS
95	95	100	100	100.0	41408	PASS
96	95	5	9	6.1	2527	PASS
173	174	0.00	2	0.8	277	PASS
174	95	50	120	83.8	34712	PASS
175	174	5	9	7.4	2577	PASS
176	174	95	101	96.3	33429	PASS
177	176	5	9	6.4	2133	PASS

m/z	Abundance
43.90	228.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
35.90	223.0
37.10	1666.0
38.10	1582.0
39.10	575.0
44.00	397.0
45.00	334.0
47.00	361.0
48.10	190.0
49.10	1345.0
50.10	7281.0
51.10	2120.0
55.10	201.0
56.10	565.0
57.10	1105.0
60.20	323.0
61.10	1709.0
62.10	1721.0
63.10	1733.0
64.20	269.0
65.10	142.0
67.20	101.0
68.10	3869.0
69.10	4023.0
70.00	337.0
72.00	172.0
73.10	1910.0
74.10	7379.0
75.10	20392.0
76.10	2192.0
77.00	214.0
77.80	150.0
79.10	1536.0
80.00	393.0
81.00	1713.0
82.00	354.0
87.00	1740.0
88.10	1765.0
91.00	196.0
92.10	1407.0
93.10	1917.0
94.10	4914.0
95.10	39544.0
96.20	2453.0
104.00	230.0
105.90	191.0
115.90	109.0
117.00	369.0
117.80	192.0
118.90	233.0
127.90	111.0
130.00	123.0
130.90	100.0
140.90	504.0
143.00	506.0
148.00	145.0
155.00	114.0
159.00	103.0
171.90	199.0
172.40	189.0
172.90	214.0
174.10	32136.0
175.10	2414.0
176.10	31160.0
177.10	1988.0
178.00	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
36.00	260.0
37.10	1848.0
38.10	1648.0
39.10	598.0
44.10	417.0
45.10	278.0
47.00	378.0
48.10	270.0
49.10	1491.0
50.10	7368.0
51.10	2325.0
52.20	129.0
55.10	191.0
56.10	630.0
57.10	1198.0
60.20	389.0
61.10	1973.0
62.10	1956.0
63.10	1932.0
64.20	238.0
65.00	207.0
68.10	4214.0
69.10	4467.0
70.00	316.0
72.00	242.0
73.10	1963.0
74.10	7775.0
75.10	21504.0
76.10	2191.0
77.00	238.0
77.90	166.0
79.10	1625.0
80.00	468.0
81.00	1749.0
82.00	368.0
87.00	1889.0
88.10	1858.0
90.90	164.0
92.10	1591.0
93.10	2117.0
94.10	5366.0
95.10	42632.0
96.10	2584.0
104.00	236.0
105.90	230.0
115.90	161.0
117.00	404.0
118.00	233.0
118.90	270.0
127.90	107.0
128.90	110.0
130.00	174.0
130.90	106.0
140.90	612.0
143.10	579.0
148.00	142.0
155.00	117.0
159.00	104.0
172.00	271.0
172.90	287.0
174.10	35824.0
175.10	2685.0
176.10	34424.0
177.10	2194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177

m/z	Abundance
36.00	332.0
37.10	1834.0
38.10	1450.0
39.10	507.0
44.10	384.0
45.10	216.0
47.00	409.0
48.10	336.0
49.10	1453.0
50.10	6667.0
51.10	2359.0
52.10	190.0
55.10	122.0
56.10	656.0
57.10	1228.0
60.10	405.0
61.10	2055.0
62.10	2127.0
63.10	1852.0
64.10	160.0
65.00	236.0
68.10	4263.0
69.10	4438.0
70.00	257.0
72.00	315.0
73.10	1836.0
74.10	7544.0
75.10	21120.0
76.10	1887.0
77.00	226.0
77.90	139.0
79.00	1697.0
80.00	490.0
81.00	1638.0
82.00	346.0
87.10	1803.0
88.10	1746.0
90.90	154.0
92.10	1500.0
93.10	2092.0
94.10	5094.0
95.10	42048.0
96.10	2544.0
97.00	109.0
104.00	232.0
105.90	247.0
115.90	210.0
117.00	359.0
118.00	237.0
119.00	314.0
128.00	110.0
128.90	140.0
130.00	187.0
135.00	101.0
137.00	102.0
140.90	673.0
143.10	577.0
147.80	117.0
154.90	116.0
157.20	114.0
172.00	311.0
172.90	329.0
174.10	36176.0
175.00	2631.0
176.10	34704.0
177.10	2218.0

Instrument :
MSVOA_U
ClientSampleId :
BFB177