

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
 Data File : VU058549.D
 Acq On : 10 Apr 2024 11:04
 Operator : MD/SY
 Sample : VU0410WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK170

Quant Time: Apr 11 01:29:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 11 01:28:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	62680	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	60856	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	25598	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	23200	5.591	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	111.800%	
7) Chloroethane-d5	1.907	69	19790	5.487	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	109.800%	
11) 1,1-Dichloroethene-d2	2.560	65	10445	5.561	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	111.200%	
20) 2-Butanone-d5	4.627	46	41590	47.557	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	95.120%	
24) Chloroform-d	5.055	84	43288	5.225	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.600%	
26) 1,2-Dichloroethane-d4	5.695	65	20153	5.213	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.200%	
32) Benzene-d6	5.721	84	85778	5.235	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.800%	
36) 1,2-Dichloropropane-d6	6.685	67	26740	5.204	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.000%	
41) Toluene-d8	7.894	98	71099	4.893	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.800%	
43) trans-1,3-Dichloroprop...	8.177	79	7270	4.558	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.200%	
46) 2-Hexanone-d5	8.630	63	26064	39.621	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	79.240%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	15497	4.272	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	85.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152	20259	4.699	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.000%	
Target Compounds					Qvalue	
13) Acetone	2.634	43	4829	6.470	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058549.D
Acq On : 10 Apr 2024 11:04
Operator : MD/SY
Sample : VU0410WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK170

Quant Time: Apr 11 01:29:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 11 01:28:06 2024
Response via : Initial Calibration

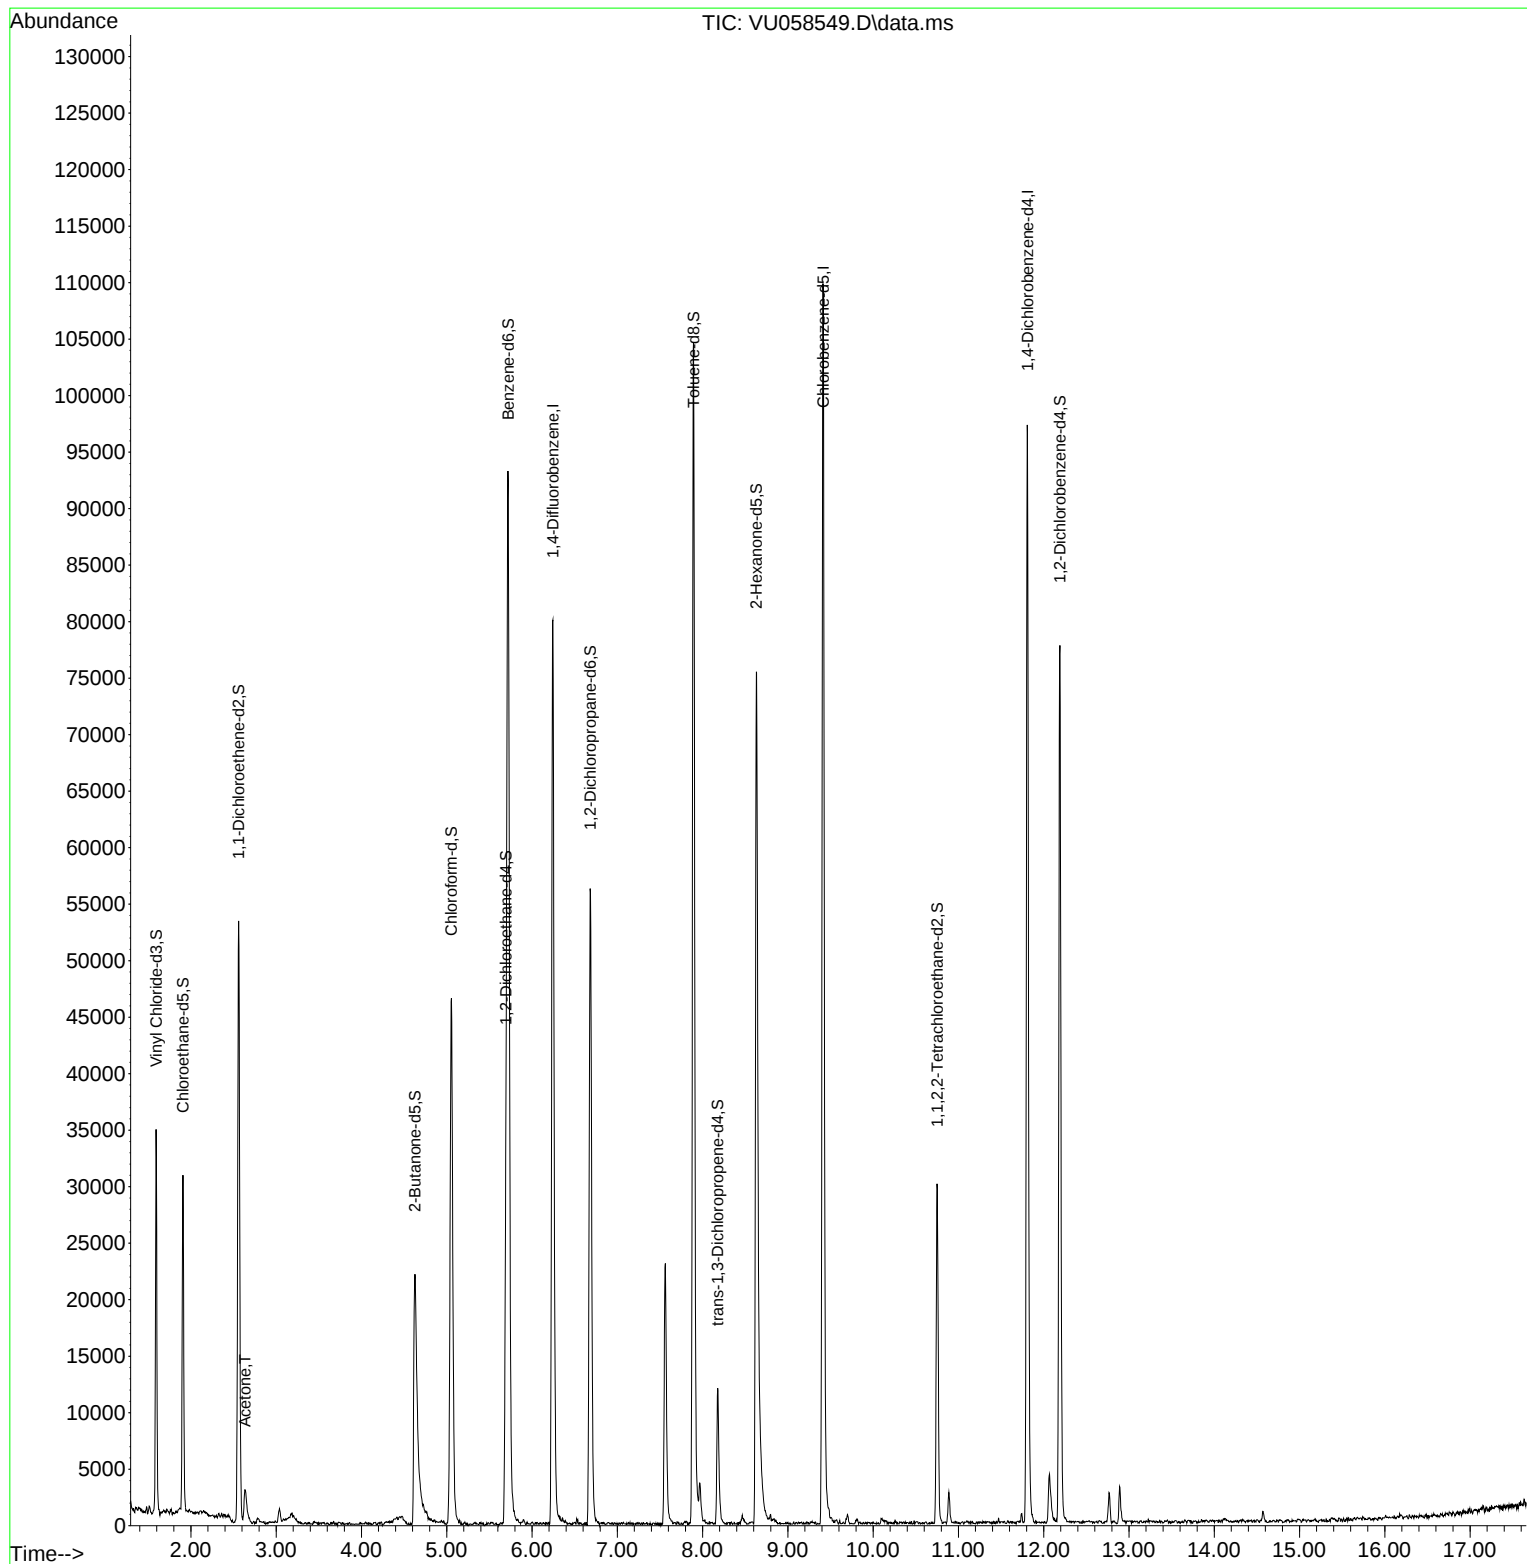

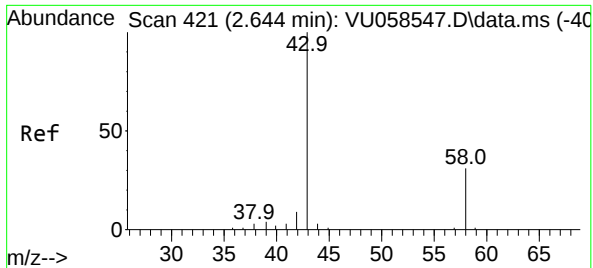

#13
 Acetone
 Concen: 6.470 ug/L
 RT: 2.634 min Scan# 41
 Delta R.T. -0.010 min
 Lab File: VU058549.D
 Acq: 10 Apr 2024 11:04

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK170

Tgt Ion: 43 Resp: 4829
 Ion Ratio Lower Upper
 43 100
 58 28.8 0.0 61.4

