

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
 Data File : VU058566.D
 Acq On : 10 Apr 2024 17:42
 Operator : MD/SY
 Sample : P2013-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EOMB4

Quant Time: Apr 11 01:33:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 11 01:28:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	79528	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	78592	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	32329	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.589	65	24288	4.613	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.200%
7) Chloroethane-d5	1.904	69	21325	4.660	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.557	65	11277	4.732	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.600%
20) 2-Butanone-d5	4.647	46	39741	35.816	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	71.640%
24) Chloroform-d	5.052	84	47087	4.480	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
26) 1,2-Dichloroethane-d4	5.695	65	22447	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
32) Benzene-d6	5.718	84	93106	4.400	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%
36) 1,2-Dichloropropane-d6	6.682	67	29060	4.379	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.600%
41) Toluene-d8	7.891	98	77190	4.114	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	8.174	79	7872	3.822	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.400%
46) 2-Hexanone-d5	8.631	63	29915	35.212	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	70.420%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	17024	3.634	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	72.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	23084	4.239	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.800%
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	4.660	96	2296	0.346	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058566.D
Acq On : 10 Apr 2024 17:42
Operator : MD/SY
Sample : P2013-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EOMB4

Quant Time: Apr 11 01:33:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 11 01:28:06 2024
Response via : Initial Calibration

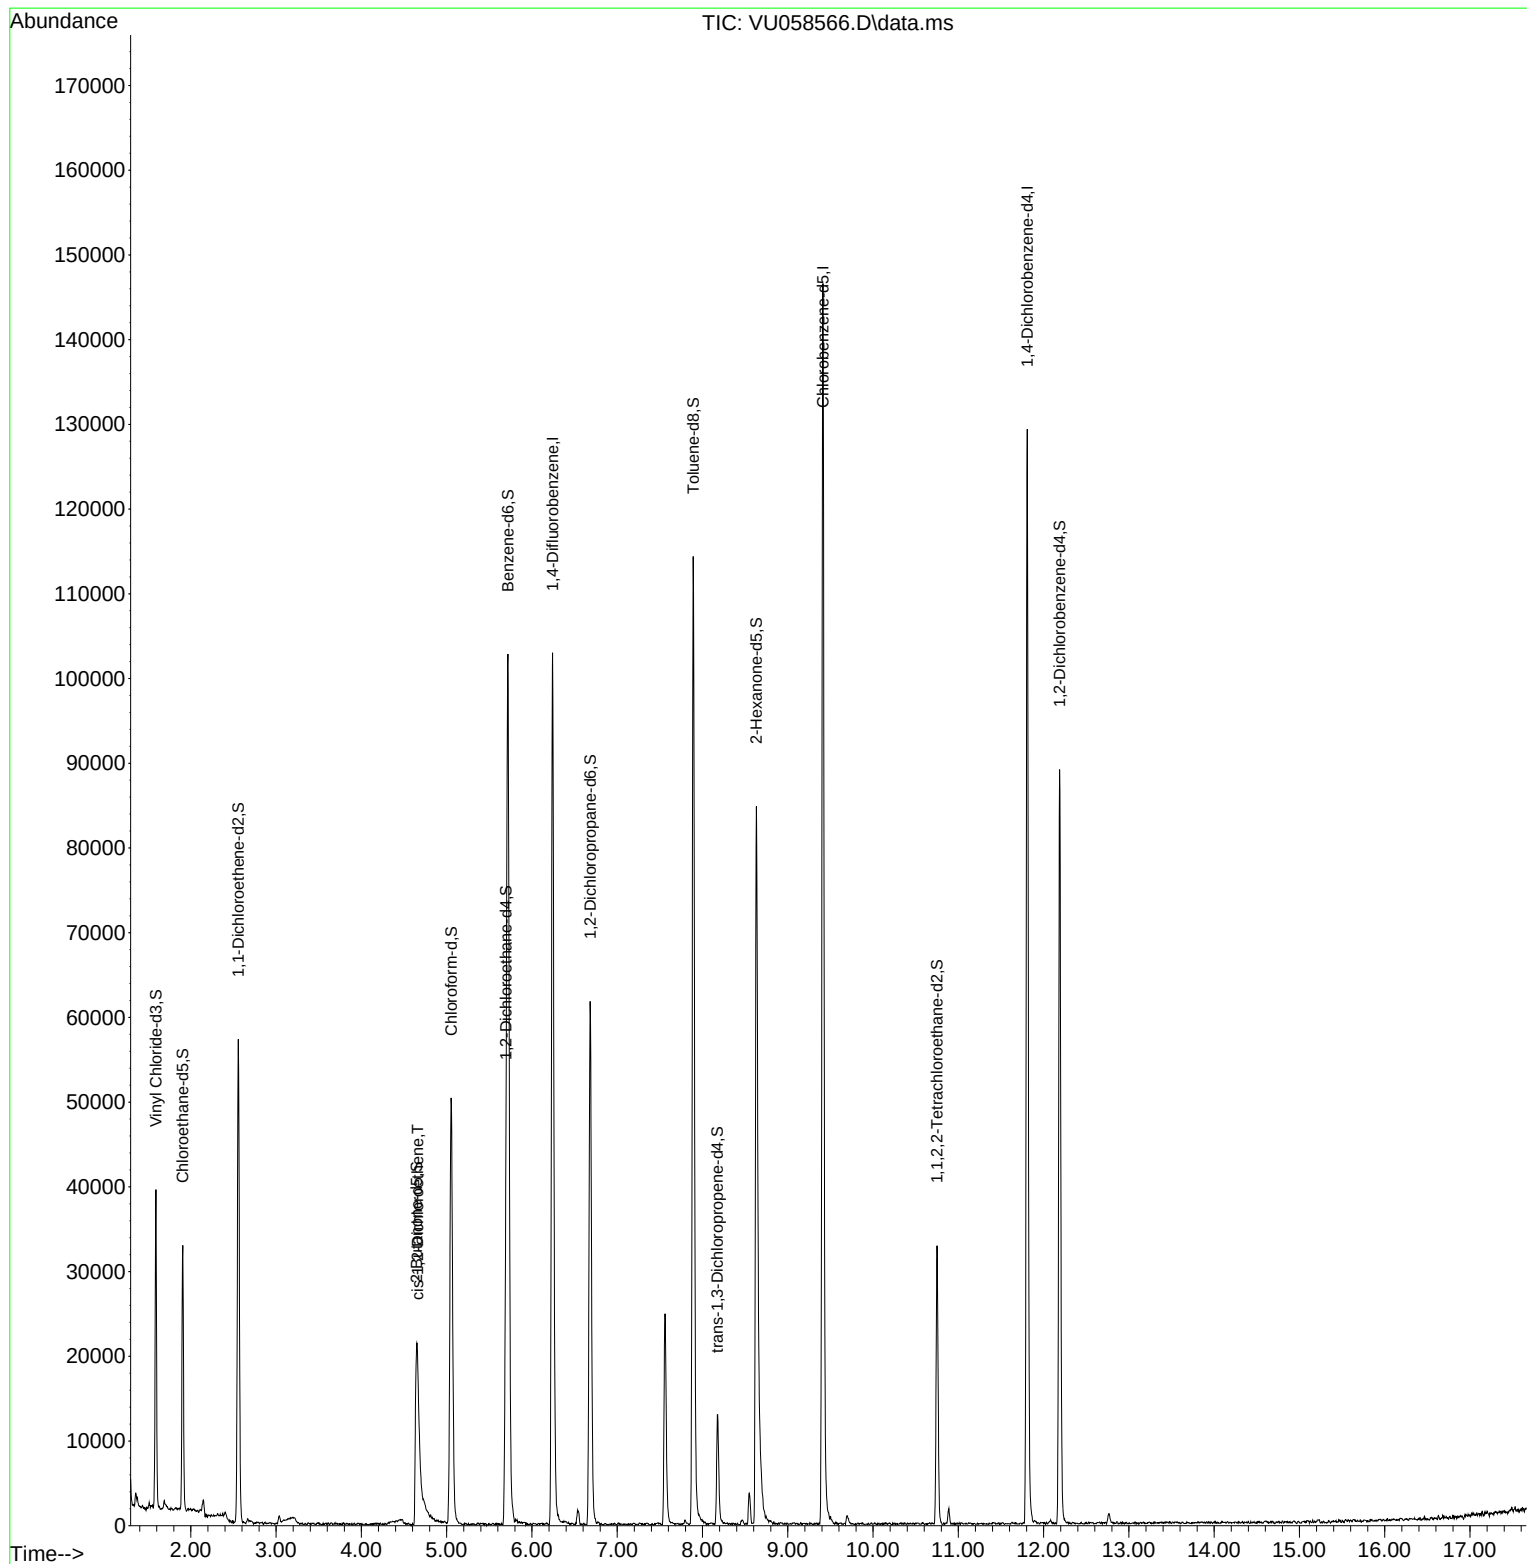

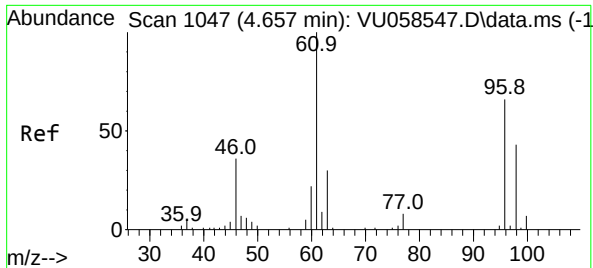

#22
 cis-1,2-Dichloroethene
 Concen: 0.346 ug/L
 RT: 4.660 min Scan# 10
 Delta R.T. 0.003 min
 Lab File: VU058566.D
 Acq: 10 Apr 2024 17:42

Instrument :
 MSVOA_U
 ClientSampleId :
 E0MB4

Tgt Ion: 96	Resp:	2296
Ion	Ratio	Lower Upper
96	100	
61	143.8	98.1 182.3
98	62.2	43.6 81.0

