

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
 Data File : VU058561.D
 Acq On : 10 Apr 2024 15:45
 Operator : MD/SY
 Sample : P2014-06DL 10X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0MD3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.354	14	20	34	rVB	38128	38373	11.55%	1.638%
2	1.486	55	61	67	rVB	4573	4769	1.43%	0.204%
3	1.596	86	95	111	rVB2	46049	54706	16.46%	2.336%
4	1.904	183	191	204	rVB	31713	40865	12.30%	1.745%
5	2.560	384	395	412	rBV	53339	87037	26.19%	3.716%
6	3.036	534	543	553	rBV2	2117	3471	1.04%	0.148%
7	3.348	628	640	651	rBV4	2454	5051	1.52%	0.216%
8	4.653	1023	1046	1074	rBV2	115097	332352	100.00%	14.189%
9	5.052	1156	1170	1190	rBV	48158	106675	32.10%	4.554%
10	5.718	1359	1377	1400	rBV2	97732	246752	74.24%	10.534%
11	6.242	1527	1540	1565	rBV	106820	202934	61.06%	8.664%
12	6.682	1664	1677	1701	rBV	59104	117629	35.39%	5.022%
13	7.560	1936	1950	1971	rBV2	23852	44036	13.25%	1.880%
14	7.891	2039	2053	2077	rBV	108110	193978	58.37%	8.281%
15	8.177	2133	2142	2159	rBV2	12138	21788	6.56%	0.930%
16	8.631	2273	2283	2318	rBV2	85968	182466	54.90%	7.790%
17	9.412	2514	2526	2551	rBV	148449	255746	76.95%	10.918%
18	10.750	2931	2942	2958	rBV	32803	53996	16.25%	2.305%
19	11.807	3259	3271	3302	rBV	126990	211374	63.60%	9.024%
20	12.187	3378	3389	3407	rBV	82172	138354	41.63%	5.907%




Sum of corrected areas: 2342352

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058561.D
Acq On : 10 Apr 2024 15:45
Operator : MD/SY
Sample : P2014-06DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0MD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

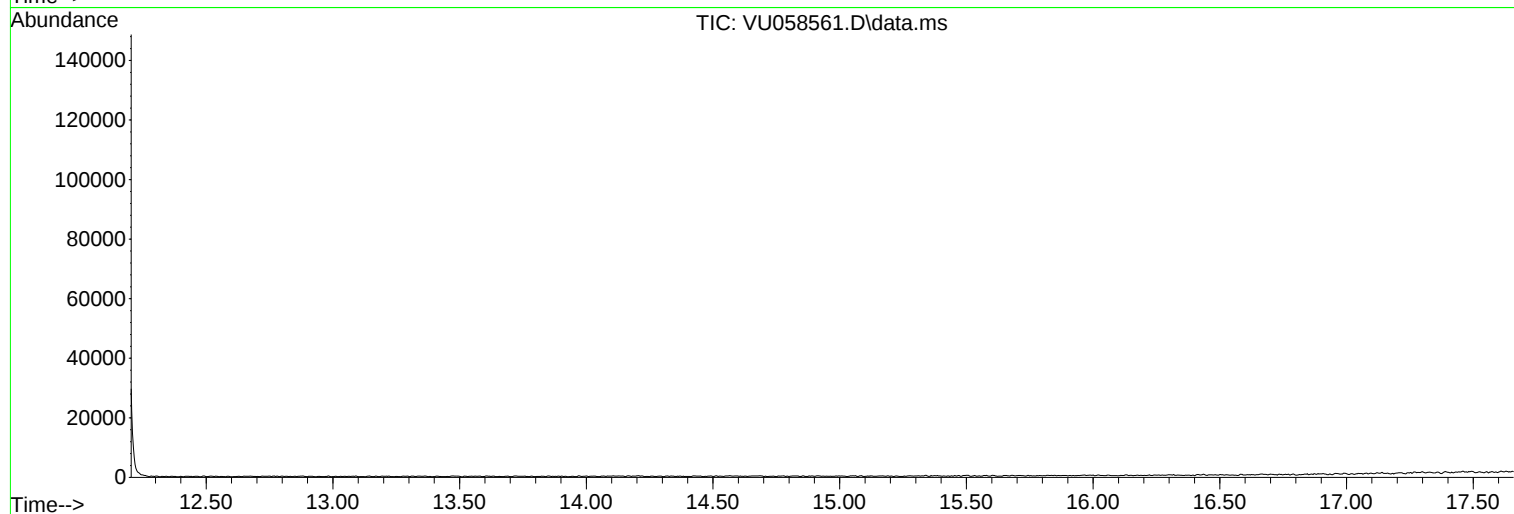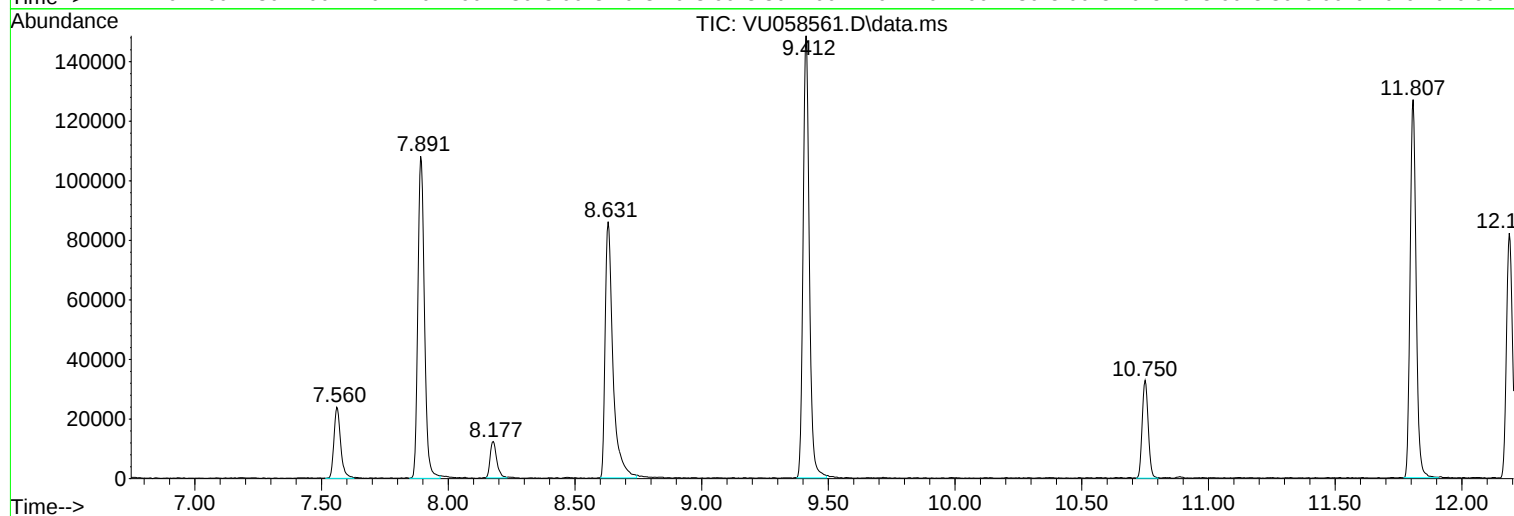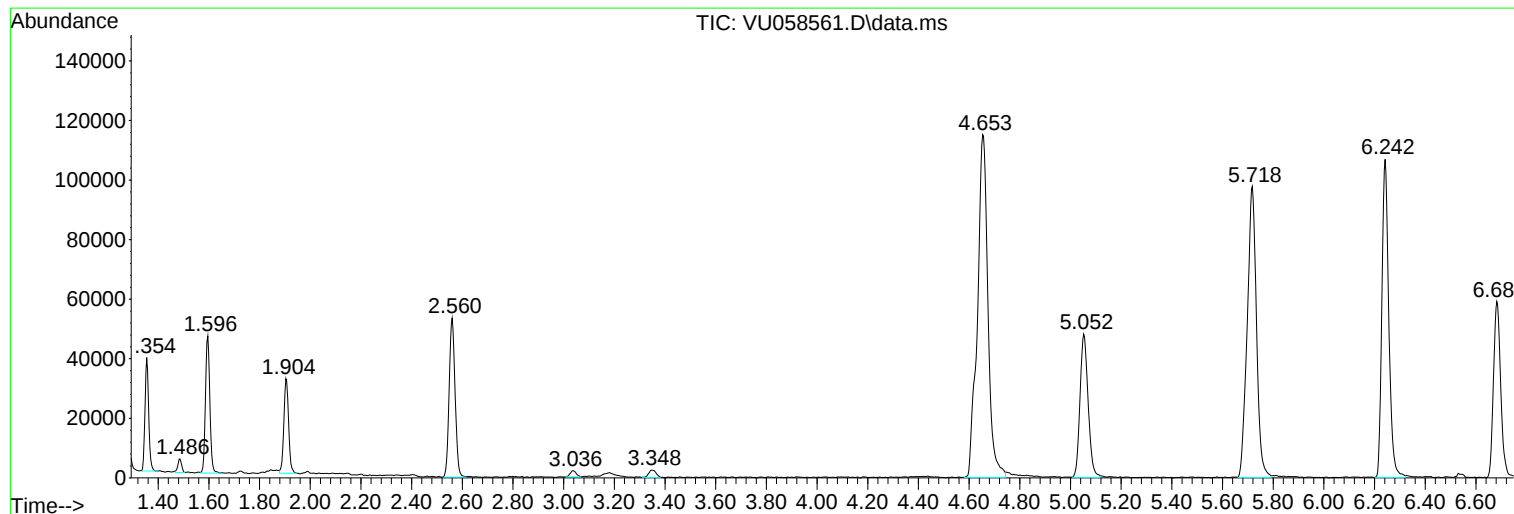

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058561.D
Acq On : 10 Apr 2024 15:45
Operator : MD/SY
Sample : P2014-06DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0MD3DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.354	0.95 ug/L	38373	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane			44	C3H8	000074-98-6	90
2	Propane			44	C3H8	000074-98-6	83
3	Propane			44	C3H8	000074-98-6	9
4	Propene			42	C3H6	000115-07-1	9
5	Acetaldehyde			44	C2H4O	000075-07-0	5

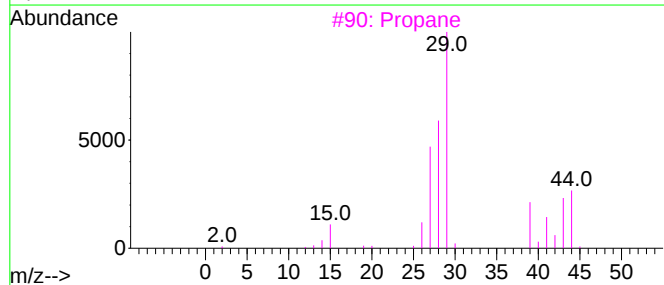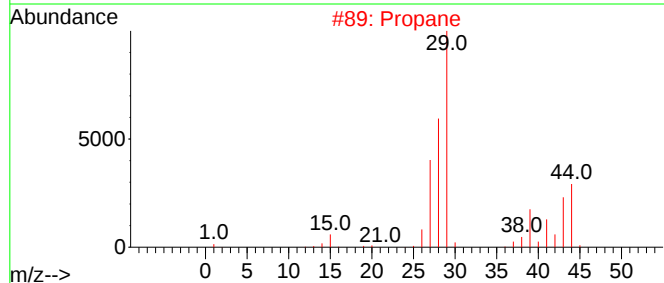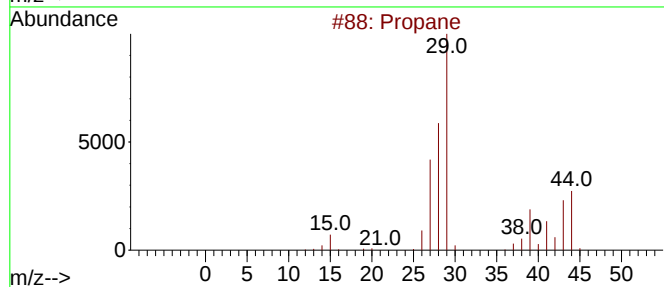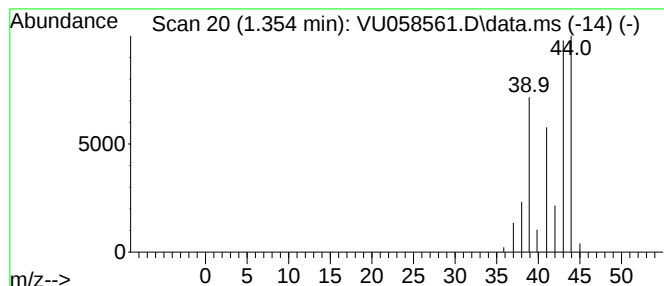

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058561.D
Acq On : 10 Apr 2024 15:45
Operator : MD/SY
Sample : P2014-06DL 10X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0MD3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.354	0.9	ug/L	38373	1	6.242	202934	5.0