

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
 Data File : VU058562.D
 Acq On : 10 Apr 2024 16:09
 Operator : MD/SY
 Sample : P1970-19 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU058562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	107	rVB	36285	40456	10.57%	1.476%
2	1.907	183	192	211	rVB	35034	46576	12.17%	1.700%
3	2.570	384	398	418	rBV3	206827	382812	100.00%	13.971%
4	3.036	534	543	554	rBV2	4266	7703	2.01%	0.281%
5	3.856	780	798	819	rBV	71653	170346	44.50%	6.217%
6	4.624	1024	1037	1070	rBV2	27061	76888	20.09%	2.806%
7	5.052	1152	1170	1190	rBV	52752	117337	30.65%	4.282%
8	5.306	1234	1249	1268	rBV2	35348	79125	20.67%	2.888%
9	5.717	1359	1377	1403	rBV3	106743	271056	70.81%	9.892%
10	6.242	1528	1540	1562	rBV	110514	214274	55.97%	7.820%
11	6.537	1624	1632	1642	rBV8	2658	4840	1.26%	0.177%
12	6.682	1665	1677	1703	rBV	66061	128743	33.63%	4.698%
13	7.560	1939	1950	1967	rBV2	26916	48290	12.61%	1.762%
14	7.891	2041	2053	2074	rBV	118644	212815	55.59%	7.767%
15	8.177	2132	2142	2156	rBV2	14216	25539	6.67%	0.932%
16	8.630	2272	2283	2319	rBV2	96094	202797	52.98%	7.401%
17	9.412	2514	2526	2555	rBV	156330	270584	70.68%	9.875%
18	10.749	2932	2942	2963	rVB	36037	59074	15.43%	2.156%
19	11.807	3260	3271	3300	rBV	133762	226280	59.11%	8.258%
20	12.187	3378	3389	3405	rBV	90929	154580	40.38%	5.641%




Sum of corrected areas: 2740115

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058562.D
Acq On : 10 Apr 2024 16:09
Operator : MD/SY
Sample : P1970-19 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

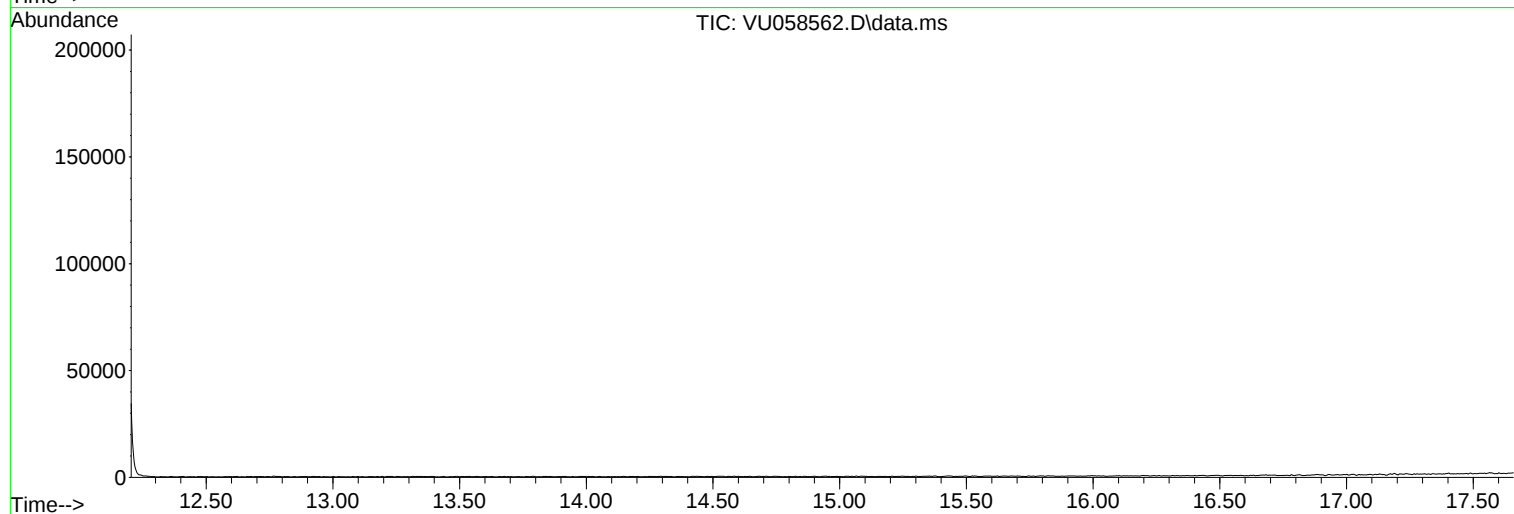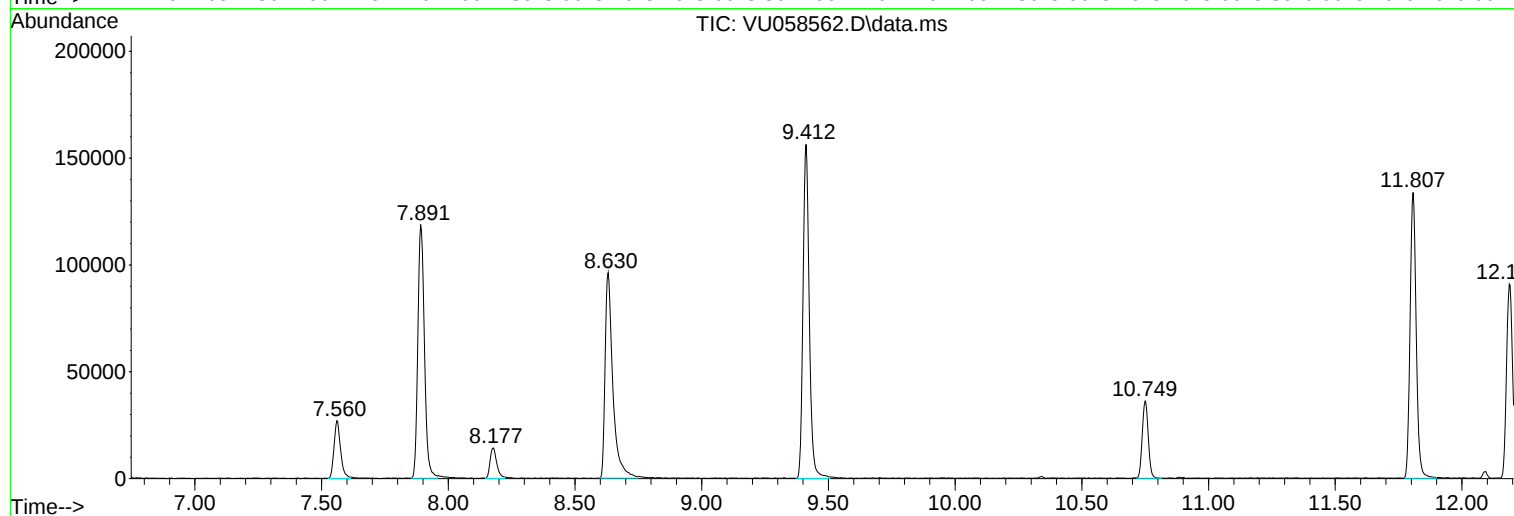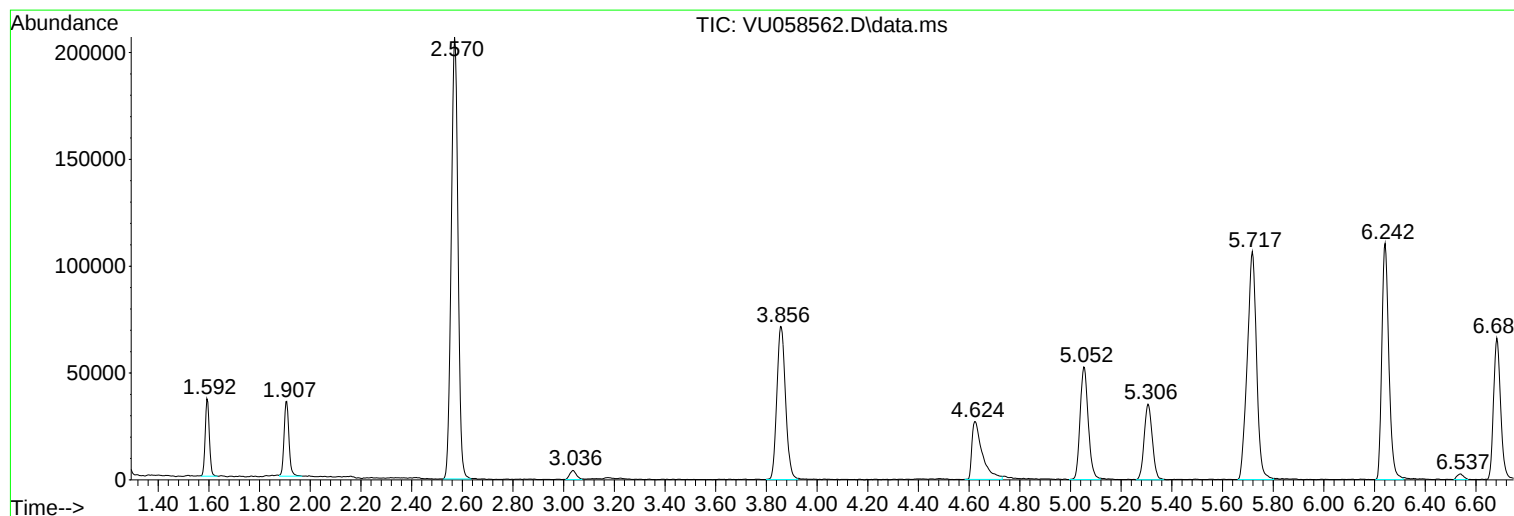

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058562.D
Acq On : 10 Apr 2024 16:09
Operator : MD/SY
Sample : P1970-19 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058562.D
Acq On : 10 Apr 2024 16:09
Operator : MD/SY
Sample : P1970-19 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc