


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041024\
Data File : VU058546.D
Acq On : 10 Apr 2024 09:04
Operator : MD/SY
Sample : BFB140
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB140

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 12 04:41:05 2024

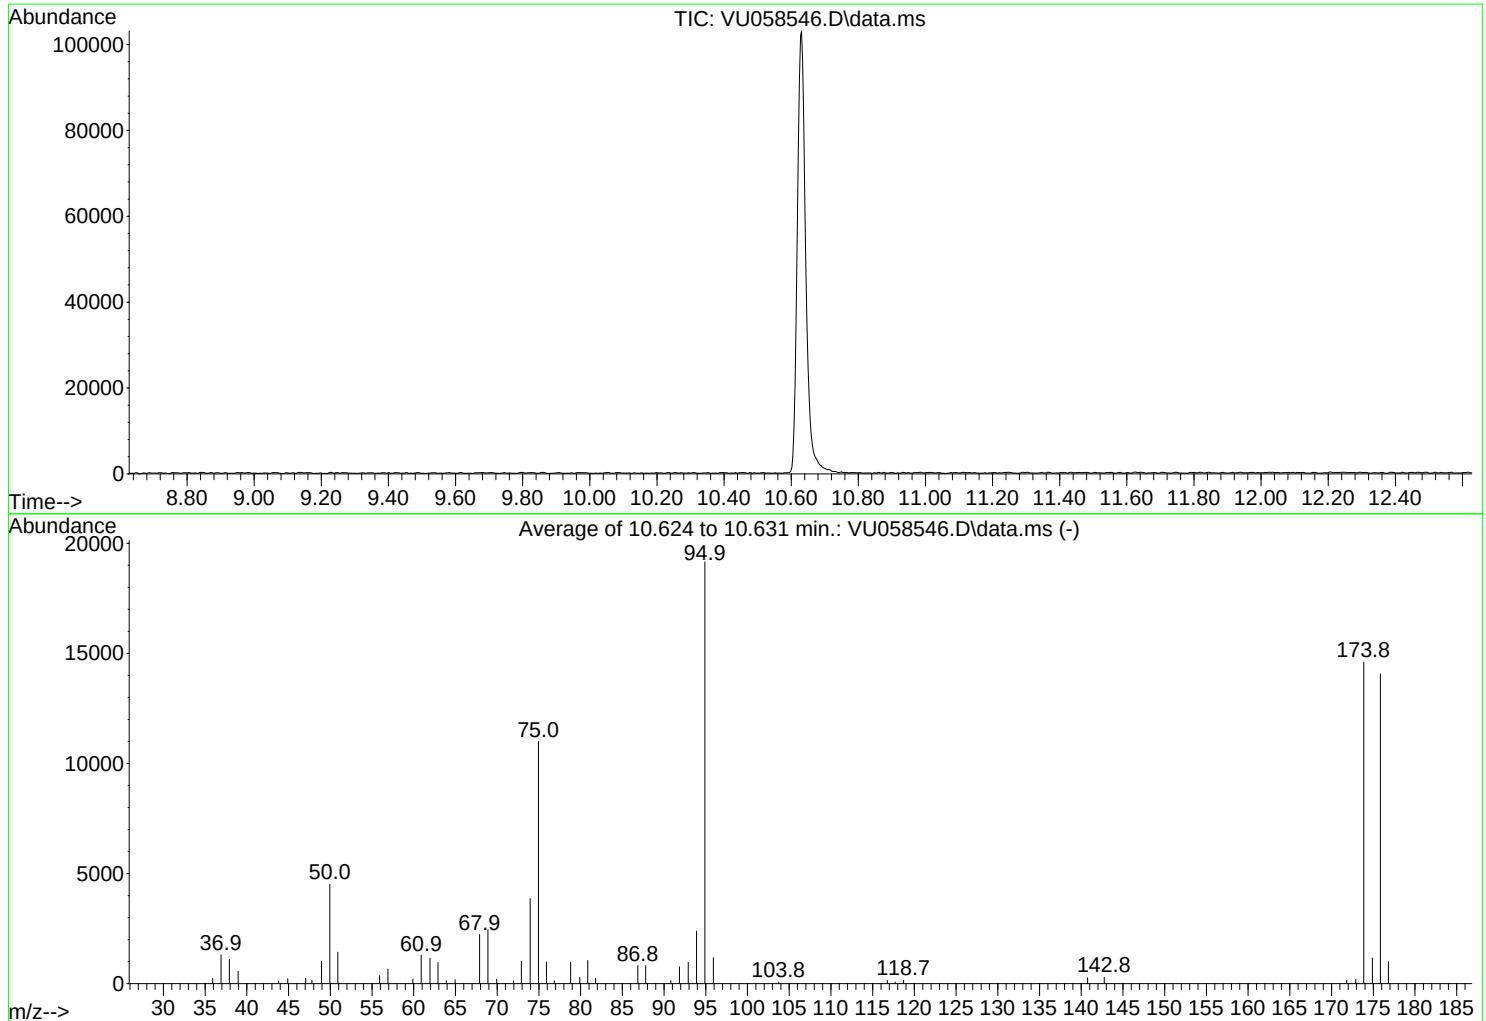

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.5	4509	PASS
75	95	30	80	57.4	10999	PASS
95	95	100	100	100.0	19155	PASS
96	95	5	9	6.1	1169	PASS
173	174	0.00	2	1.3	190	PASS
174	95	50	120	76.2	14596	PASS
175	174	5	9	8.0	1166	PASS
176	174	95	101	96.4	14071	PASS
177	176	5	9	7.1	995	PASS

m/z	Abundance
39.80	108.0
43.80	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
35.90	226.0
36.90	1125.0
37.90	1086.0
38.90	513.0
43.80	268.0
44.90	208.0
47.00	229.0
47.80	147.0
48.90	959.0
49.90	4110.0
50.90	1356.0
55.90	346.0
56.90	610.0
59.90	193.0
60.90	1197.0
61.90	1088.0
62.90	891.0
63.90	136.0
65.00	159.0
67.90	2110.0
68.90	2270.0
70.00	194.0
71.90	116.0
72.90	944.0
73.90	3684.0
75.00	10165.0
75.90	937.0
76.80	121.0
78.80	884.0
79.90	245.0
80.80	982.0
81.80	203.0
86.80	727.0
87.80	801.0
90.80	135.0
91.80	722.0
92.90	897.0
93.90	2243.0
94.90	18040.0
95.90	1128.0
116.80	165.0
117.70	117.0
118.70	129.0
140.70	259.0
142.70	247.0
171.80	132.0
173.90	13527.0
174.90	1091.0
175.90	12938.0
176.80	964.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
35.90	247.0
36.90	1362.0
37.90	1122.0
39.00	577.0
43.90	301.0
44.90	219.0
47.10	261.0
47.80	152.0
48.90	1043.0
50.00	4636.0
50.90	1455.0
55.90	377.0
56.90	686.0
59.90	227.0
60.90	1315.0
62.00	1169.0
62.90	986.0
63.90	143.0
65.00	186.0
67.90	2300.0
68.90	2540.0
70.00	212.0
72.00	139.0
72.90	1055.0
73.90	3953.0
75.00	11368.0
75.90	1013.0
76.90	143.0
78.80	994.0
79.90	287.0
80.80	1097.0
81.80	255.0
86.90	844.0
87.80	836.0
90.80	140.0
91.90	808.0
92.90	1007.0
93.90	2415.0
94.90	19720.0
95.90	1176.0
103.80	108.0
116.70	146.0
117.70	120.0
118.70	165.0
140.80	280.0
142.80	296.0
171.80	151.0
172.90	267.0
173.90	14931.0
174.90	1225.0
175.80	14412.0
176.80	1024.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140

m/z	Abundance
35.90	239.0
36.90	1442.0
37.90	1099.0
39.00	587.0
39.80	128.0
43.90	310.0
44.90	240.0
47.00	237.0
47.80	164.0
49.00	1022.0
49.90	4780.0
50.90	1491.0
55.90	365.0
56.90	695.0
59.90	211.0
60.90	1337.0
62.00	1188.0
62.90	1009.0
63.90	125.0
64.90	196.0
67.90	2276.0
68.90	2541.0
69.90	201.0
72.00	147.0
72.90	1034.0
74.00	3958.0
74.90	11465.0
75.90	1002.0
76.90	137.0
78.80	1008.0
79.90	303.0
80.90	1074.0
81.80	253.0
86.90	896.0
87.80	826.0
90.80	135.0
91.90	754.0
92.90	1006.0
93.90	2483.0
94.90	19704.0
95.90	1202.0
103.70	114.0
116.70	128.0
118.70	161.0
140.80	278.0
142.80	323.0
171.80	174.0
172.90	303.0
173.80	15330.0
174.90	1181.0
175.80	14863.0
176.80	997.0

Instrument :
MSVOA_U
ClientSampleId :
BFB140