
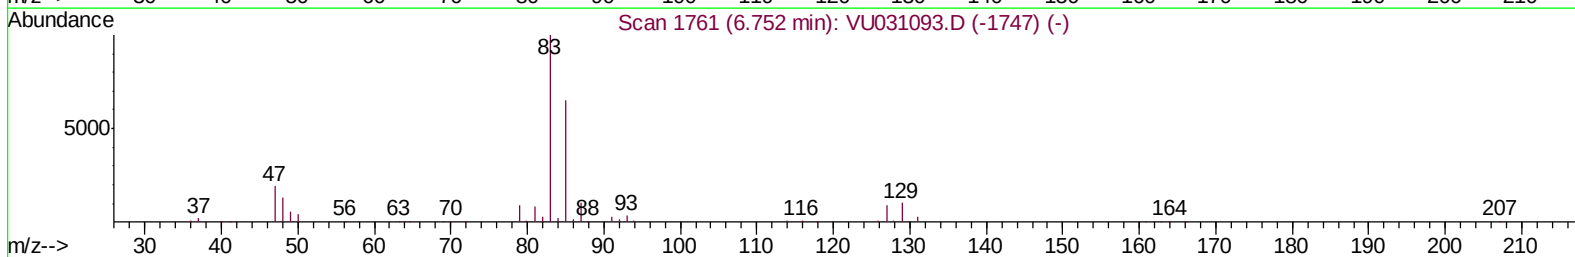
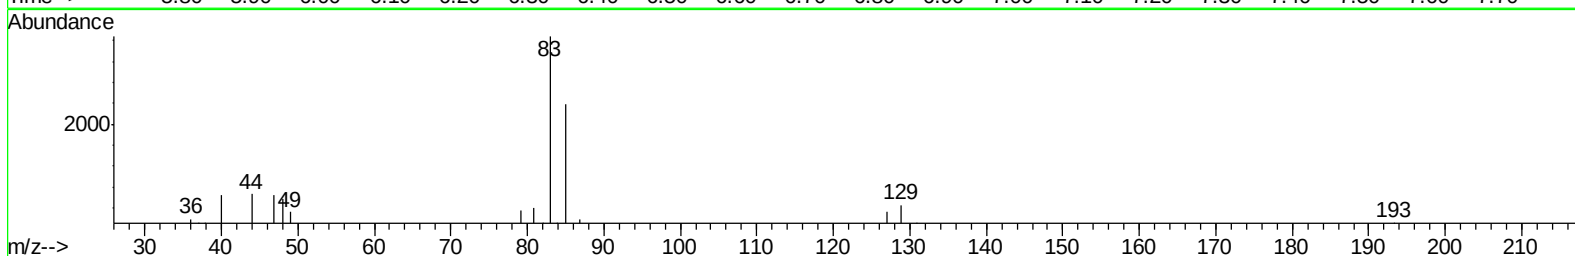


Data File : VU031113.D
Acq On : 12 Apr 2019 08:38
Operator : JC/SP
Sample : K2341-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 105 Sample Multiplier: 1

Quant Time: Apr 12 23:34:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 23:21:49 2019
Response via : Initial Calibration

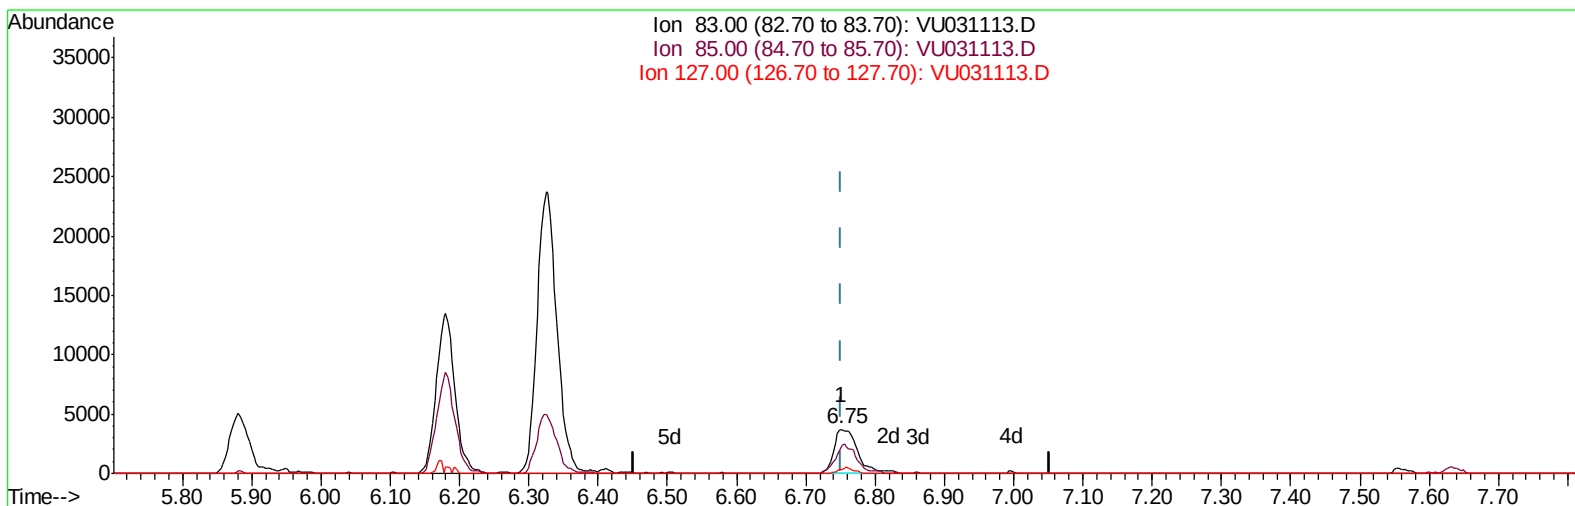

TIC: VU031113.D

(38) Bromodichloromethane (T)

6.752min (+0.000) 1.48ug/L m

response 8575

Ion	Exp%	Act%
83.00	100	100
85.00	66.40	64.81
127.00	8.30	8.70
0.00	0.00	0.00