
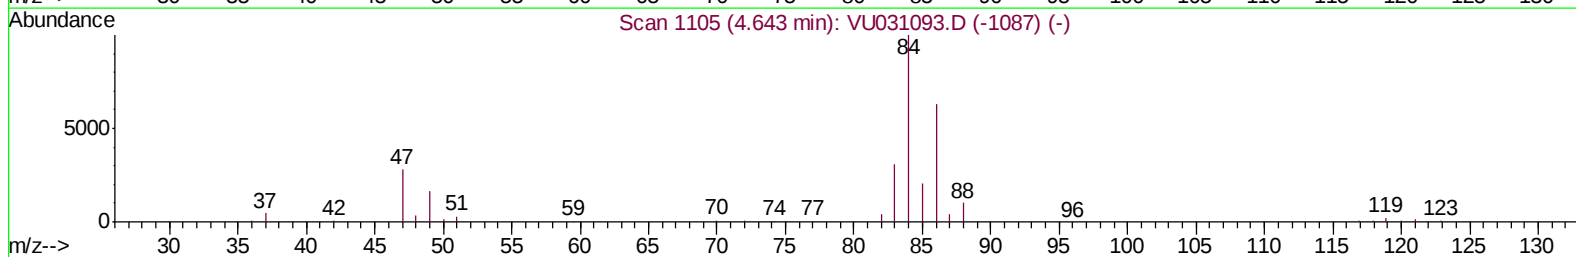
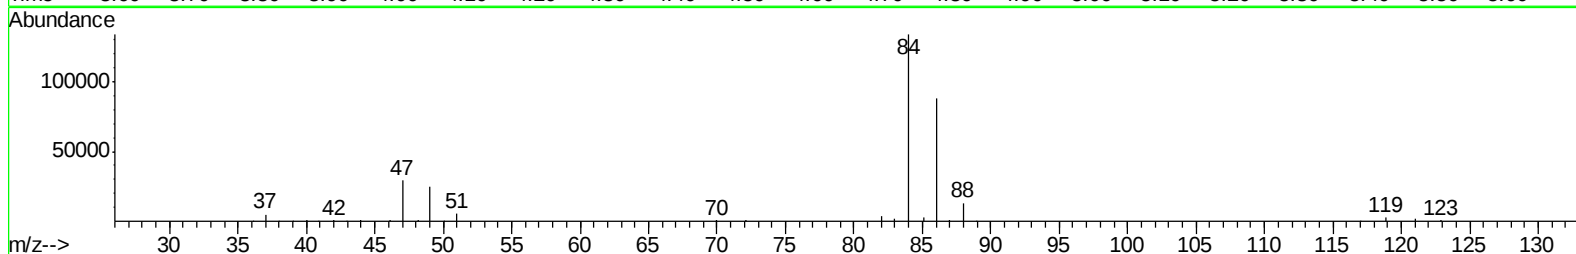


Data File : VU031116.D
Acq On : 12 Apr 2019 09:46
Operator : JC/SP
Sample : VIBLK41
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 108 Sample Multiplier: 1

Quant Time: Apr 12 23:35:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 23:21:49 2019
Response via : Initial Calibration

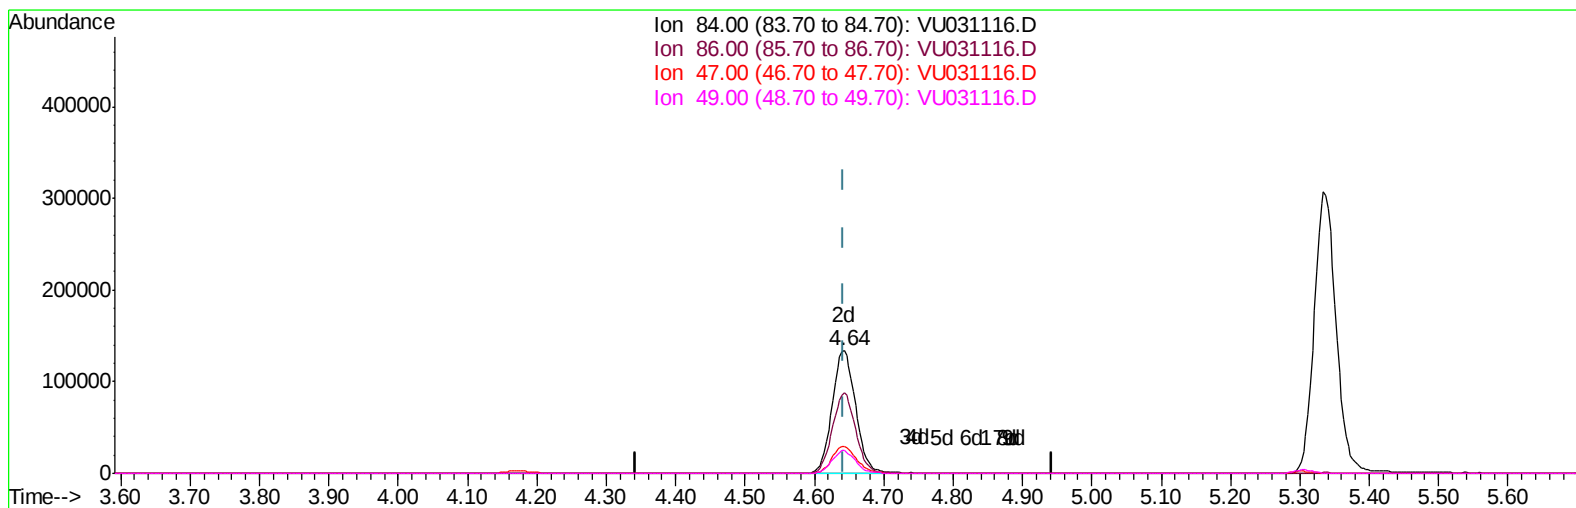

TIC: VU031116.D

(24) Chloroform-d (S)

4.643min (-0.000) 48.77ug/L m

response 312796

Ion	Exp%	Act%
84.00	100	100
86.00	62.90	0.03#
47.00	47.00	0.03#
49.00	26.80	0.01#