
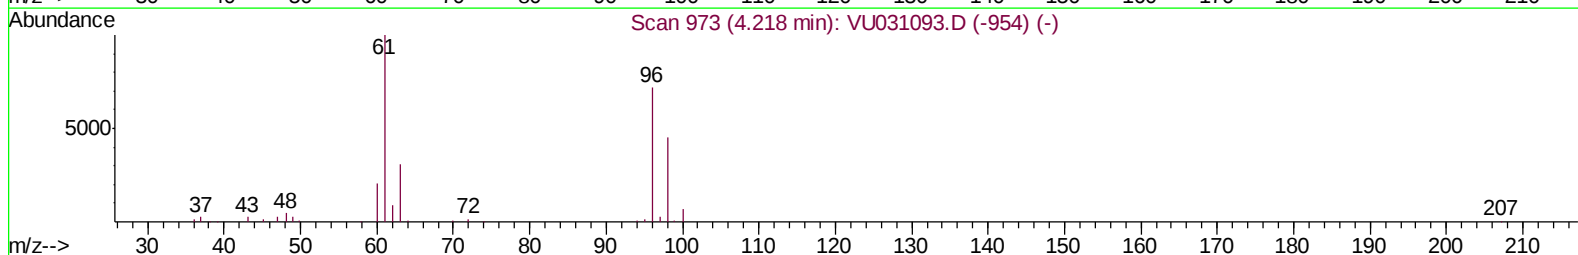
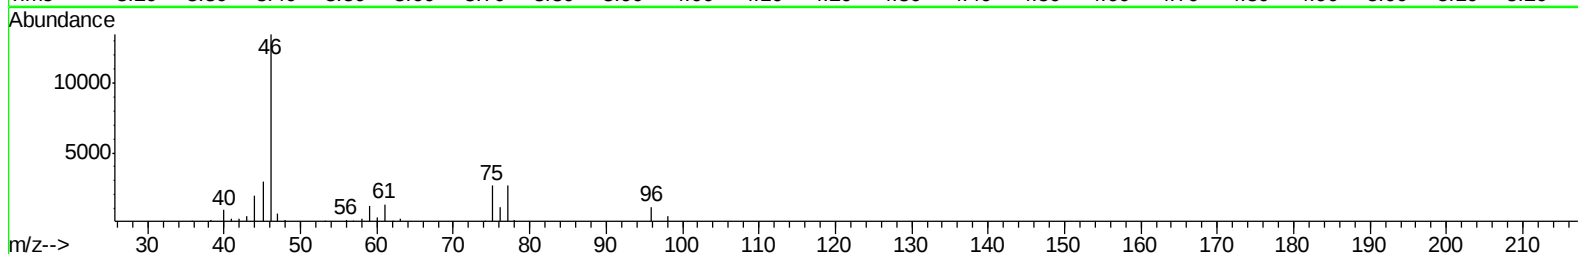


Data File : VU031120.D
Acq On : 12 Apr 2019 11:18
Operator : JC/SP
Sample : K2341-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 112 Sample Multiplier: 1

Quant Time: Apr 12 23:36:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 23:21:49 2019
Response via : Initial Calibration

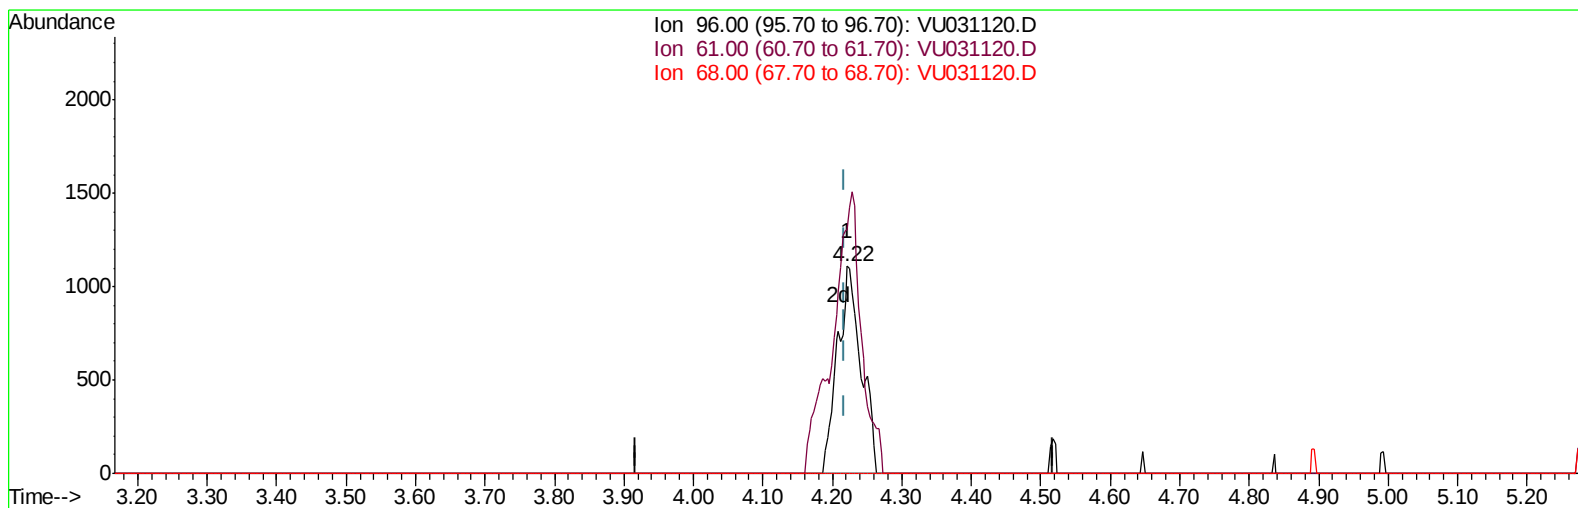

TIC: VU031120.D

(20) cis-1,2-Dichloroethene (T)

4.222min (+0.003) 0.68ug/L m

response 2616

Ion	Exp%	Act%
96.00	100	100
61.00	147.00	117.49
68.00	0.00	0.00
0.00	0.00	0.00