
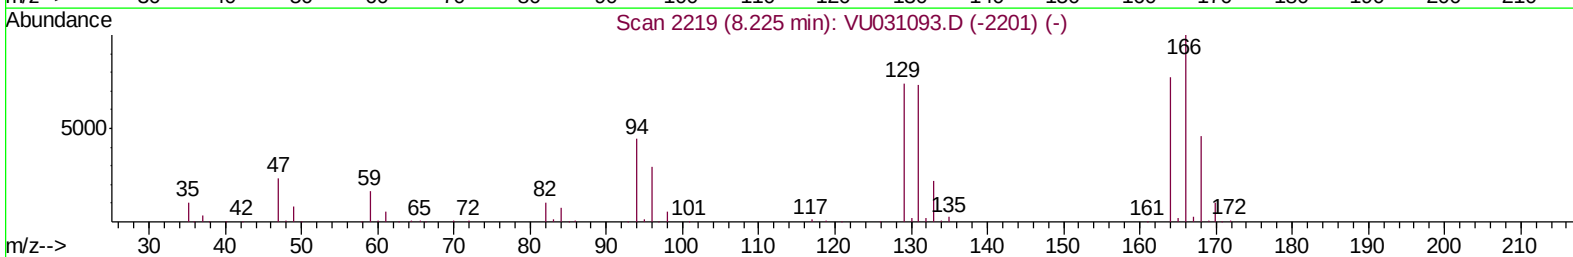
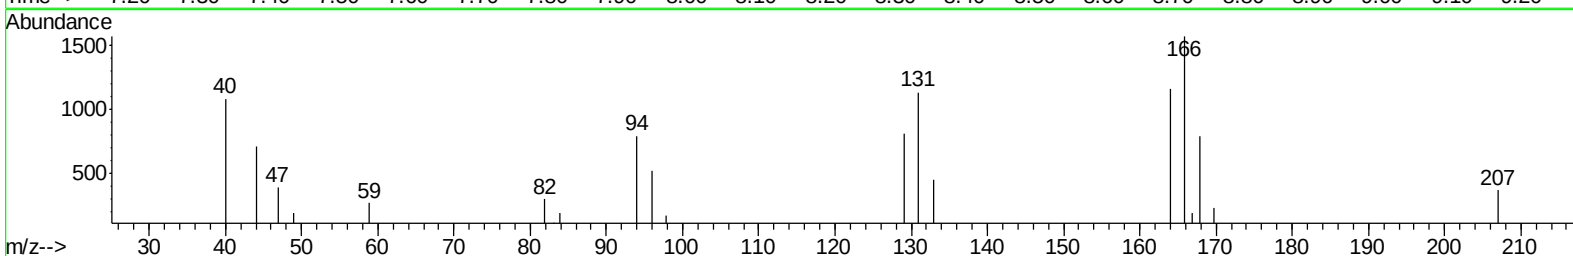


Data File : VU031120.D
Acq On : 12 Apr 2019 11:18
Operator : JC/SP
Sample : K2341-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 112 Sample Multiplier: 1

Quant Time: Apr 12 23:36:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 23:21:49 2019
Response via : Initial Calibration

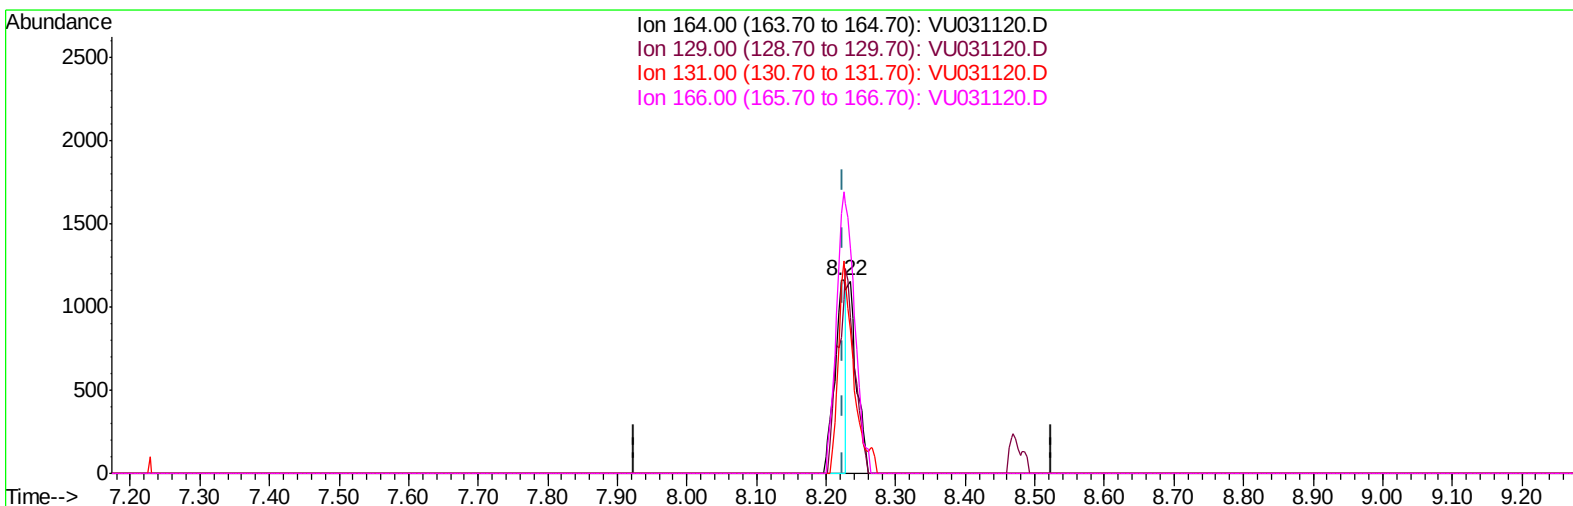

TIC: VU031120.D

(46) Tetrachloroethene (T)

8.222min (-0.003) 0.48ug/L

response 1301

Ion	Exp%	Act%
164.00	100	100
129.00	96.30	70.03
131.00	94.20	97.42
166.00	126.60	134.88