

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031031.D
 Acq On : 10 Apr 2019 23:00
 Operator : JC/SP
 Sample : K2254-22ME
 Misc : 5.45g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC68ME

Quant Time: Apr 11 05:24:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 05:17:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	481470	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	483667	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	246891	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	117124	27.25	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	54.50%#
7) Chloroethane-d5	1.71	69	94	0.03	ug/L	0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	0.06%#
11) 1,1-Dichloroethene-d2	2.24	63	187977	24.18	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	48.36%#
21) 2-Butanone-d5	4.19	46	295330	86.70	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.70%
24) Chloroform-d	4.64	84	232188	35.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	70.74%
26) 1,2-Dichloroethane-d4	5.30	65	172601	38.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.06%
32) Benzene-d6	5.33	84	480014	34.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.00%#
36) 1,2-Dichloropropane-d6	6.32	67	174421	36.05	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	72.10%
41) Toluene-d8	7.56	98	409099	32.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	65.38%#
43) trans-1,3-Dichloropropene-	7.85	79	74650	33.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.66%
47) 2-Hexanone-d5	8.32	63	196921	89.04	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.04%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	279851	42.88	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.76%
64) 1,2-Dichlorobenzene-d4	11.86	152	196532	40.48	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.96%

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
9) Trichlorofluoromethane	1.82	101	3873	0.628	ug/L #	81
15) Methyl Acetate	2.62	43	4959	0.918	ug/L #	79
16) Methylene chloride	2.68	84	2324	0.575	ug/L	91
25) Chloroform	4.67	83	18791	2.564	ug/L	99
29) Cyclohexane	4.96	56	4713	0.684	ug/L #	73
35) Methylcyclohexane	6.40	83	12645	2.111	ug/L	93
39) cis-1,3-Dichloropropene	7.22	75	4309	0.675	ug/L	89
42) Toluene	7.63	91	6443	0.399	ug/L	94
45) 1,1,2-Trichloroethane	8.04	97	2722	0.716	ug/L #	31
52) Ethylbenzene	9.25	91	53531	3.040	ug/L	99
53) m,p-Xylene	9.38	106	15264	2.485	ug/L	95
54) o-xylene	9.78	106	10982	1.798	ug/L	98
56) Isopropylbenzene	10.17	105	17608	1.095	ug/L	94
69) Naphthalene	13.74	128	82354	5.240	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031031.D
Acq On : 10 Apr 2019 23:00
Operator : JC/SP
Sample : K2254-22ME
Misc : 5.45g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC68ME

Quant Time: Apr 11 05:24:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:17:40 2019
Response via : Initial Calibration

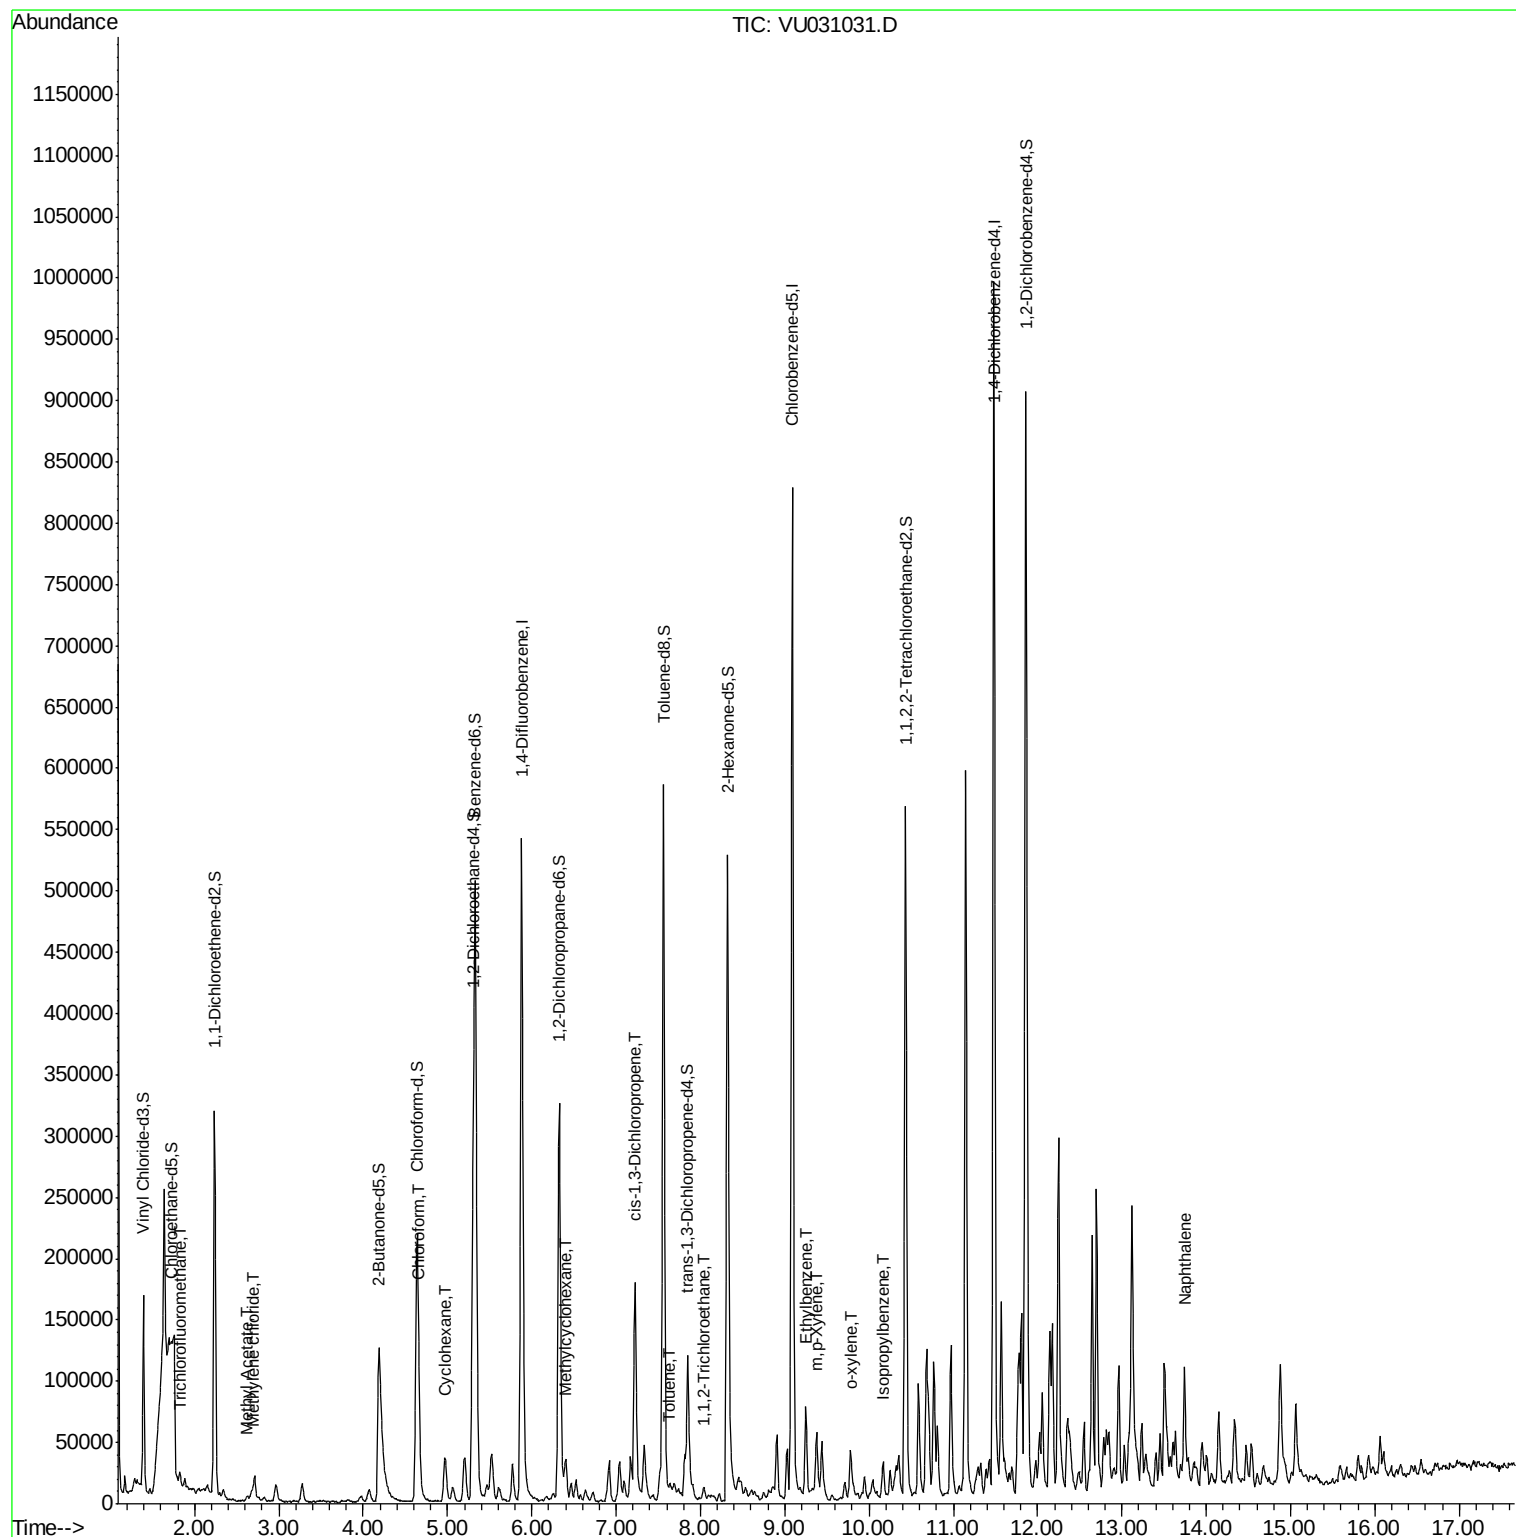

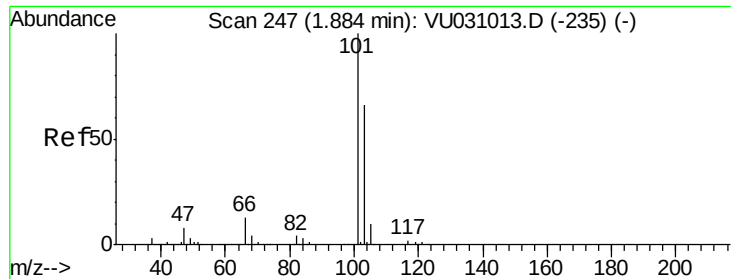

#9

Trichlorofluoromethane

Concen: 0.628 ug/L

RT: 1.82 min Scan# 228

Delta R.T. -0.06 min

Lab File: VU031031.D

Acq: 10 Apr 2019 23:00

Instrument :

MSVOA_U

ClientSampleId :


BFC68ME

Tot Ion:101 Resp: 3873

Ion Ratio Lower Upper




101 100

103 79.5 51.8 77.8#

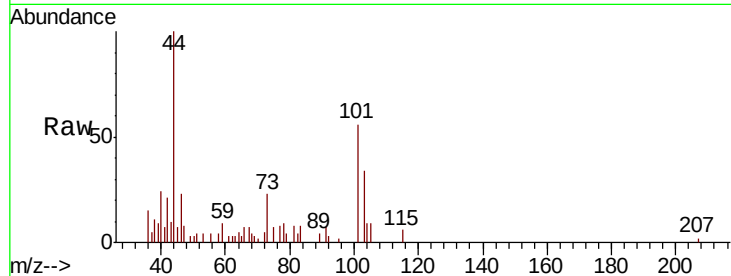

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 103.00 (102.70 to 103.70): V

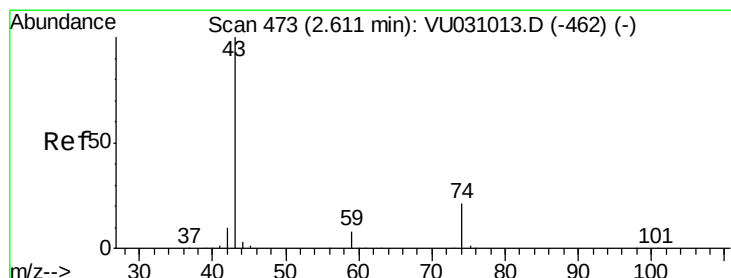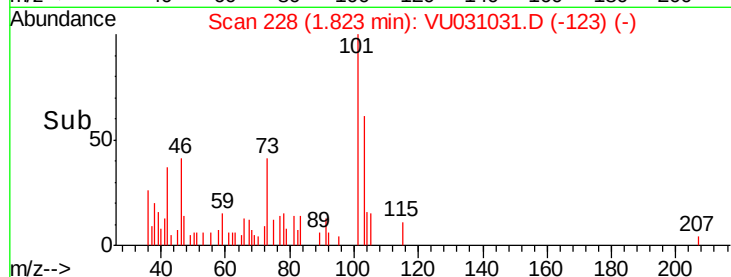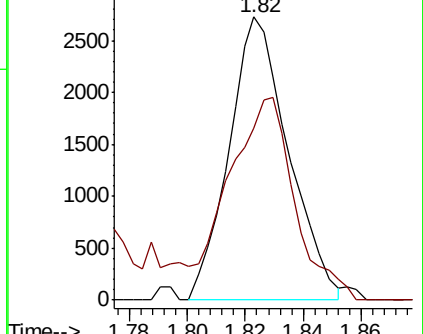

#15

Methyl Acetate

Concen: 0.918 ug/L

RT: 2.62 min Scan# 477

Delta R.T. 0.01 min

Lab File: VU031031.D


Acq: 10 Apr 2019 23:00

Tgt Ion: 43 Resp: 4959

Ion Ratio Lower Upper



43 100


74 11.5 17.1 25.7#

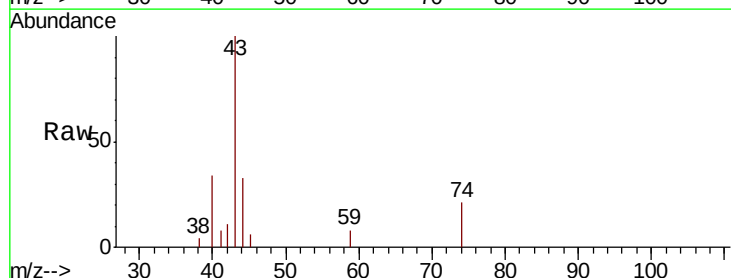

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 74.00 (73.70 to 74.70): VU0



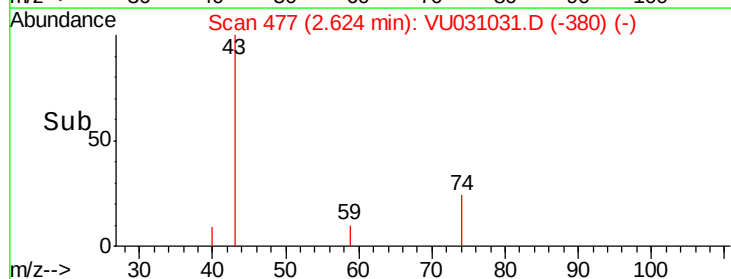
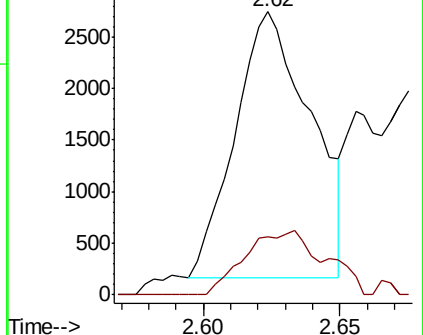


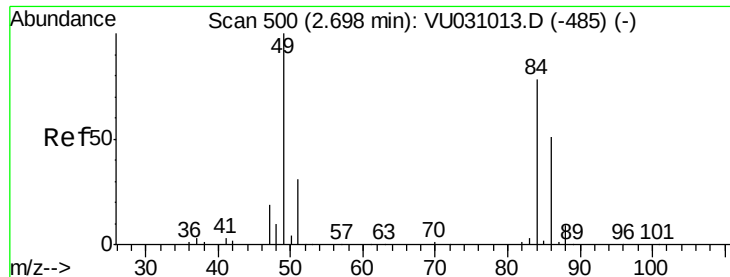

#16
Methvlene chloride
Concen: 0.575 ug/L
RT: 2.68 min Scan# 494
Delta R.T. -0.02 min
Lab File: VU031031.D
Acq: 10 Apr 2019 23:00




Instrument :
MSVOA_U
ClientSampleId :
BFC68ME


Tot Ion: 84 Resp: 2324
Ion Ratio Lower Upper
84 100
86 49.2 45.1 83.7
49 142.7 96.5 179.1

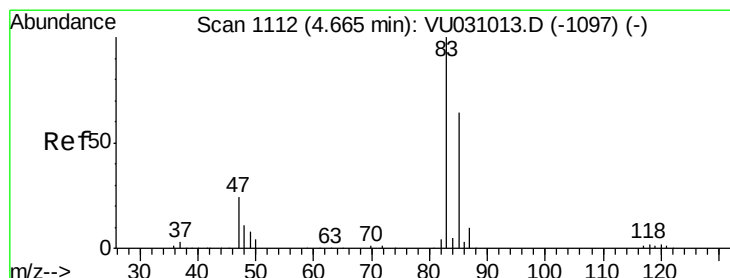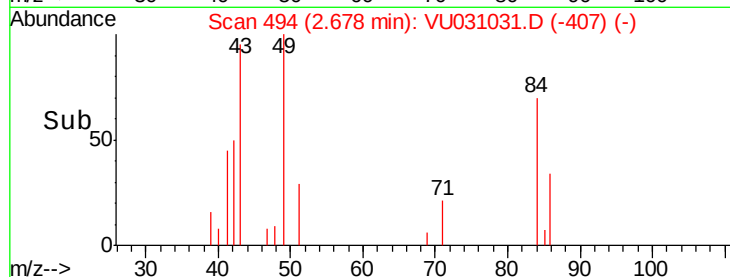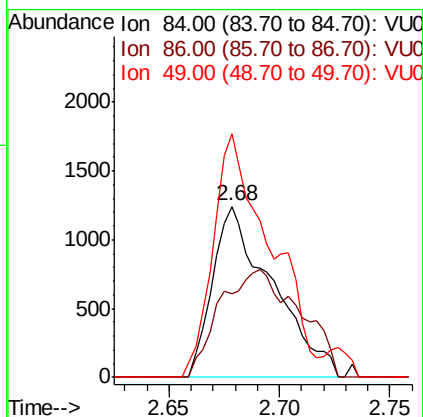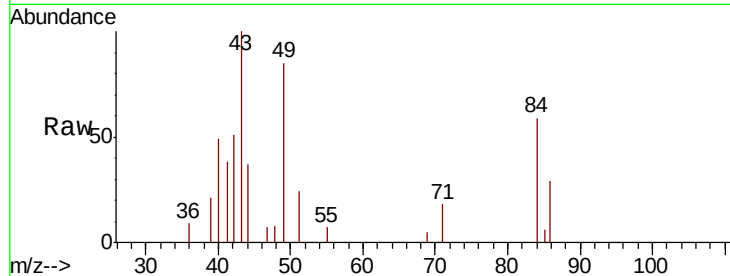

#25
Chloroform
Concen: 2.564 ug/L
RT: 4.67 min Scan# 1113
Delta R.T. 0.00 min
Lab File: VU031031.D
Acq: 10 Apr 2019 23:00

Tgt Ion: 83 Resp: 18791
Ion Ratio Lower Upper
83 100
85 66.2 45.8 85.0


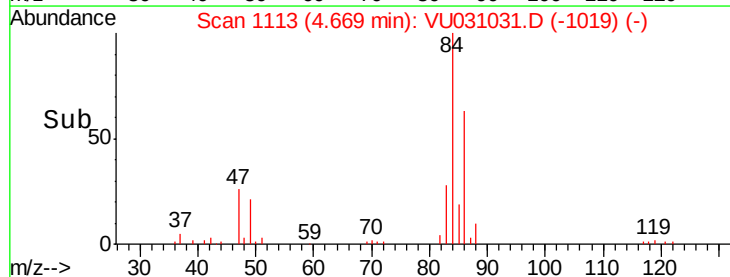
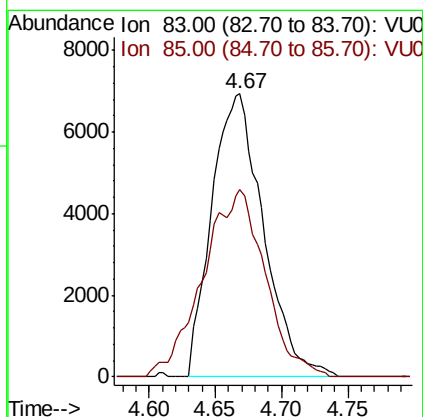
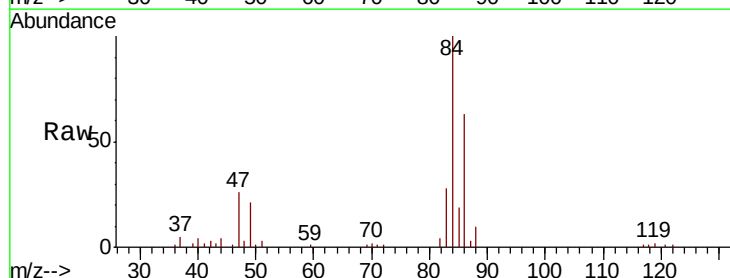


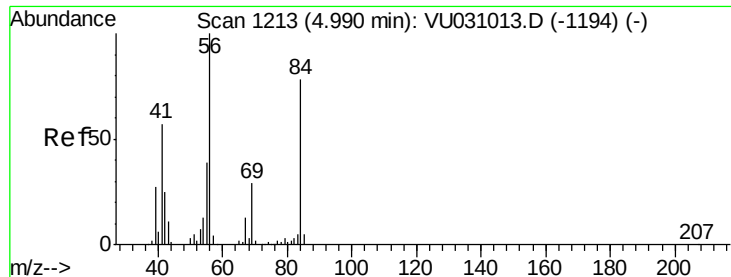

#29
Cyclohexane
Concen: 0.684 ug/L
RT: 4.96 min Scan# 1205
Delta R.T. -0.03 min
Lab File: VU031031.D
Acq: 10 Apr 2019 23:00




Instrument :
MSVOA_U
ClientSampleId :
BFC68ME


Tot Ion: 56 Resp: 4713
Ion Ratio Lower Upper
56 100
69 38.1 22.0 33.0#
84 97.7 58.2 87.2#

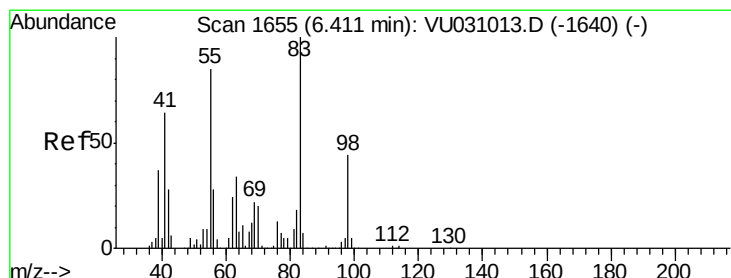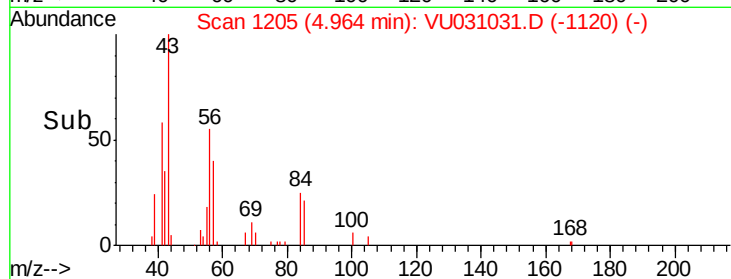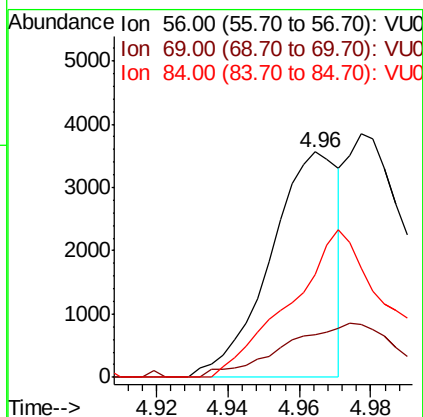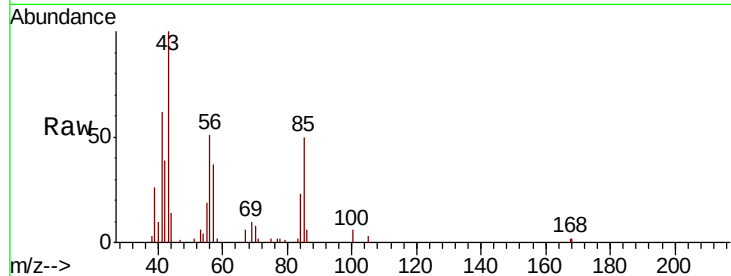

#35
Methylcyclohexane
Concen: 2.111 ug/L
RT: 6.40 min Scan# 1653
Delta R.T. -0.01 min
Lab File: VU031031.D
Acq: 10 Apr 2019 23:00

Tgt Ion: 83 Resp: 12645
Ion Ratio Lower Upper
83 100
55 99.0 71.6 107.4
98 43.3 35.4 53.0


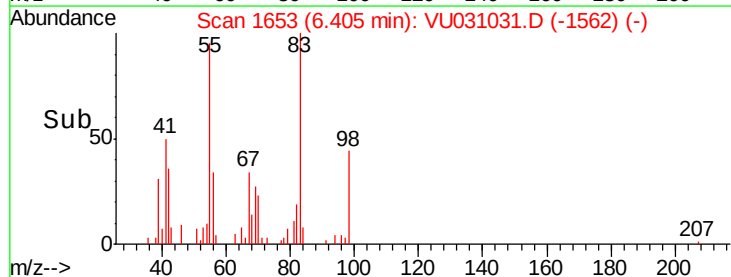
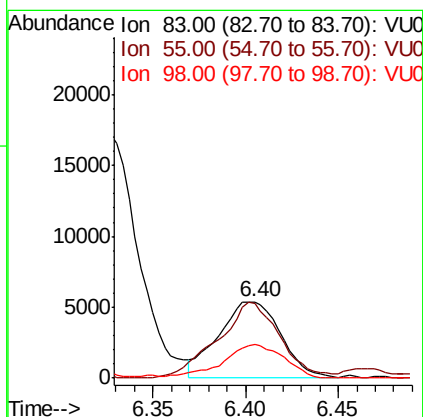
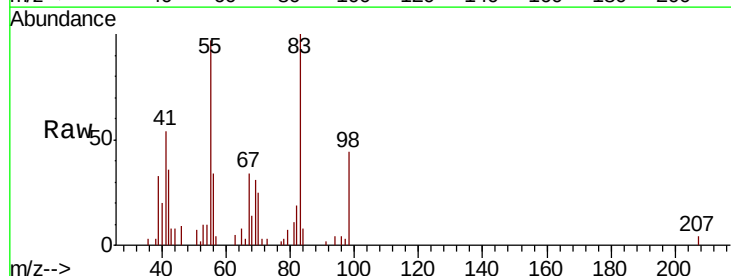


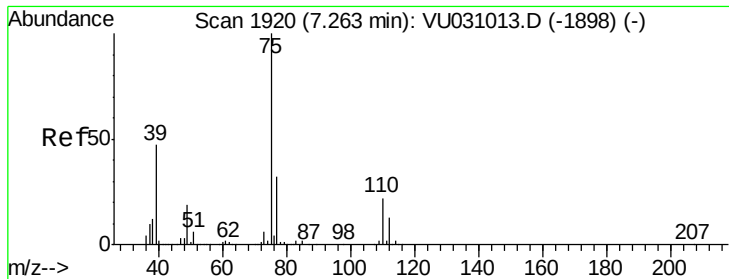

#39
 cis-1,3-Dichloropropene
 Concen: 0.675 ug/L
 RT: 7.22 min Scan# 1908
 Delta R.T. -0.04 min
 Lab File: VU031031.D
 Acq: 10 Apr 2019 23:00




Instrument :
 MSVOA_U
 ClientSampled :
 BFC68ME


Tot Ion: 75 Resp: 4309
 Ion Ratio Lower Upper
 75 100
 77 39.1 23.1 42.9

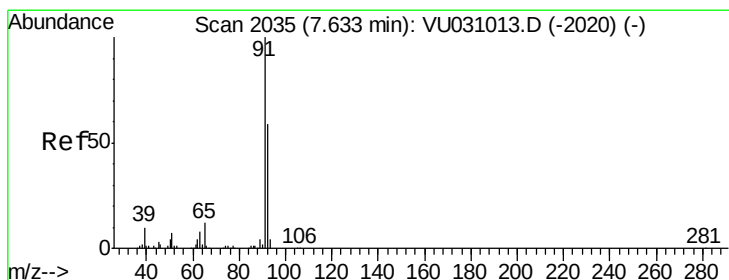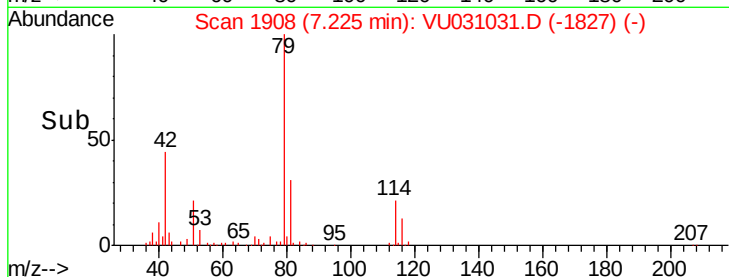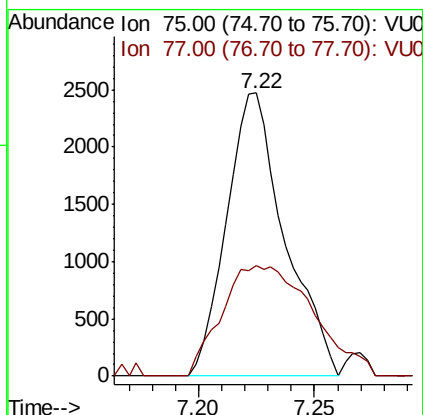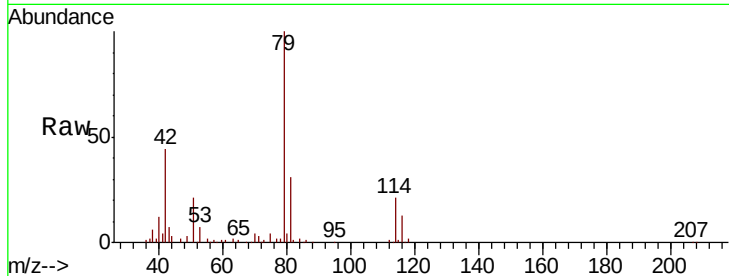

#42
 Toluene
 Concen: 0.399 ug/L
 RT: 7.63 min Scan# 2035
 Delta R.T. -0.00 min
 Lab File: VU031031.D
 Acq: 10 Apr 2019 23:00

Tgt Ion: 91 Resp: 6443
 Ion Ratio Lower Upper
 91 100
 92 53.0 40.0 74.4


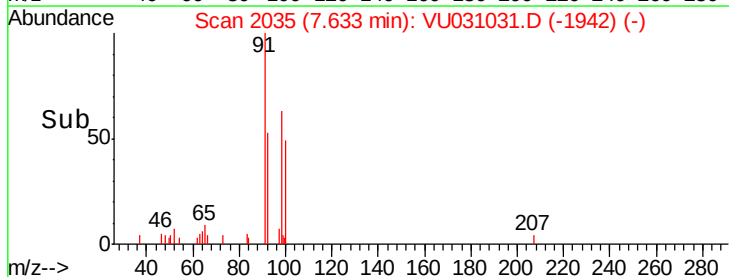
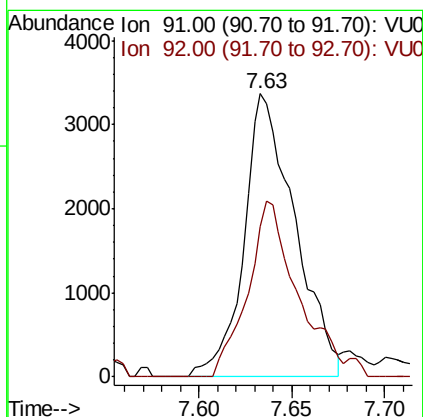
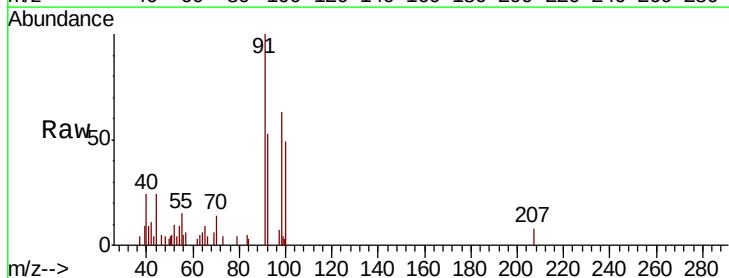


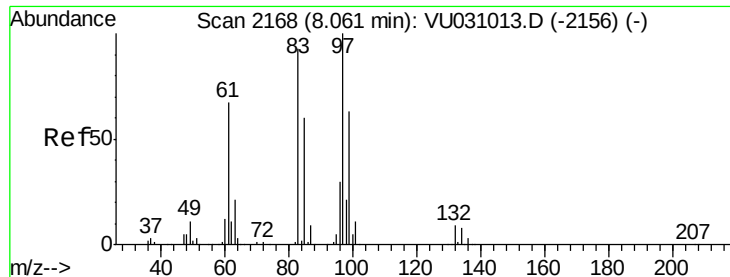

#45
 1,1,2-Trichloroethane
 Concen: 0.716 ug/L
 RT: 8.04 min Scan# 2161
 Delta R.T. -0.02 min
 Lab File: VU031031.D
 Acq: 10 Apr 2019 23:00




Instrument :
 MSVOA_U
 ClientSampleId :
 BFC68ME


Tot Ion: 97 Resp: 2722
 Ion Ratio Lower Upper
 97 100
 99 0.0 44.0 81.8#
 83 19.5 65.3 121.3#
 85 27.4 42.5 78.9#

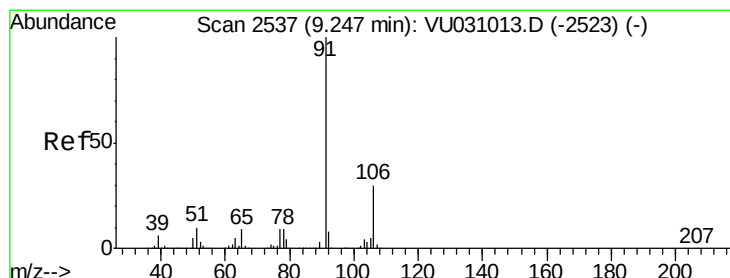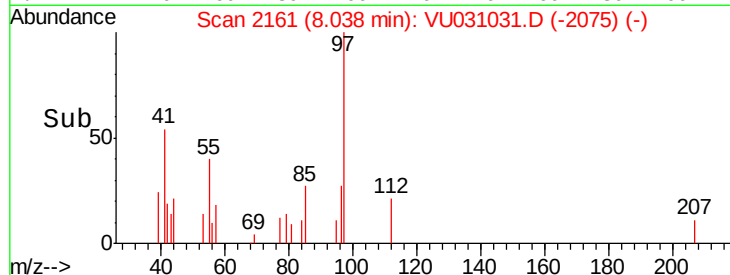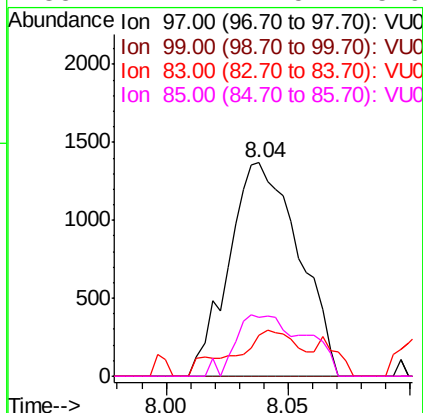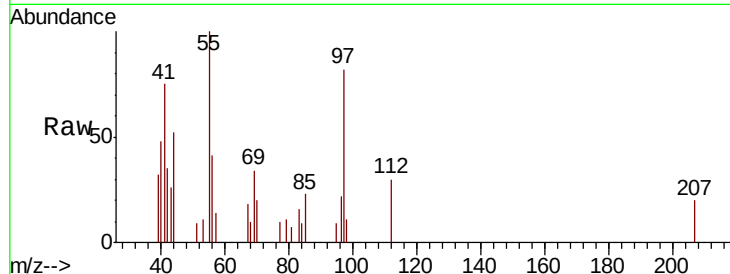

#52
 Ethylbenzene
 Concen: 3.040 ug/L
 RT: 9.25 min Scan# 2538
 Delta R.T. 0.00 min
 Lab File: VU031031.D
 Acq: 10 Apr 2019 23:00

Tgt Ion: 91 Resp: 53531
 Ion Ratio Lower Upper
 91 100
 106 29.8 20.4 37.8

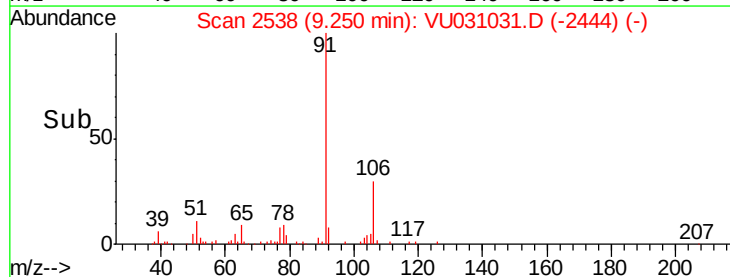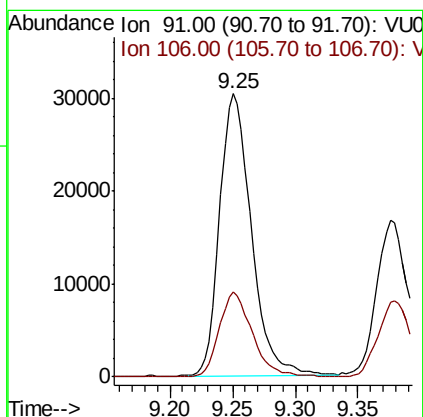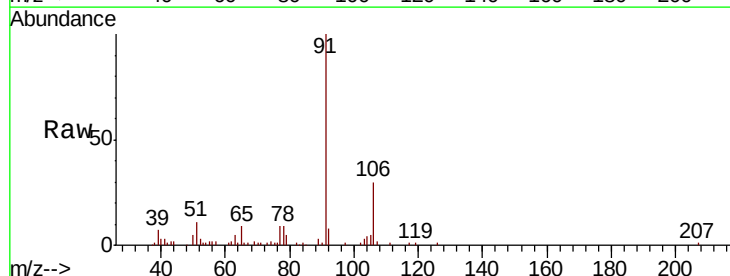

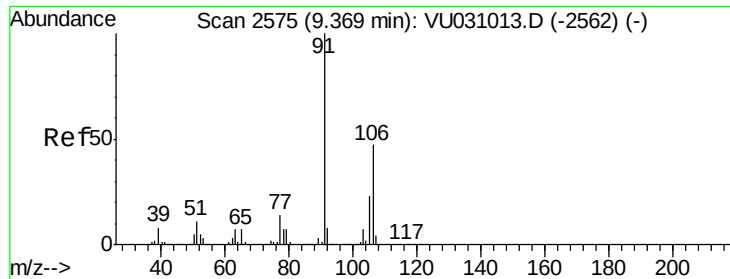

#53

m,p-Xylene

Concen: 2.485 ug/L

RT: 9.38 min Scan# 2578

Delta R.T. 0.01 min

Lab File: VU031031.D

Acq: 10 Apr 2019 23:00

Instrument :

MSVOA_U

ClientSampleId :


BFC68ME

Tot Ion:106 Resp: 15264

Ion Ratio Lower Upper




106 100

91 202.9 148.0 274.8

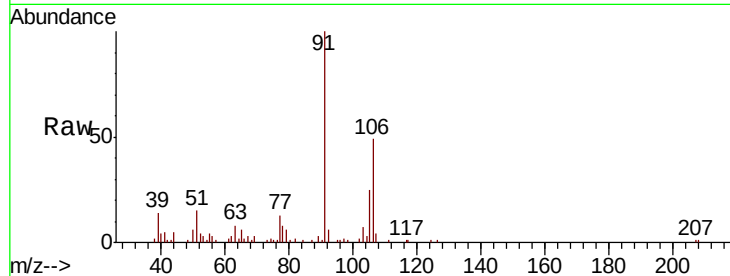

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

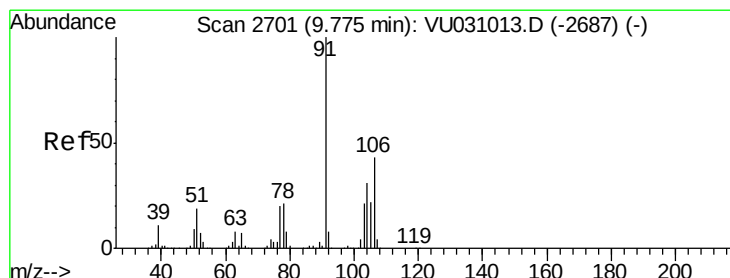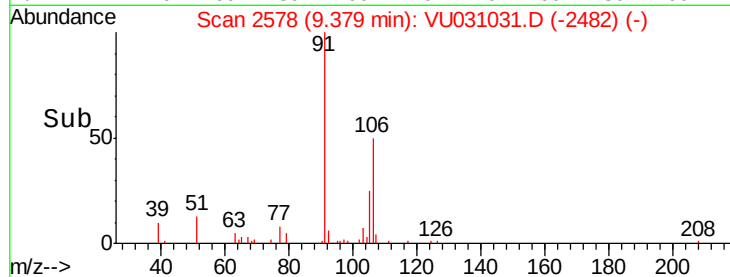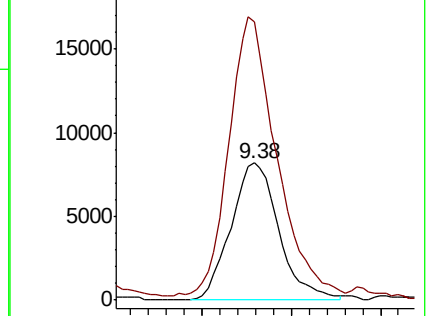

#54

o-xylene

Concen: 1.798 ug/L

RT: 9.78 min Scan# 2703

Delta R.T. 0.01 min

Lab File: VU031031.D


Acq: 10 Apr 2019 23:00

Tgt Ion:106 Resp: 10982

Ion Ratio Lower Upper



106 100


91 221.0 156.7 290.9

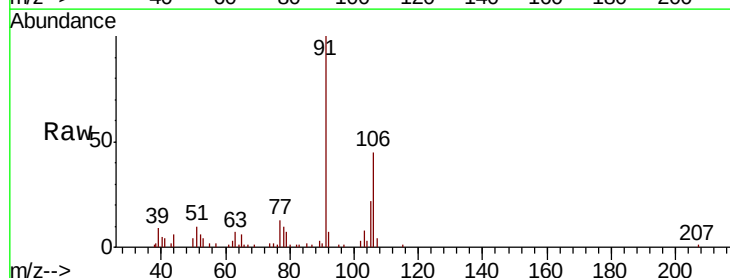

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

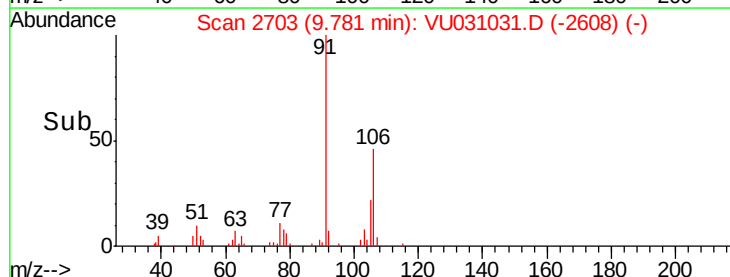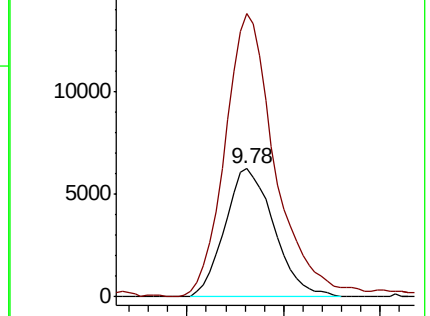

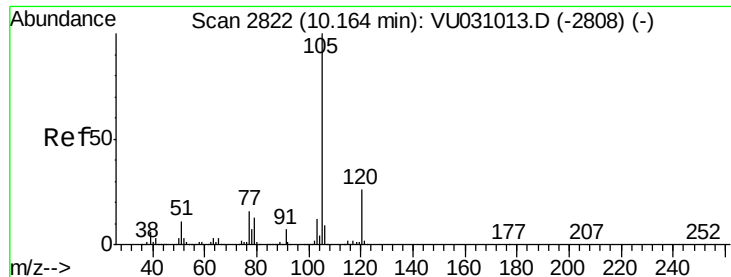

#56

Isopropylbenzene

Concen: 1.095 ug/L

RT: 10.17 min Scan# 2823

Delta R.T. 0.00 min

Lab File: VU031031.D

Acq: 10 Apr 2019 23:00

Instrument :

MSVOA_U

ClientSampleId :

BFC68ME


Tot Ion:105 Resp: 17608

Ion Ratio Lower Upper

105 100

120 27.8 20.4 30.6




77 20.1 13.4 20.2

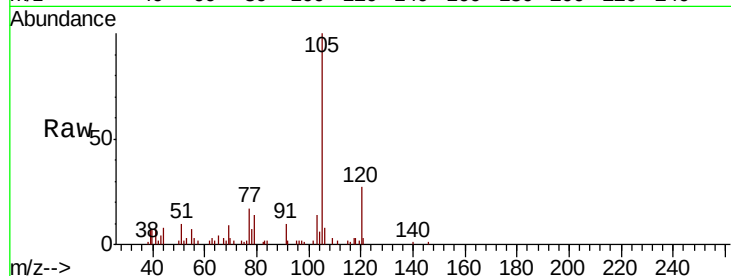

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): V

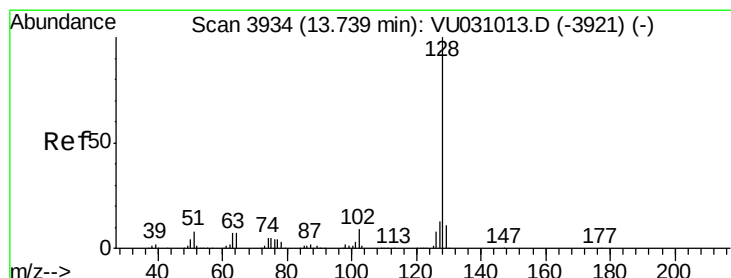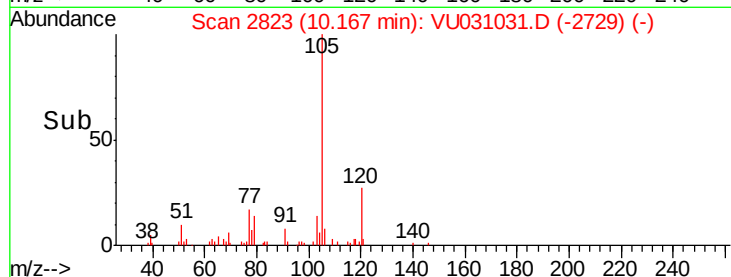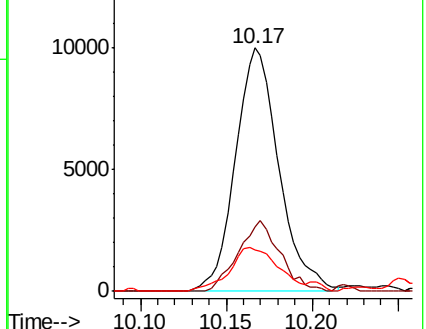

#69

Naphthalene

Concen: 5.240 ug/L

RT: 13.74 min Scan# 3935

Delta R.T. 0.00 min

Lab File: VU031031.D

Acq: 10 Apr 2019 23:00


Tgt Ion:128 Resp: 82354

Ion Ratio Lower Upper

128 100

127 13.5 10.4 15.6

129 10.3 8.6 12.8

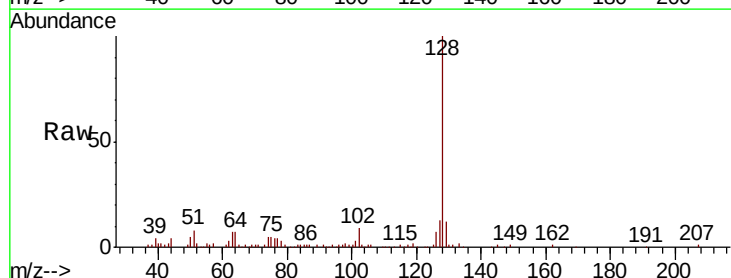

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

