


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031047.D
Acq On : 11 Apr 2019 06:32
Operator : JC/SP
Sample : K2299-27
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
DB707

Manual Integrations
APPROVED

MMDadoda
4/12/2019 5:45:07 PM

Quant Time: Apr 11 08:43:23 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 08:09:01 2019
Response via : Initial Calibration

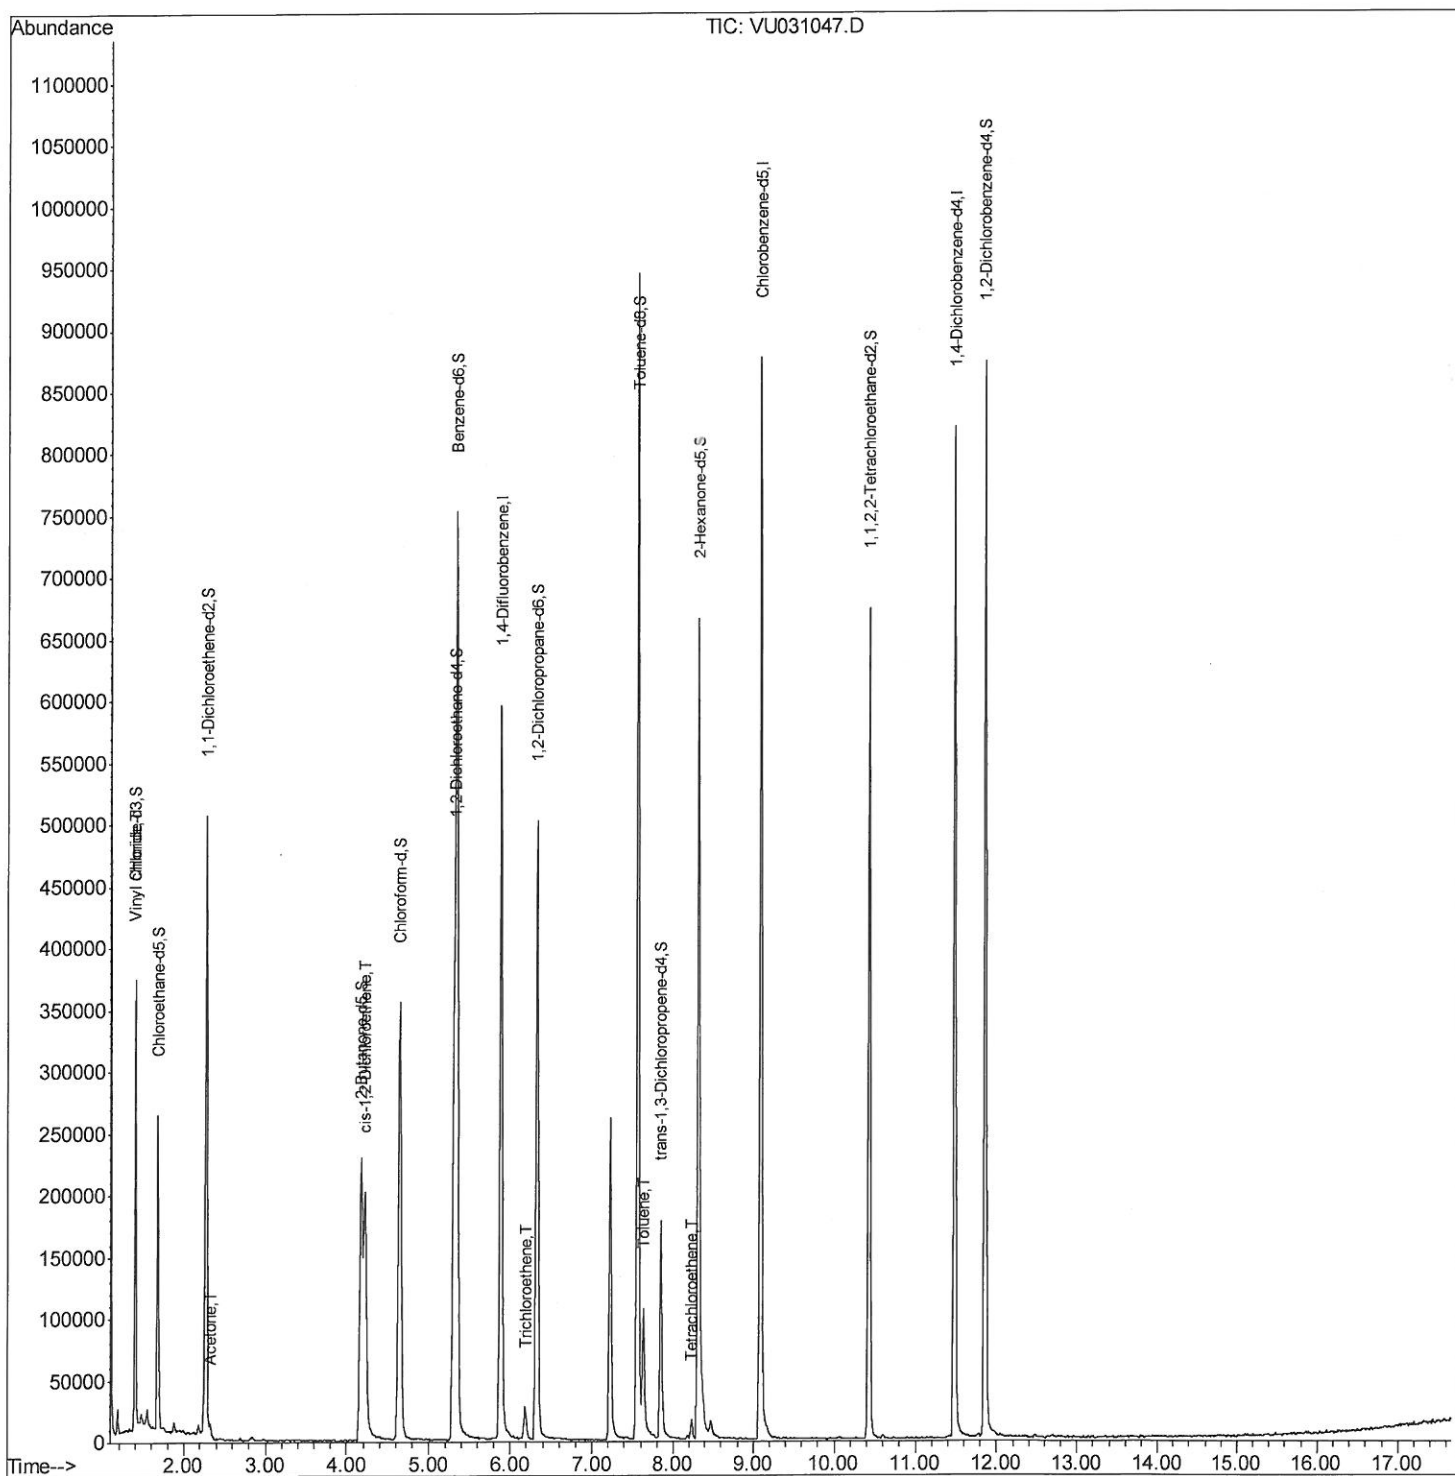

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031047.D
Acq On : 11 Apr 2019 06:32
Operator : JC/SP
Sample : K2299-27
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB707

Manual Integrations
APPROVED

MMDadoda
4/12/2019 5:45:07 PM

Quant Time: Apr 11 08:42:48 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 08:09:01 2019
Response via : Initial Calibration

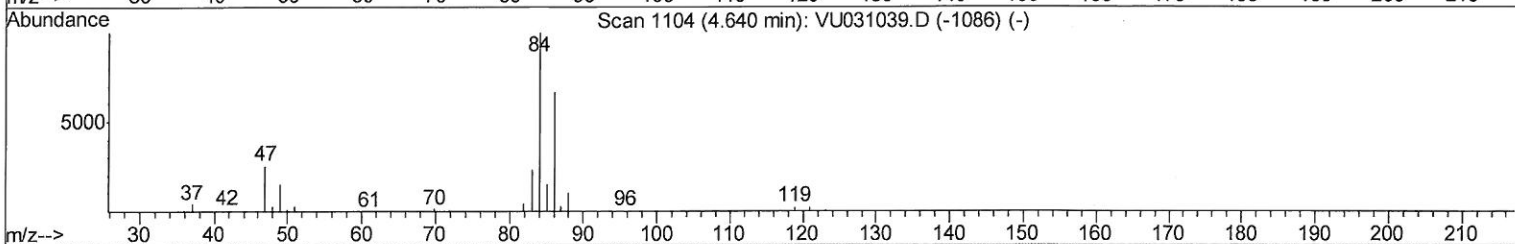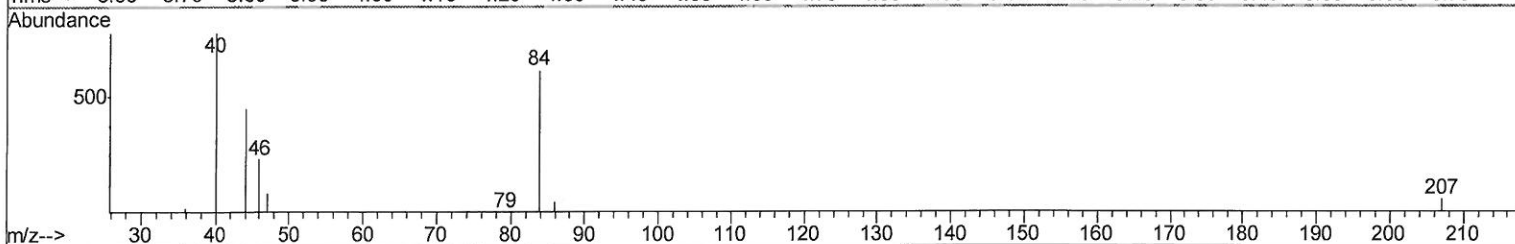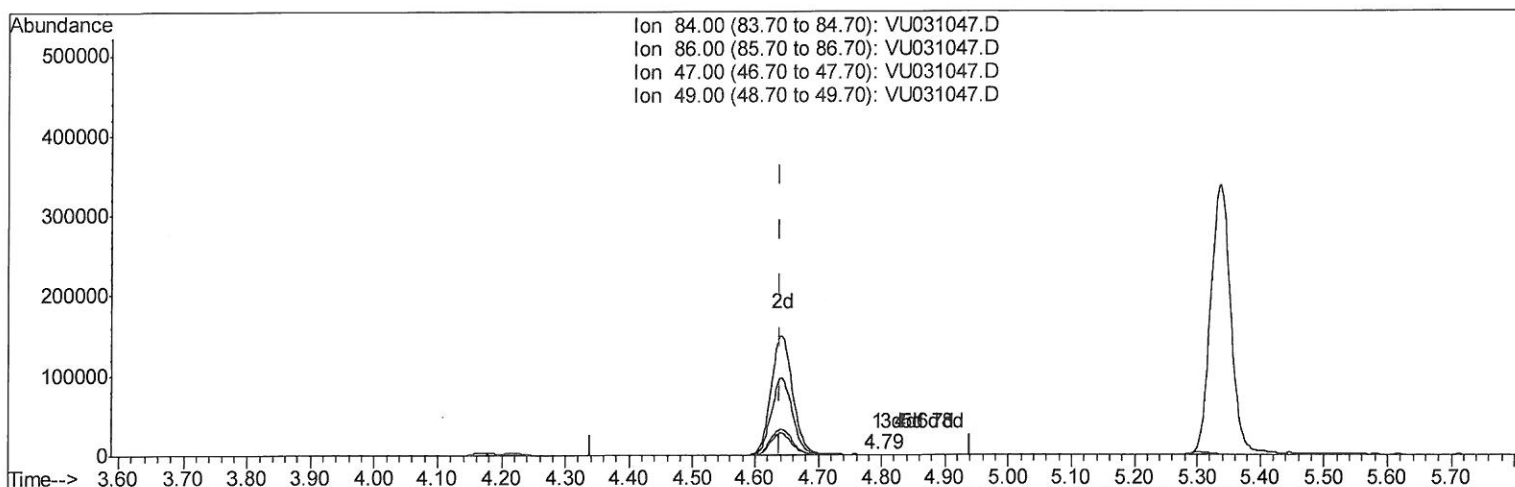

TIC: VU031047.D

(24) Chloroform-d (S)

4.794min (+0.154) 0.04ug/L

response 248

Ion	Exp%	Act%
84.00	100	100
86.00	62.90	68.95
47.00	47.00	46.77
49.00	26.80	29.03

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031047.D
Acq On : 11 Apr 2019 06:32
Operator : JC/SP
Sample : K2299-27
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB707

Manual Integrations
APPROVED

MMDadoda
4/12/2019 5:45:07 PM

Quant Time: Apr 11 08:42:48 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 08:09:01 2019
Response via : Initial Calibration

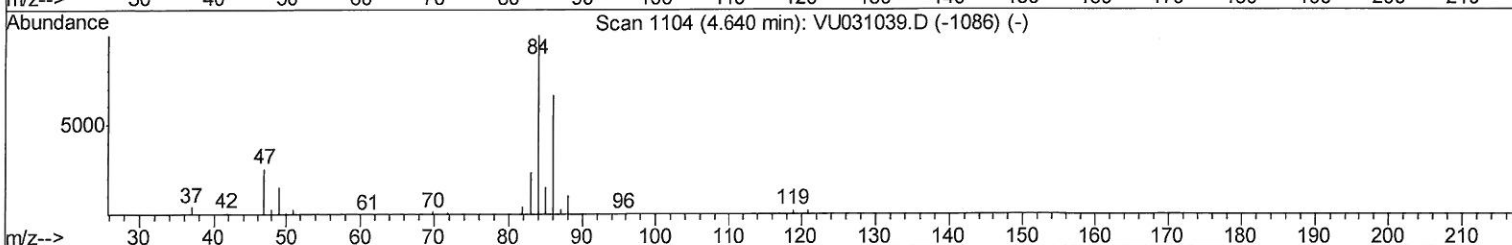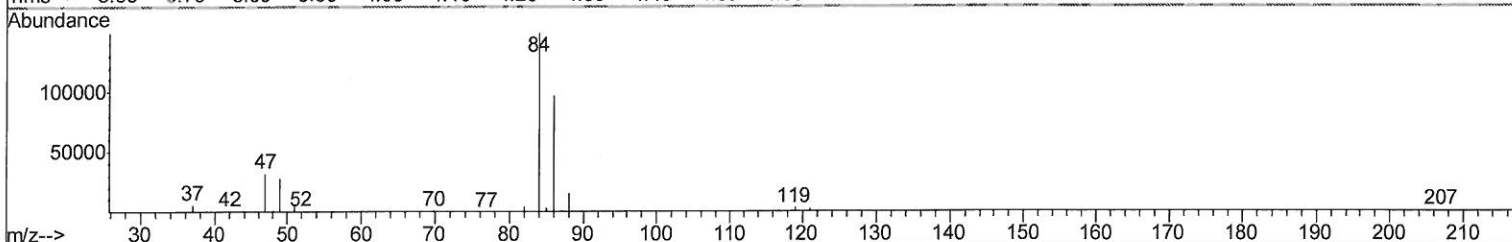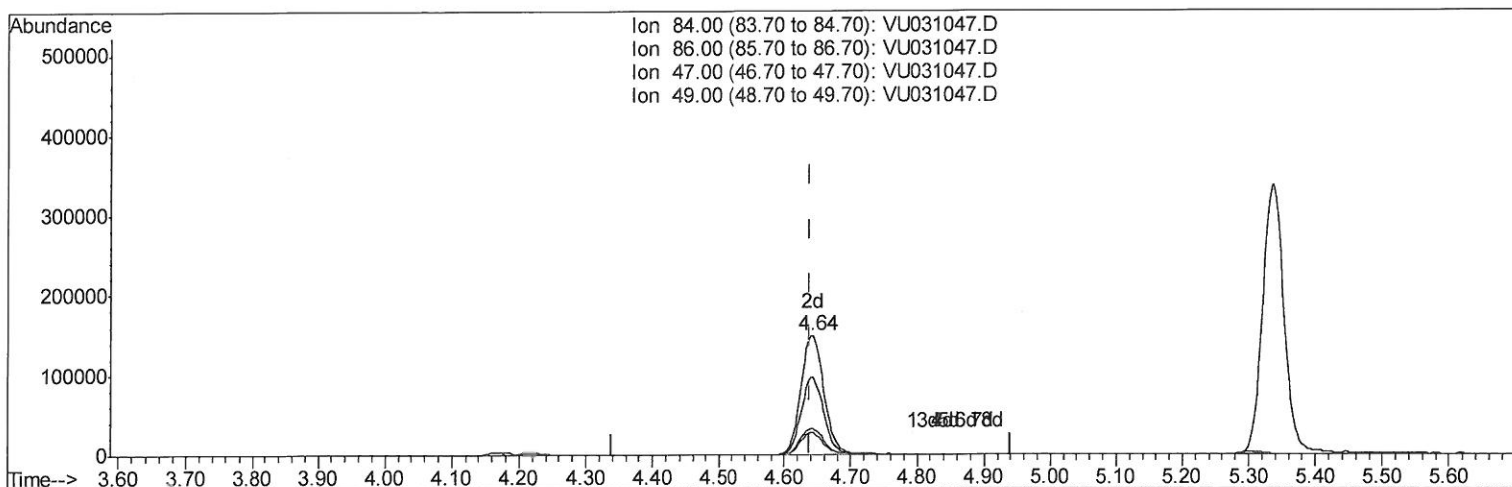

TIC: VU031047.D

(24) Chloroform-d (S)

4.643min (+0.003) 52.41ug/L m

response 356208

Ion	Exp%	Act%
84.00	100	100
86.00	62.90	0.05#
47.00	47.00	0.03#
49.00	26.80	0.02#

→ MD
4/13/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031047.D
 Acq On : 11 Apr 2019 06:32
 Operator : JC/SP
 Sample : K2299-27
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB707

Manual Integrations
 APPROVED

MMDadoda
 4/12/2019 5:45:07 PM

Quant Time: Apr 11 08:43:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 08:09:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	498374	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	495517	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	218451	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	216602	48.69	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.38%
7) Chloroethane-d5	1.68	69	177660	52.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.24%
11) 1,1-Dichloroethene-d2	2.27	63	299297	37.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.40%
21) 2-Butanone-d5	4.17	46	381534	108.21	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.21%
24) Chloroform-d	4.64	84	356208m	52.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.82%
26) 1,2-Dichloroethane-d4	5.31	65	248296	53.54	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.08%
32) Benzene-d6	5.34	84	751218	51.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.86%
36) 1,2-Dichloropropane-d6	6.32	67	257197	51.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.76%
41) Toluene-d8	7.56	98	642096	50.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.16%
43) trans-1,3-Dichloropropene-	7.85	79	107738	47.66	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.32%
47) 2-Hexanone-d5	8.31	63	231942	102.37	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.37%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	352490	52.71	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	105.42%
64) 1,2-Dichlorobenzene-d4	11.85	152	237744	55.34	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.68%

MD
 4/13/19

Target Compounds

					Ovalue	
5) Vinyl chloride	1.40	62	21409	3.906	ug/L	# 61
13) Acetone	2.32	43	9831	2.725	ug/L	97
20) cis-1,2-Dichloroethene	4.22	96	101652	25.168	ug/L	86
34) Trichloroethene	6.19	95	9897	2.488	ug/L	95
42) Toluene	7.63	91	77276	4.669	ug/L	99
46) Tetrachloroethene	8.22	164	4164	1.440	ug/L	# 86

(#) = qualifier out of range (m) = manual integration (+) = signals summed