

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031088.D
 Acq On : 11 Apr 2019 22:43
 Operator : JC/SP
 Sample : K2354-01ME
 Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2T3ME

Quant Time: Apr 12 07:12:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 12 04:43:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	421036	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	421762	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	197074	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	80385	21.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	42.78%#
7) Chloroethane-d5	1.64	69	66273	23.23	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	46.46%#
11) 1,1-Dichloroethene-d2	2.23	63	124466	18.31	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	36.62%#
21) 2-Butanone-d5	4.19	46	167733	56.31	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	56.31%
24) Chloroform-d	4.64	84	154540	26.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	53.84%#
26) 1,2-Dichloroethane-d4	5.30	65	114632	29.26	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	58.52%#
32) Benzene-d6	5.33	84	317213	25.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	51.52%#
36) 1,2-Dichloropropane-d6	6.32	67	111429	26.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	52.82%#
41) Toluene-d8	7.56	98	260406	23.86	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	47.72%#
43) trans-1,3-Dichloropropene-	7.85	79	46871	24.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	48.72%#
47) 2-Hexanone-d5	8.32	63	110314	57.20	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	57.20%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	175209	30.78	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	61.56%#
64) 1,2-Dichlorobenzene-d4	11.86	152	111433	28.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	57.50%#


Target Compounds					Ovalue
46) Tetrachloroethene	8.22	164	28880	11.735 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031088.D
Acq On : 11 Apr 2019 22:43
Operator : JC/SP
Sample : K2354-01ME
Misc : 5.71a/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 79 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2T3ME

Quant Time: Apr 12 07:12:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 12 04:43:47 2019
Response via : Initial Calibration

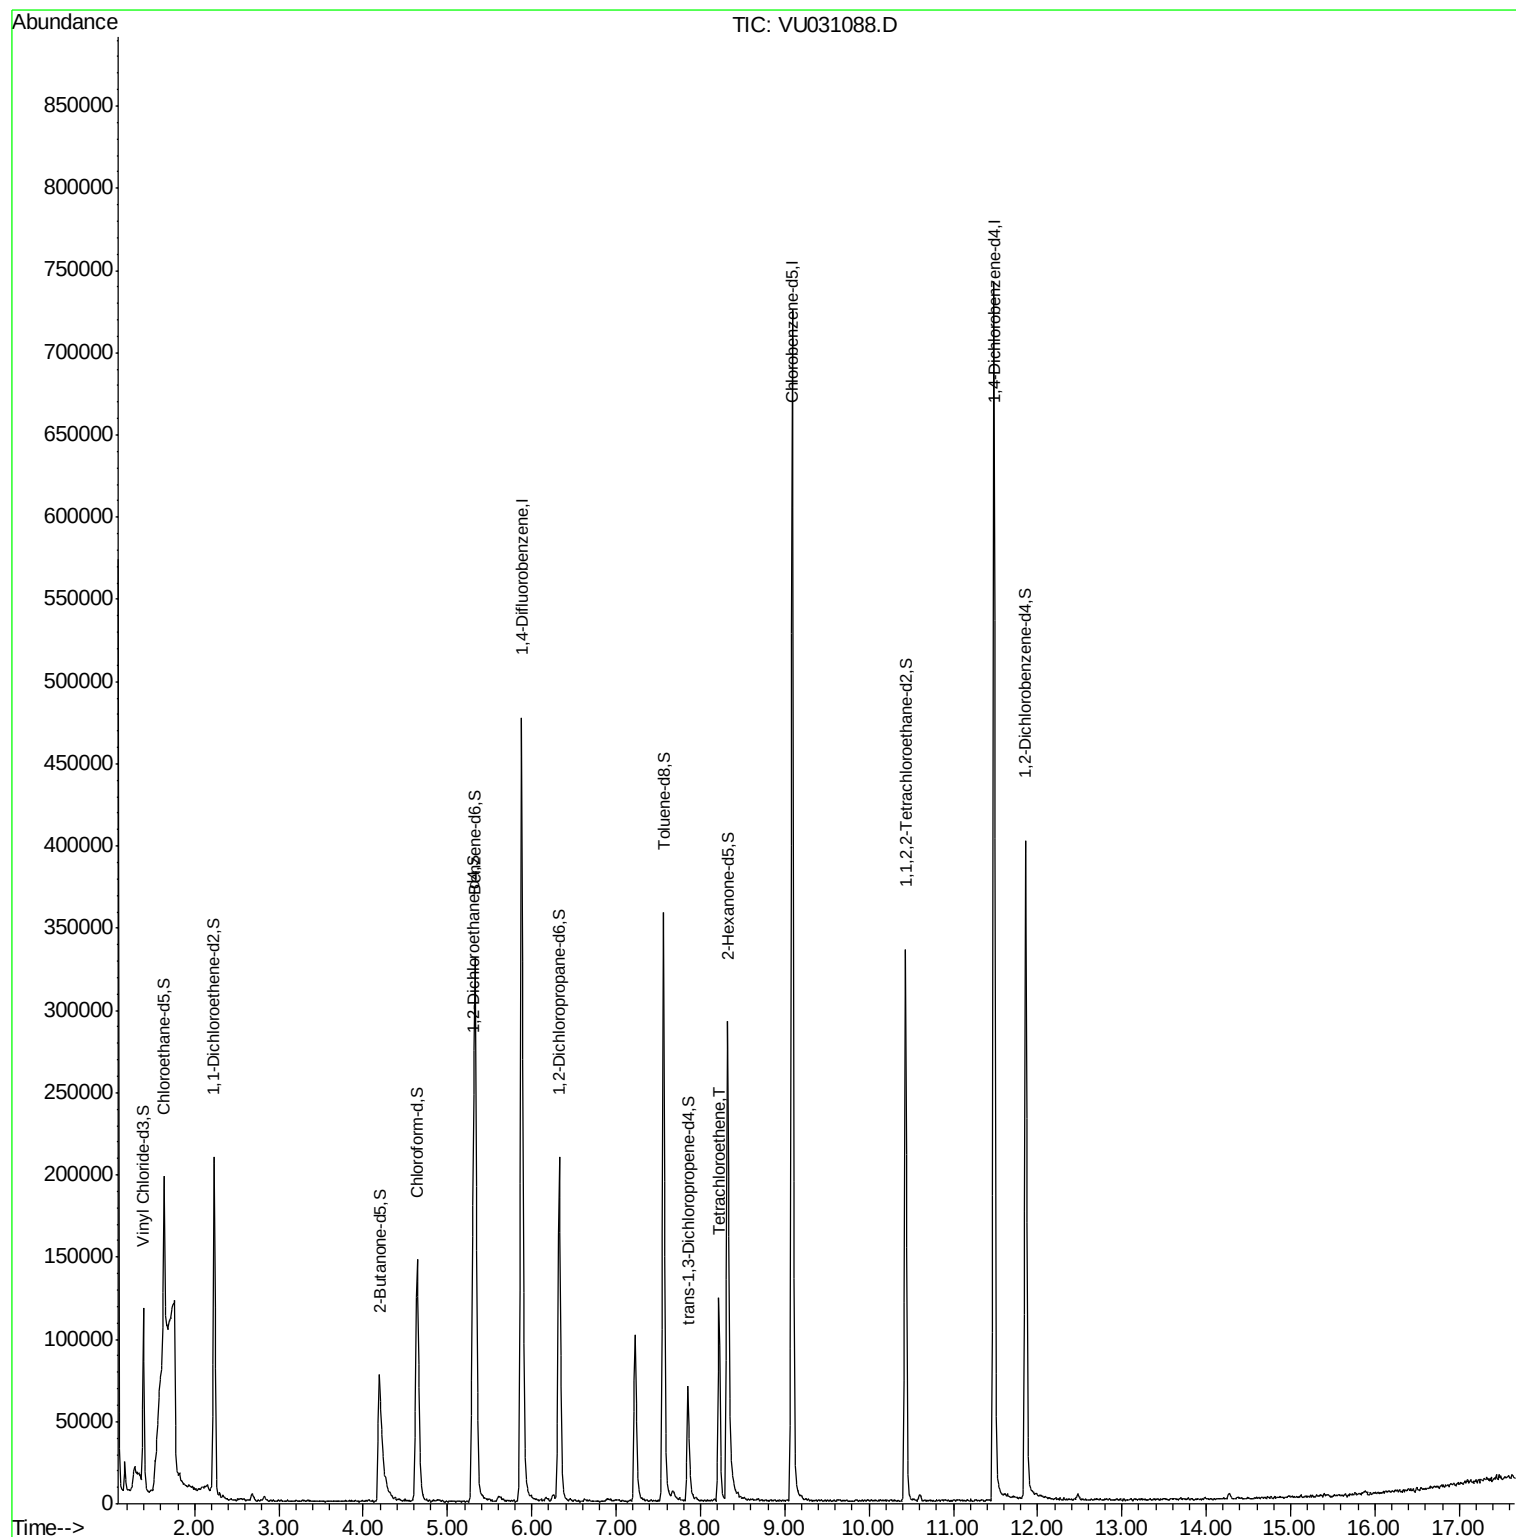

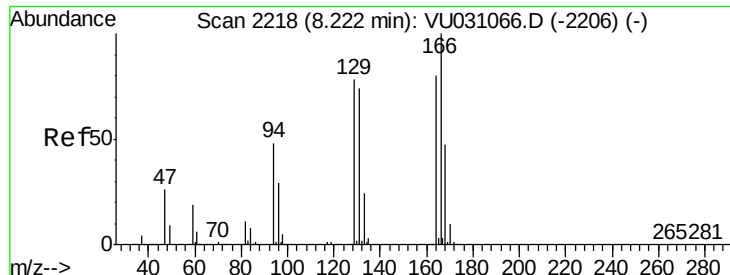

#46

Tetrachloroethene

Concen: 11.735 ug/L

RT: 8.22 min Scan# 2218

Delta R.T. -0.00 min

Lab File: VU031088.D


Acq: 11 Apr 2019 22:43

Instrument :

MSVOA_U

ClientSampleId :

BF2T3ME

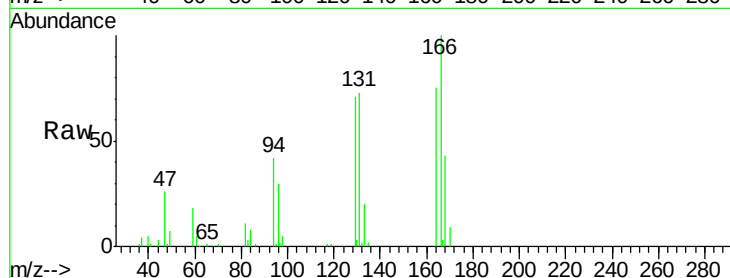

Tot Ion:164 Resp: 28880

Ion Ratio Lower Upper

164 100

129 94.8 67.4 125.2

131 96.8 65.9 122.5

166 132.8 88.6 164.6

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

