

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031018.D
 Acq On : 10 Apr 2019 18:04
 Operator : JC/SP
 Sample : K2249-13DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	36	rVB2	17902	18014	0.83%	0.104%
2	1.396	87	95	108	rBV	339328	361052	16.72%	2.083%
3	1.675	174	182	197	rVB	253483	321951	14.91%	1.857%
4	2.267	355	366	380	rBV2	519163	809300	37.49%	4.669%
5	2.428	411	416	417	rBV3	3172	2343	0.11%	0.014%
6	2.511	440	442	445	rVB4	949	513	0.02%	0.003%
7	2.556	449	456	459	rBV5	909	1013	0.05%	0.006%
8	2.579	461	463	469	rVB5	1142	1085	0.05%	0.006%
9	2.605	469	471	474	rBV2	758	570	0.03%	0.003%
10	2.698	493	500	511	rVV5	4021	5597	0.26%	0.032%
11	2.759	517	519	523	rBV3	781	654	0.03%	0.004%
12	2.814	530	536	538	rBV4	1492	1640	0.08%	0.009%
13	2.974	582	586	590	rBV5	1659	1409	0.07%	0.008%
14	3.048	605	609	611	rBV3	750	580	0.03%	0.003%
15	3.068	613	615	619	rVB	871	481	0.02%	0.003%
16	3.219	656	662	664	rBV4	651	598	0.03%	0.003%
17	3.270	674	678	687	rBV3	472	582	0.03%	0.003%
18	3.363	705	707	713	rBV4	560	551	0.03%	0.003%
19	3.441	717	731	746	rBV	24719	52796	2.45%	0.305%
20	3.611	777	784	787	rBV3	697	900	0.04%	0.005%
21	3.704	807	813	819	rBV4	583	971	0.04%	0.006%
22	3.936	880	885	887	rBV3	580	509	0.02%	0.003%
23	4.170	942	958	969	rBV	217333	563079	26.08%	3.248%
24	4.408	1029	1032	1038	rVB6	1682	1628	0.08%	0.009%
25	4.563	1077	1080	1083	rBV2	723	462	0.02%	0.003%
26	4.640	1088	1104	1136	rVV	344889	851674	39.45%	4.913%
27	4.830	1161	1163	1168	rBV3	679	497	0.02%	0.003%
28	4.910	1170	1188	1209	rBV	542426	1320172	61.15%	7.616%
29	5.058	1233	1234	1237	rVB3	1472	562	0.03%	0.003%
30	5.103	1246	1248	1251	rBV3	589	470	0.02%	0.003%
31	5.177	1268	1271	1273	rBV4	970	723	0.03%	0.004%
32	5.215	1279	1283	1286	rBV3	1138	1018	0.05%	0.006%
33	5.334	1295	1320	1341	rBV2	730212	2158971	100.00%	12.455%
34	5.881	1477	1490	1522	rBV	552114	1117433	51.76%	6.447%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031018.D
 Acq On : 10 Apr 2019 18:04
 Operator : JC/SP
 Sample : K2249-13DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.100	1555	1558	1559	rBV2	1150	719	0.03%	0.004%
36	6.190	1575	1586	1599	rVB7	16057	36304	1.68%	0.209%
37	6.325	1612	1628	1653	rBV	480797	979368	45.36%	5.650%
38	6.617	1714	1719	1724	rVB6	1164	1069	0.05%	0.006%
39	6.698	1742	1744	1751	rVB4	1006	987	0.05%	0.006%
40	6.772	1763	1767	1771	rBV3	1080	807	0.04%	0.005%
41	6.833	1784	1786	1789	rBV2	814	554	0.03%	0.003%
42	7.042	1845	1851	1853	rBV3	798	673	0.03%	0.004%
43	7.103	1867	1870	1873	rBV2	650	439	0.02%	0.003%
44	7.225	1895	1908	1927	rBV	251563	469614	21.75%	2.709%
45	7.431	1969	1972	1976	rVB4	935	715	0.03%	0.004%
46	7.559	1999	2012	2032	rBV	903571	1613853	74.75%	9.310%
47	7.846	2088	2101	2124	rBV	176662	324691	15.04%	1.873%
48	8.071	2166	2171	2180	rVB8	3163	4312	0.20%	0.025%
49	8.157	2195	2198	2199	rBV3	777	551	0.03%	0.003%
50	8.173	2199	2203	2206	rVV	1975	1762	0.08%	0.010%
51	8.225	2208	2219	2234	rVV2	66213	111376	5.16%	0.643%
52	8.309	2234	2245	2289	rBV	625850	1231911	57.06%	7.107%
53	8.794	2392	2396	2398	rBV3	628	493	0.02%	0.003%
54	8.964	2446	2449	2451	rBV3	1266	676	0.03%	0.004%
55	9.006	2459	2462	2463	rBV2	891	462	0.02%	0.003%
56	9.087	2474	2487	2522	rBV	822615	1418751	65.71%	8.185%
57	9.289	2547	2550	2556	rVB5	823	819	0.04%	0.005%
58	9.328	2560	2562	2564	rVV2	859	483	0.02%	0.003%
59	9.405	2579	2586	2590	rBV5	948	1097	0.05%	0.006%
60	9.424	2590	2592	2594	rBV3	893	533	0.02%	0.003%
61	9.582	2637	2641	2645	rBV3	828	816	0.04%	0.005%
62	9.714	2678	2682	2687	rBV4	731	710	0.03%	0.004%
63	9.739	2687	2690	2695	rVB3	763	671	0.03%	0.004%
64	9.778	2695	2702	2704	rBV2	786	791	0.04%	0.005%
65	9.845	2719	2723	2725	rBV3	614	480	0.02%	0.003%
66	9.987	2765	2767	2774	rVB2	671	645	0.03%	0.004%
67	10.106	2800	2804	2809	rVB3	667	530	0.02%	0.003%
68	10.257	2848	2851	2857	rBV3	977	769	0.04%	0.004%
69	10.292	2857	2862	2864	rBV3	793	687	0.03%	0.004%
70	10.427	2890	2904	2929	rBV	643964	1065302	49.34%	6.146%
71	10.540	2936	2939	2942	rBV2	823	520	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031018.D
 Acq On : 10 Apr 2019 18:04
 Operator : JC/SP
 Sample : K2249-13DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YE3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.733	2997	2999	3005	rVB4	788	736	0.03%	0.004%
73	10.942	3060	3064	3066	rBV2	561	575	0.03%	0.003%
74	10.977	3073	3075	3080	rVB	634	454	0.02%	0.003%
75	11.045	3093	3096	3097	rBV	724	444	0.02%	0.003%
76	11.083	3102	3108	3109	rBV2	1019	944	0.04%	0.005%
77	11.180	3134	3138	3139	rBV	741	485	0.02%	0.003%
78	11.386	3199	3202	3208	rVB3	641	447	0.02%	0.003%
79	11.482	3219	3232	3254	rBV	689317	1144734	53.02%	6.604%
80	11.855	3336	3348	3381	rBV	766981	1293551	59.92%	7.463%
81	12.273	3475	3478	3481	rVB3	910	666	0.03%	0.004%
82	12.389	3510	3514	3516	rBV3	962	844	0.04%	0.005%
83	12.405	3516	3519	3521	rVB	826	443	0.02%	0.003%
84	12.614	3581	3584	3586	rBV2	1053	616	0.03%	0.004%
85	12.678	3598	3604	3611	rBV6	1067	1584	0.07%	0.009%
86	12.958	3686	3691	3693	rBV2	965	945	0.04%	0.005%
87	13.038	3713	3716	3721	rVB2	1168	881	0.04%	0.005%
88	13.099	3733	3735	3741	rVB3	1241	1043	0.05%	0.006%
89	13.170	3754	3757	3760	rVB3	936	489	0.02%	0.003%
90	13.421	3831	3835	3836	rBV2	1297	934	0.04%	0.005%
91	13.717	3924	3927	3929	rVB2	1038	534	0.02%	0.003%
92	13.990	4009	4012	4013	rBV2	1039	514	0.02%	0.003%
93	14.022	4019	4022	4026	rVB5	1615	1173	0.05%	0.007%
94	14.083	4039	4041	4046	rVB4	1186	746	0.03%	0.004%
95	14.154	4061	4063	4066	rBV2	927	607	0.03%	0.004%
96	14.218	4081	4083	4086	rBV	750	524	0.02%	0.003%
97	14.511	4171	4174	4176	rBV3	690	548	0.03%	0.003%
98	14.836	4271	4275	4277	rBV3	1050	835	0.04%	0.005%
99	14.926	4297	4303	4307	rBV6	1195	1857	0.09%	0.011%
100	15.328	4425	4428	4431	rBV3	968	832	0.04%	0.005%


Sum of corrected areas: 17333723

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031018.D
Acq On : 10 Apr 2019 18:04
Operator : JC/SP
Sample : K2249-13DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

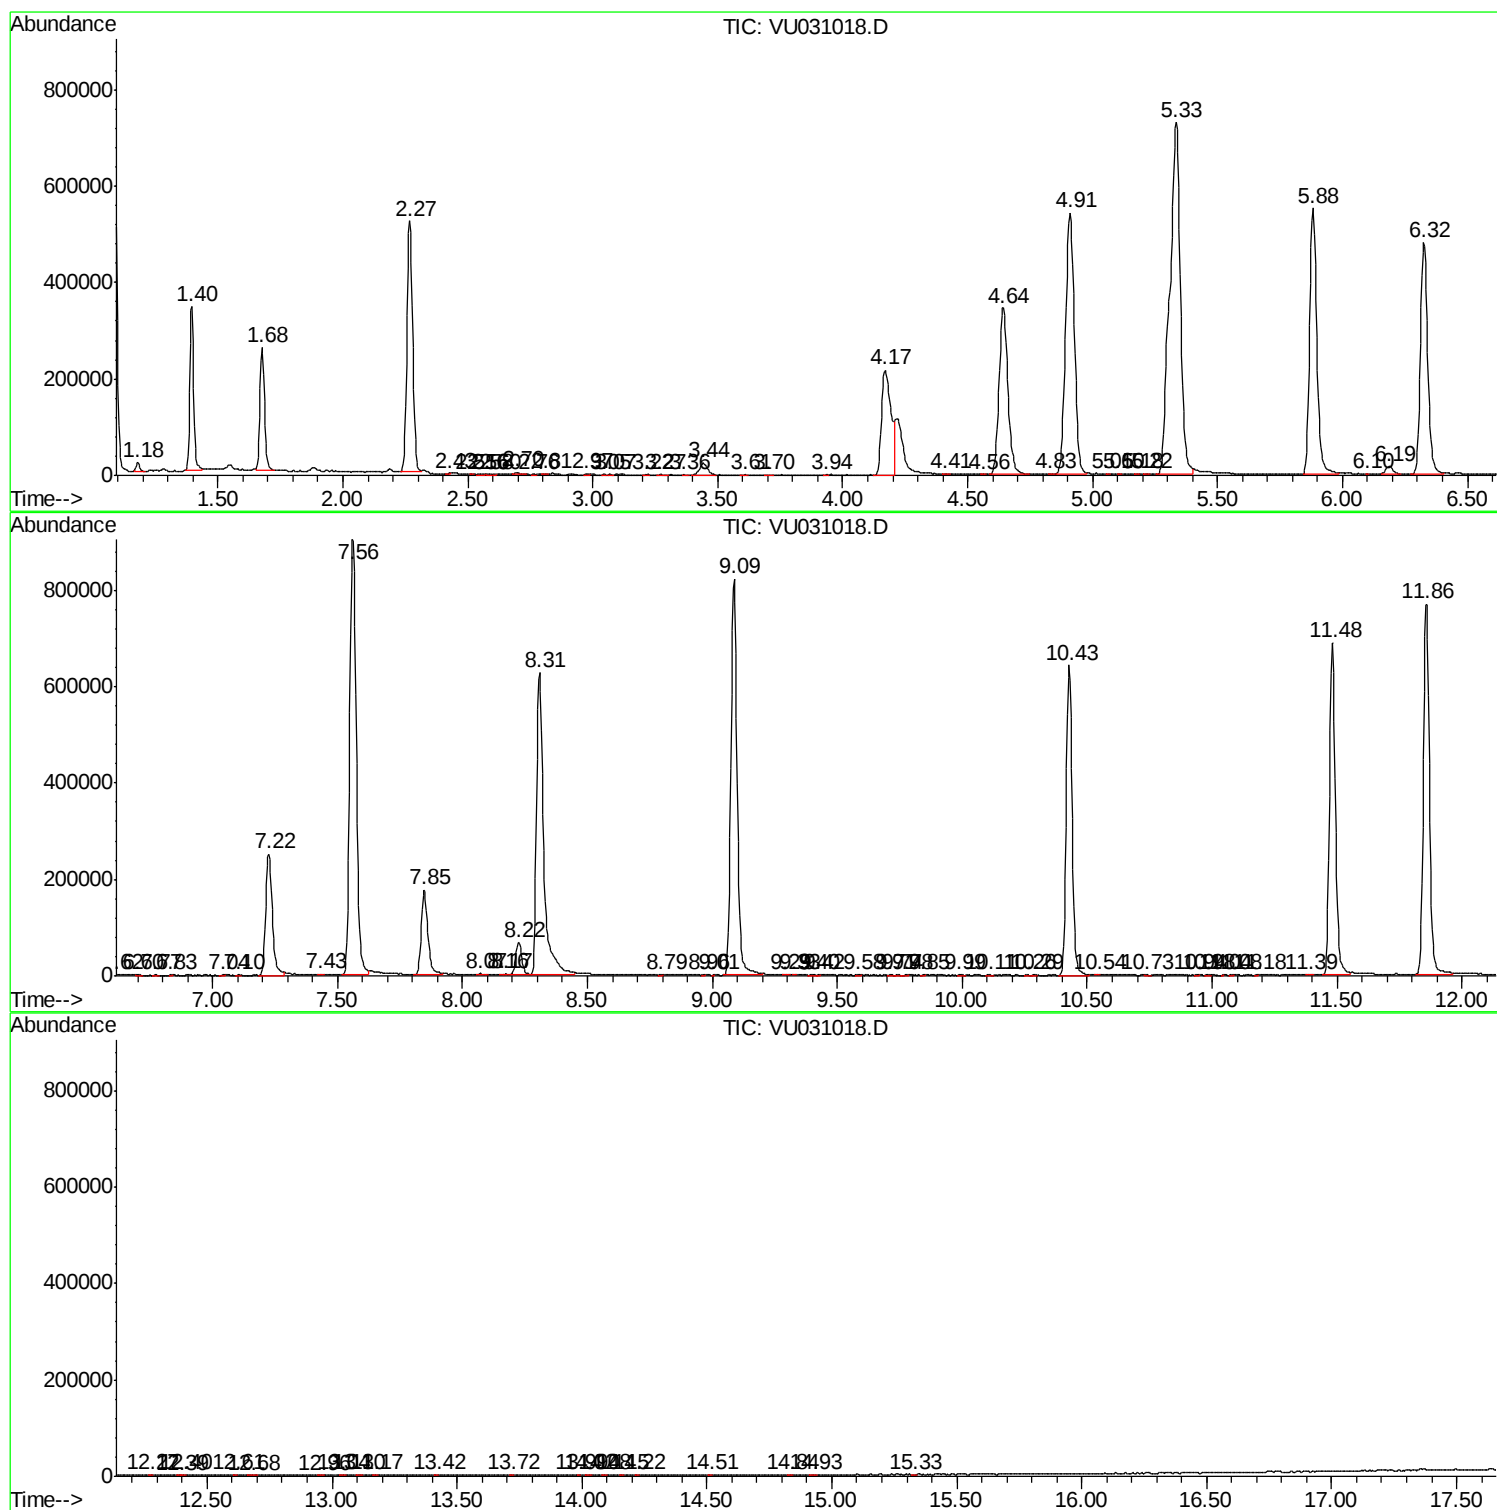

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031018.D
Acq On : 10 Apr 2019 18:04
Operator : JC/SP
Sample : K2249-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031018.D
Acq On : 10 Apr 2019 18:04
Operator : JC/SP
Sample : K2249-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YE3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc