

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031019.D
 Acq On : 10 Apr 2019 18:26
 Operator : JC/SP
 Sample : K2249-12DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB	11744	10047	0.47%	0.060%
2	1.396	88	95	112	rVB	373997	387723	18.05%	2.332%
3	1.675	174	182	199	rBV2	248731	367972	17.13%	2.213%
4	2.267	355	366	380	rBV	511869	789572	36.75%	4.749%
5	2.431	414	417	418	rBV2	1021	642	0.03%	0.004%
6	2.695	490	499	511	rBV7	4263	6595	0.31%	0.040%
7	2.788	524	528	533	rBV6	994	1211	0.06%	0.007%
8	2.823	535	539	543	rVV4	1113	1300	0.06%	0.008%
9	2.846	543	546	548	rVV2	1100	825	0.04%	0.005%
10	2.858	548	550	555	rVB2	761	497	0.02%	0.003%
11	2.981	576	588	596	rBV3	8274	15634	0.73%	0.094%
12	3.067	610	615	622	rVB4	792	758	0.04%	0.005%
13	3.196	650	655	660	rBV3	980	990	0.05%	0.006%
14	3.251	668	672	677	rVB3	531	524	0.02%	0.003%
15	3.440	715	731	751	rVV	278972	634001	29.51%	3.813%
16	3.823	847	850	854	rVB2	709	517	0.02%	0.003%
17	3.865	861	863	867	rVB3	754	545	0.03%	0.003%
18	4.045	914	919	921	rBV2	585	535	0.02%	0.003%
19	4.170	944	958	963	rBV2	220283	437475	20.36%	2.631%
20	4.511	1062	1064	1069	rVB4	1166	790	0.04%	0.005%
21	4.569	1079	1082	1085	rBV3	1159	920	0.04%	0.006%
22	4.643	1088	1105	1132	rVV	337688	845048	39.33%	5.082%
23	4.820	1157	1160	1161	rBV3	963	540	0.03%	0.003%
24	4.910	1173	1188	1206	rBV2	162047	382178	17.79%	2.298%
25	5.180	1265	1272	1278	rBV5	733	1130	0.05%	0.007%
26	5.219	1281	1284	1285	rBV3	948	501	0.02%	0.003%
27	5.334	1296	1320	1354	rBV2	715565	2148616	100.00%	12.922%
28	5.559	1387	1390	1392	rBV3	1052	766	0.04%	0.005%
29	5.624	1407	1410	1415	rVB5	1680	1513	0.07%	0.009%
30	5.653	1415	1419	1422	rBV3	1520	1359	0.06%	0.008%
31	5.694	1430	1432	1438	rVB4	977	735	0.03%	0.004%
32	5.759	1450	1452	1456	rVB3	1546	960	0.04%	0.006%
33	5.817	1467	1470	1471	rBV2	1091	688	0.03%	0.004%
34	5.881	1476	1490	1517	rBV	541171	1090746	50.77%	6.560%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031019.D
 Acq On : 10 Apr 2019 18:26
 Operator : JC/SP
 Sample : K2249-12DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.128	1565	1567	1572	rVB3	866	581	0.03%	0.003%
36	6.190	1572	1586	1594	rBV3	4944	11357	0.53%	0.068%
37	6.325	1612	1628	1649	rBV	473496	968076	45.06%	5.822%
38	6.543	1694	1696	1703	rVB7	1272	900	0.04%	0.005%
39	6.694	1741	1743	1751	rVB4	1288	1248	0.06%	0.008%
40	6.743	1755	1758	1762	rVB4	1218	846	0.04%	0.005%
41	6.768	1762	1766	1769	rVB2	965	804	0.04%	0.005%
42	6.833	1780	1786	1790	rBV3	1101	948	0.04%	0.006%
43	7.083	1857	1864	1866	rVB4	763	663	0.03%	0.004%
44	7.106	1866	1871	1875	rVB5	754	895	0.04%	0.005%
45	7.135	1875	1880	1883	rBV3	529	630	0.03%	0.004%
46	7.186	1891	1896	1897	rBV3	721	497	0.02%	0.003%
47	7.225	1897	1908	1928	rBV	244935	450711	20.98%	2.711%
48	7.562	1998	2013	2045	rBV	904656	1606027	74.75%	9.659%
49	7.849	2090	2102	2125	rBV	172765	316991	14.75%	1.906%
50	8.013	2150	2153	2156	rVB3	1089	606	0.03%	0.004%
51	8.141	2189	2193	2198	rBV4	1056	901	0.04%	0.005%
52	8.177	2198	2204	2211	rVB9	2051	2986	0.14%	0.018%
53	8.225	2211	2219	2230	rBV5	6579	10481	0.49%	0.063%
54	8.308	2234	2245	2278	rBV	614727	1226550	57.09%	7.377%
55	8.556	2320	2322	2326	rBV3	1004	727	0.03%	0.004%
56	8.611	2336	2339	2349	rVB6	1187	1481	0.07%	0.009%
57	8.845	2410	2412	2417	rVB5	1263	1028	0.05%	0.006%
58	8.884	2417	2424	2425	rBV5	925	979	0.05%	0.006%
59	8.926	2434	2437	2442	rBV3	676	614	0.03%	0.004%
60	9.087	2474	2487	2509	rBV	817601	1380205	64.24%	8.301%
61	9.328	2558	2562	2564	rBV3	1435	1111	0.05%	0.007%
62	9.366	2570	2574	2575	rBV2	1319	875	0.04%	0.005%
63	9.585	2637	2642	2645	rVB3	668	720	0.03%	0.004%
64	9.726	2681	2686	2690	rBV3	641	617	0.03%	0.004%
65	9.855	2721	2726	2728	rBV3	1088	810	0.04%	0.005%
66	9.900	2737	2740	2745	rVB3	756	539	0.03%	0.003%
67	9.926	2745	2748	2751	rBV4	577	506	0.02%	0.003%
68	10.029	2777	2780	2784	rVB3	731	498	0.02%	0.003%
69	10.180	2820	2827	2829	rBV4	692	774	0.04%	0.005%
70	10.427	2892	2904	2927	rVV	639301	1048278	48.79%	6.304%
71	10.595	2952	2956	2960	rBV5	1093	1147	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031019.D
 Acq On : 10 Apr 2019 18:26
 Operator : JC/SP
 Sample : K2249-12DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E3YD6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.614	2960	2962	2970	rVB3	1452	1235	0.06%	0.007%
73	10.681	2981	2983	2985	rBV2	826	493	0.02%	0.003%
74	10.810	3020	3023	3029	rBV4	563	514	0.02%	0.003%
75	10.881	3040	3045	3048	rBV3	556	569	0.03%	0.003%
76	10.926	3053	3059	3062	rBV3	725	624	0.03%	0.004%
77	10.955	3065	3068	3072	rBV2	714	557	0.03%	0.003%
78	11.083	3103	3108	3113	rBV6	953	1023	0.05%	0.006%
79	11.254	3156	3161	3163	rBV2	697	638	0.03%	0.004%
80	11.267	3163	3165	3169	rVB3	901	619	0.03%	0.004%
81	11.376	3195	3199	3202	rBV2	529	488	0.02%	0.003%
82	11.424	3206	3214	3218	rVB3	900	1276	0.06%	0.008%
83	11.479	3218	3231	3259	rBV	676413	1131326	52.65%	6.804%
84	11.803	3329	3332	3334	rBV3	693	533	0.02%	0.003%
85	11.855	3336	3348	3371	rBV	769420	1297186	60.37%	7.801%
86	12.353	3498	3503	3507	rBV3	1396	1159	0.05%	0.007%
87	12.829	3648	3651	3655	rBV	703	664	0.03%	0.004%
88	12.881	3665	3667	3670	rVB	1151	634	0.03%	0.004%
89	13.385	3821	3824	3829	rBV5	708	783	0.04%	0.005%
90	13.411	3829	3832	3834	rVV2	821	522	0.02%	0.003%
91	13.807	3952	3955	3958	rBV	917	534	0.02%	0.003%
92	13.971	4004	4006	4010	rVB2	1102	714	0.03%	0.004%
93	14.012	4016	4019	4021	rBV3	861	557	0.03%	0.003%
94	14.569	4188	4192	4194	rBV2	1086	881	0.04%	0.005%
95	14.623	4205	4209	4211	rBV2	1110	820	0.04%	0.005%
96	14.665	4218	4222	4225	rBV2	1623	1434	0.07%	0.009%
97	14.816	4267	4269	4272	rBV2	852	536	0.02%	0.003%
98	15.115	4358	4362	4365	rBV3	1601	1400	0.07%	0.008%
99	15.160	4374	4376	4379	rBV	965	720	0.03%	0.004%
100	15.450	4463	4466	4472	rBV4	1534	1798	0.08%	0.011%


Sum of corrected areas: 16627697

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031019.D
Acq On : 10 Apr 2019 18:26
Operator : JC/SP
Sample : K2249-12DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD6DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

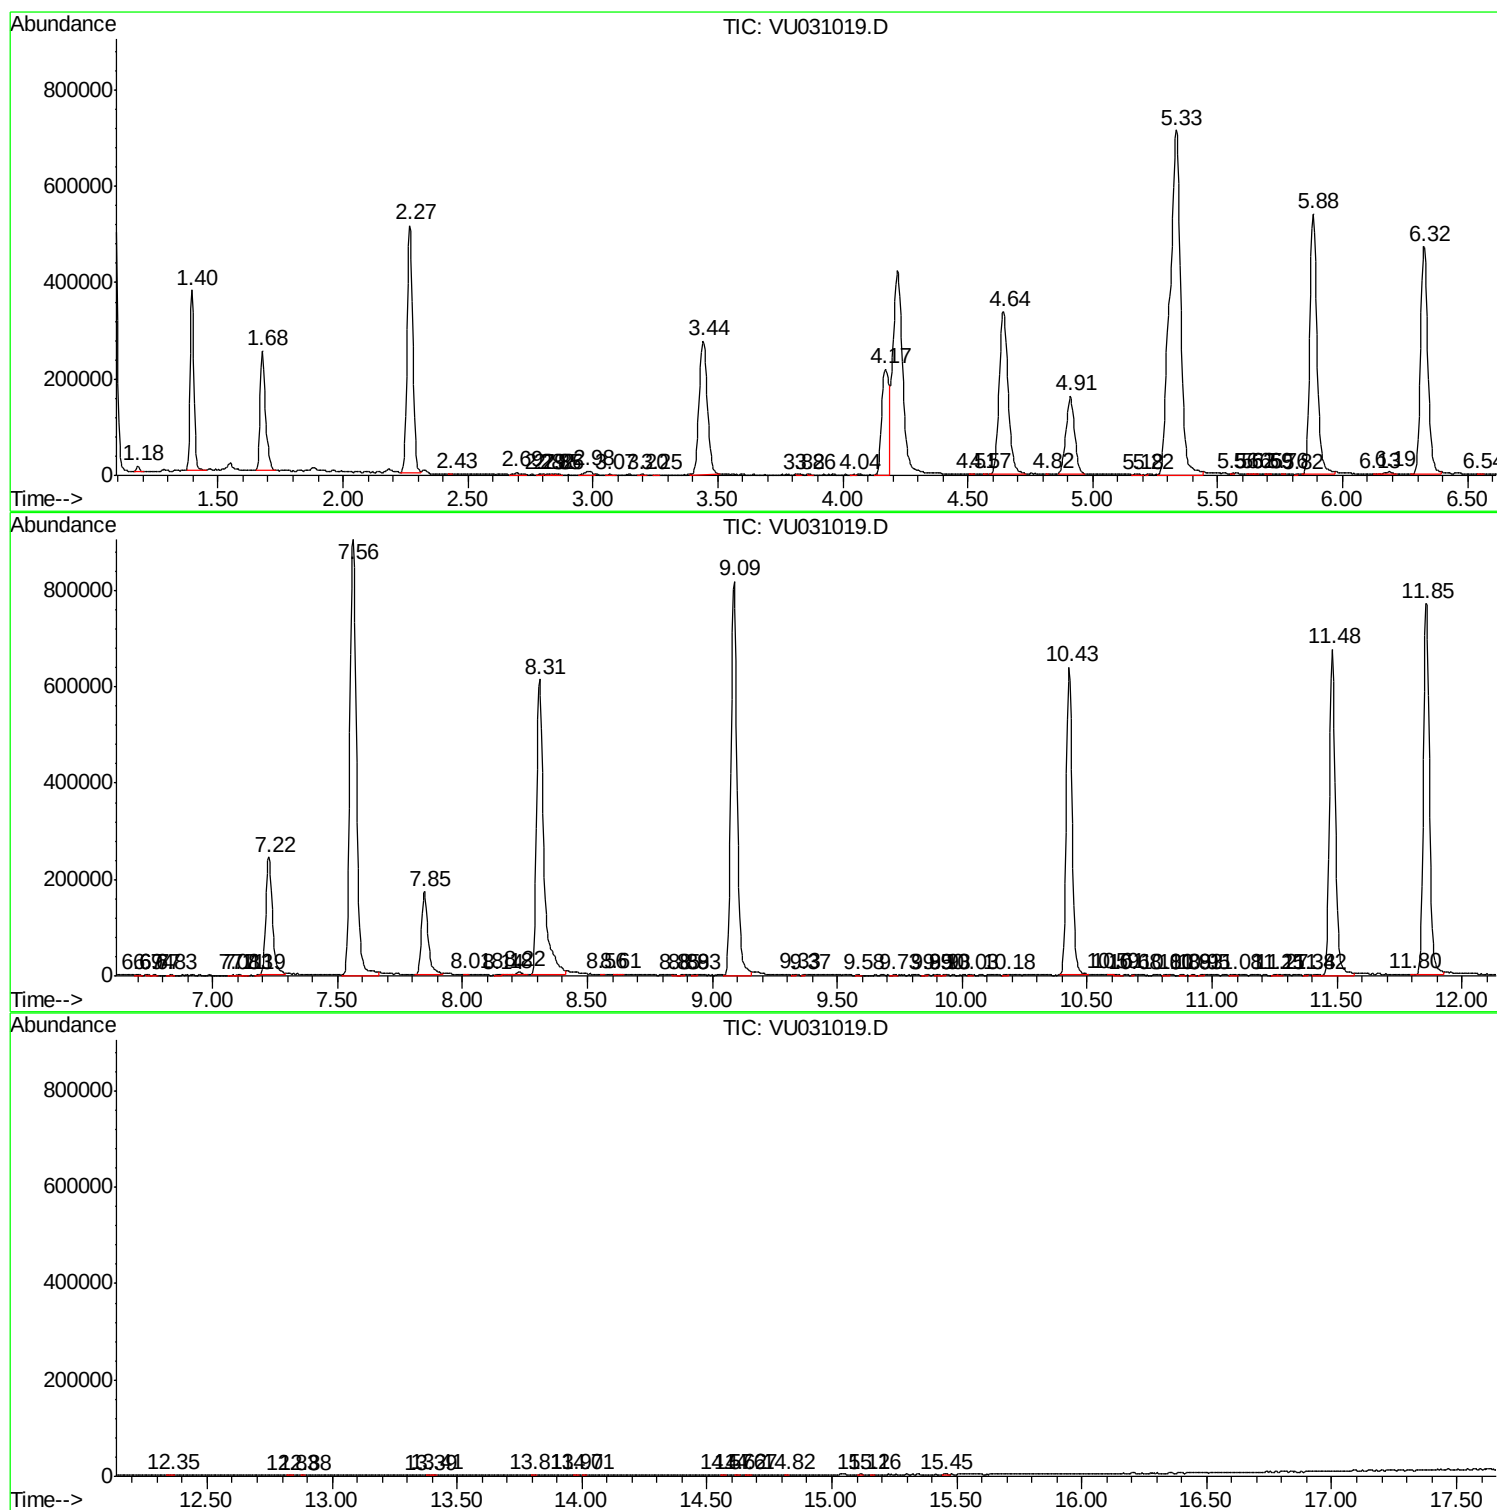

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031019.D
Acq On : 10 Apr 2019 18:26
Operator : JC/SP
Sample : K2249-12DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031019.D
Acq On : 10 Apr 2019 18:26
Operator : JC/SP
Sample : K2249-12DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E3YD6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc