

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031042.D
 Acq On : 11 Apr 2019 04:37
 Operator : JC/SP
 Sample : K2339-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	37	rVB3	16968	16863	0.74%	0.098%
2	1.395	87	95	106	rBV	352855	363302	15.96%	2.121%
3	1.678	174	183	200	rVB	252003	332670	14.62%	1.942%
4	2.267	356	366	379	rBV	528378	795456	34.95%	4.645%
5	2.437	410	419	435	rBV2	18307	35749	1.57%	0.209%
6	2.585	461	465	470	rVB5	842	826	0.04%	0.005%
7	2.698	489	500	514	rBV3	10369	18652	0.82%	0.109%
8	2.788	526	528	531	rBV2	865	594	0.03%	0.003%
9	2.826	534	540	543	rBV5	1661	2188	0.10%	0.013%
10	2.903	561	564	567	rBV3	783	646	0.03%	0.004%
11	2.926	567	571	575	rVV5	809	616	0.03%	0.004%
12	3.270	676	678	681	rBV	851	534	0.02%	0.003%
13	3.289	681	684	687	rVV3	1090	772	0.03%	0.005%
14	3.633	788	791	795	rBV2	793	731	0.03%	0.004%
15	3.897	866	873	876	rBV3	1824	1925	0.08%	0.011%
16	3.977	893	898	902	rBV4	513	590	0.03%	0.003%
17	4.170	946	958	991	rBV2	231053	638324	28.05%	3.727%
18	4.643	1086	1105	1133	rBV	360745	895975	39.37%	5.231%
19	4.781	1145	1148	1151	rBV3	933	533	0.02%	0.003%
20	4.881	1176	1179	1183	rVB4	1365	1111	0.05%	0.006%
21	4.981	1206	1210	1214	rBV5	1256	1120	0.05%	0.007%
22	5.202	1276	1279	1283	rBV3	690	627	0.03%	0.004%
23	5.334	1296	1320	1350	rBV2	771458	2275980	100.00%	13.289%
24	5.781	1457	1459	1465	rBV5	822	813	0.04%	0.005%
25	5.881	1478	1490	1519	rBV	608972	1229408	54.02%	7.178%
26	6.154	1571	1575	1576	rBV3	1187	753	0.03%	0.004%
27	6.183	1576	1584	1587	rVV8	3783	4842	0.21%	0.028%
28	6.325	1615	1628	1650	rBV	504151	1021142	44.87%	5.962%
29	6.543	1693	1696	1700	rVB4	1081	859	0.04%	0.005%
30	6.562	1700	1702	1704	rBV2	878	555	0.02%	0.003%
31	6.656	1729	1731	1736	rVB5	1065	655	0.03%	0.004%
32	6.688	1738	1741	1744	rVB2	951	606	0.03%	0.004%
33	6.887	1798	1803	1805	rBV3	809	566	0.02%	0.003%
34	7.225	1896	1908	1933	rBV	256363	487350	21.41%	2.846%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031042.D
 Acq On : 11 Apr 2019 04:37
 Operator : JC/SP
 Sample : K2339-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	7.421	1966	1969	1974	rBV4	1140	1065	0.05%	0.006%
36	7.456	1978	1980	1984	rBV3	1217	1057	0.05%	0.006%
37	7.562	2000	2013	2037	rBV	967471	1747065	76.76%	10.201%
38	7.849	2091	2102	2120	rBV	176080	324184	14.24%	1.893%
39	8.035	2155	2160	2163	rBV6	1282	1037	0.05%	0.006%
40	8.106	2180	2182	2185	rBV3	806	568	0.02%	0.003%
41	8.138	2189	2192	2195	rVV3	864	717	0.03%	0.004%
42	8.177	2195	2204	2214	rVB3	4539	7985	0.35%	0.047%
43	8.267	2226	2232	2234	rBV2	844	912	0.04%	0.005%
44	8.308	2234	2245	2287	rBV	646205	1324041	58.17%	7.731%
45	8.694	2360	2365	2368	rVB6	951	935	0.04%	0.005%
46	8.746	2379	2381	2386	rVB4	891	625	0.03%	0.004%
47	8.836	2407	2409	2418	rVV4	707	704	0.03%	0.004%
48	8.890	2422	2426	2431	rVB5	501	543	0.02%	0.003%
49	8.932	2434	2439	2444	rBV4	771	900	0.04%	0.005%
50	8.980	2450	2454	2457	rBV3	698	571	0.03%	0.003%
51	8.996	2457	2459	2463	rVB3	880	599	0.03%	0.003%
52	9.025	2463	2468	2473	rBV4	876	1002	0.04%	0.006%
53	9.086	2473	2487	2524	rBV	895419	1565326	68.78%	9.140%
54	9.308	2553	2556	2559	rBV4	1361	1077	0.05%	0.006%
55	9.324	2559	2561	2564	rVV3	869	549	0.02%	0.003%
56	9.350	2564	2569	2573	rVV7	966	946	0.04%	0.006%
57	9.440	2595	2597	2603	rVB6	767	635	0.03%	0.004%
58	9.508	2616	2618	2622	rVB3	1104	598	0.03%	0.003%
59	9.598	2642	2646	2650	rVB2	606	623	0.03%	0.004%
60	9.623	2650	2654	2657	rBV3	834	744	0.03%	0.004%
61	9.730	2683	2687	2689	rBV2	821	540	0.02%	0.003%
62	10.032	2778	2781	2784	rBV2	679	549	0.02%	0.003%
63	10.070	2787	2793	2798	rVB	833	927	0.04%	0.005%
64	10.106	2798	2804	2807	rBV3	909	804	0.04%	0.005%
65	10.125	2807	2810	2813	rBV3	1032	769	0.03%	0.004%
66	10.254	2847	2850	2856	rVB	788	804	0.04%	0.005%
67	10.286	2856	2860	2863	rBV2	817	545	0.02%	0.003%
68	10.324	2870	2872	2877	rVB4	924	818	0.04%	0.005%
69	10.363	2877	2884	2888	rBV2	905	1022	0.04%	0.006%
70	10.427	2892	2904	2931	rVV	684924	1118472	49.14%	6.531%
71	10.604	2951	2959	2968	rVB5	5090	8003	0.35%	0.047%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031042.D
 Acq On : 11 Apr 2019 04:37
 Operator : JC/SP
 Sample : K2339-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.713	2989	2993	2998	rVB5	921	817	0.04%	0.005%
73	10.746	2999	3003	3007	rBV3	666	609	0.03%	0.004%
74	10.794	3015	3018	3020	rBV	947	584	0.03%	0.003%
75	10.852	3031	3036	3040	rBV4	788	822	0.04%	0.005%
76	11.186	3133	3140	3143	rBV3	747	820	0.04%	0.005%
77	11.402	3204	3207	3210	rBV4	913	551	0.02%	0.003%
78	11.482	3219	3232	3262	rBV	824500	1365544	60.00%	7.973%
79	11.855	3333	3348	3374	rBV	870809	1486212	65.30%	8.678%
80	12.299	3481	3486	3492	rVB6	1172	1537	0.07%	0.009%
81	12.360	3502	3505	3509	rVB3	886	631	0.03%	0.004%
82	12.527	3555	3557	3563	rVB3	810	708	0.03%	0.004%
83	12.591	3575	3577	3580	rVB3	1343	793	0.03%	0.005%
84	12.617	3580	3585	3588	rBV3	980	773	0.03%	0.005%
85	12.697	3607	3610	3613	rBV2	786	624	0.03%	0.004%
86	13.205	3765	3768	3771	rBV2	941	738	0.03%	0.004%
87	13.440	3838	3841	3843	rBV3	1174	742	0.03%	0.004%
88	13.466	3847	3849	3854	rVB2	1012	660	0.03%	0.004%
89	13.807	3949	3955	3957	rBV3	1498	1465	0.06%	0.009%
90	13.922	3987	3991	3992	rBV2	712	560	0.02%	0.003%
91	14.134	4055	4057	4060	rVB2	1262	607	0.03%	0.004%
92	14.154	4060	4063	4066	rBV3	1366	966	0.04%	0.006%
93	14.411	4139	4143	4146	rBV3	962	1021	0.04%	0.006%
94	14.543	4181	4184	4187	rVB3	1628	979	0.04%	0.006%
95	14.569	4187	4192	4196	rBV3	1502	1614	0.07%	0.009%
96	14.675	4222	4225	4230	rBV3	1253	1334	0.06%	0.008%
97	14.745	4245	4247	4250	rBV3	920	598	0.03%	0.003%
98	14.845	4275	4278	4282	rBV2	1814	999	0.04%	0.006%
99	14.897	4291	4294	4296	rBV3	1312	709	0.03%	0.004%
100	15.128	4363	4366	4370	rVB3	1484	1029	0.05%	0.006%


Sum of corrected areas: 17126640

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031042.D
Acq On : 11 Apr 2019 04:37
Operator : JC/SP
Sample : K2339-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC73

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

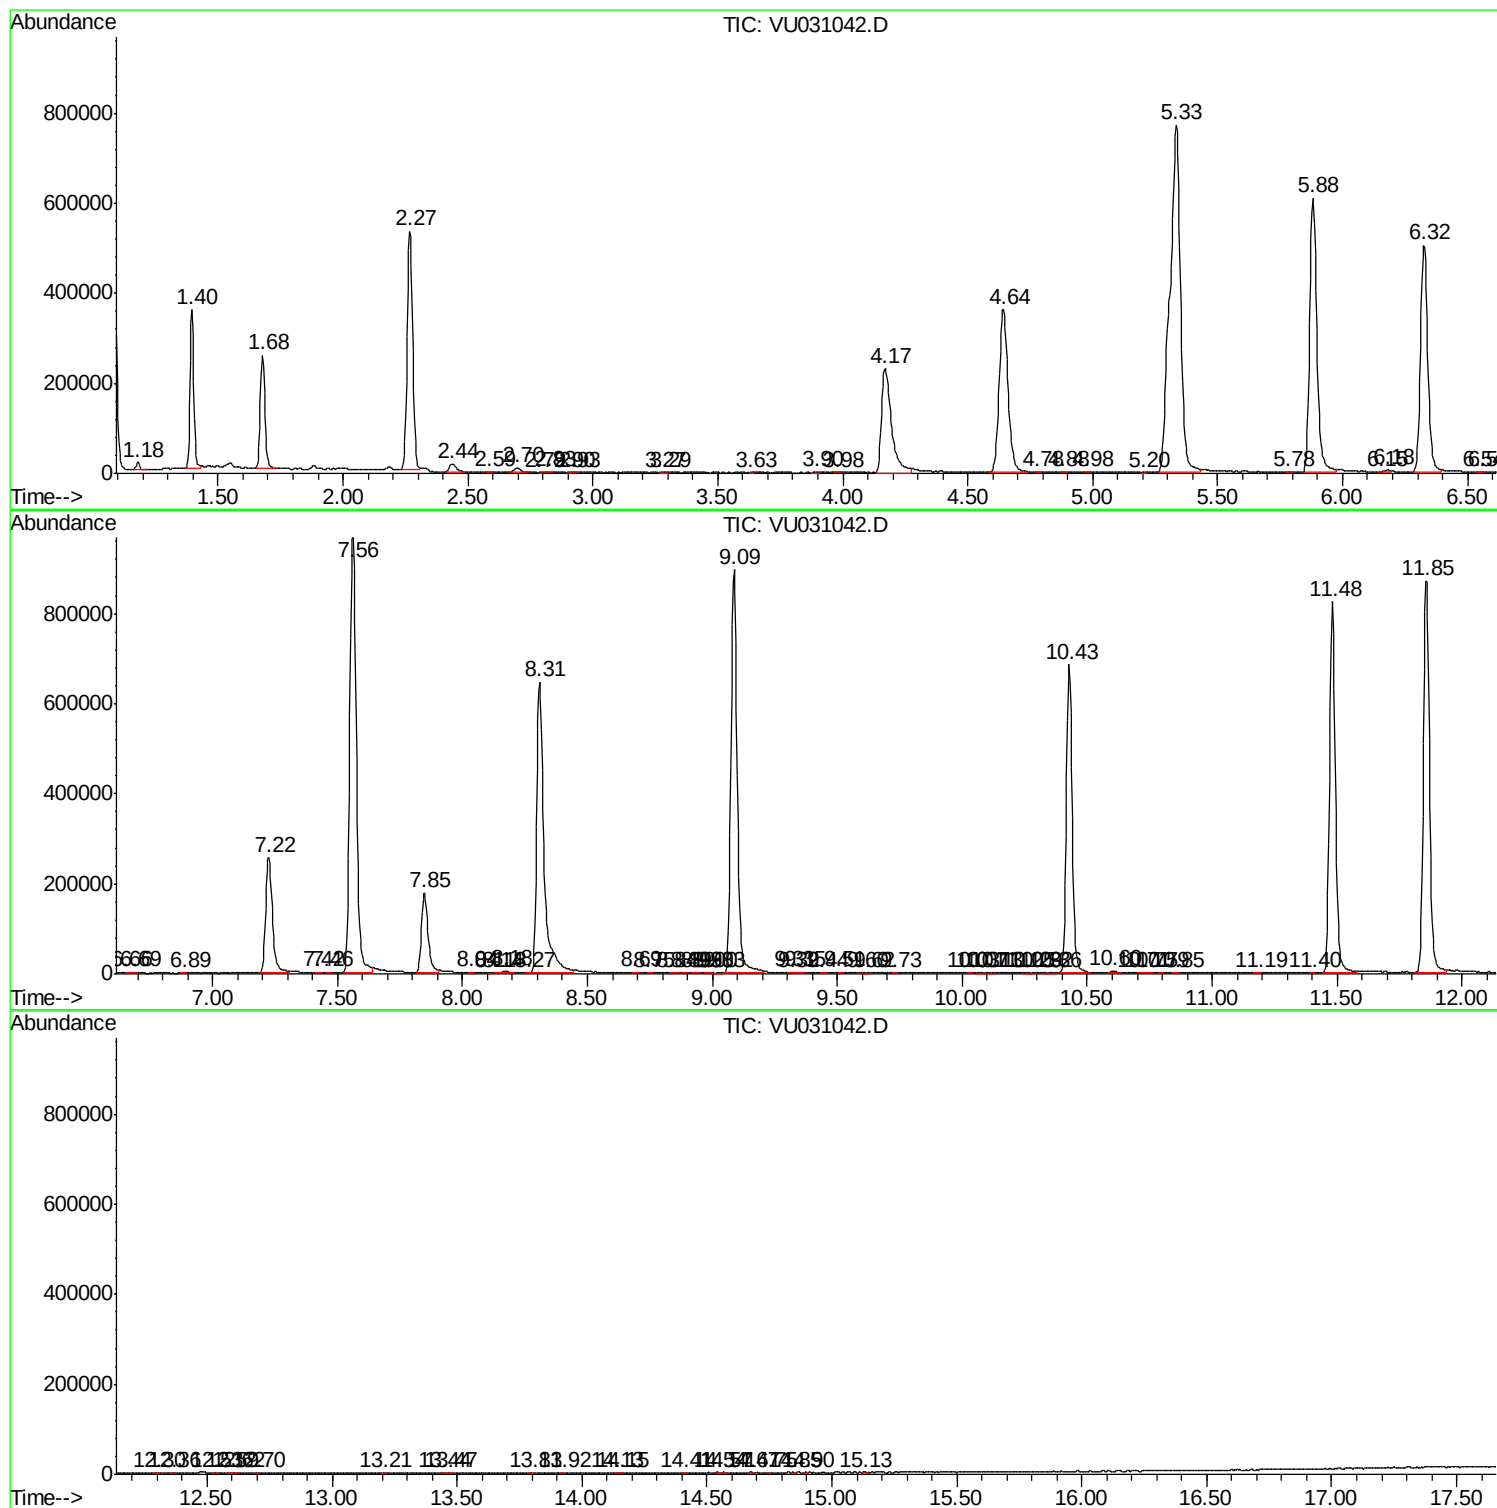

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031042.D
Acq On : 11 Apr 2019 04:37
Operator : JC/SP
Sample : K2339-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC73

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031042.D
Acq On : 11 Apr 2019 04:37
Operator : JC/SP
Sample : K2339-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC73

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc