

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031046.D
 Acq On : 11 Apr 2019 06:09
 Operator : JC/SP
 Sample : K2299-26
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB706

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	39	rVB	15724	14977	0.68%	0.087%
2	1.396	88	95	109	rBV	335883	352227	15.93%	2.043%
3	1.675	174	182	198	rVB	254137	326092	14.75%	1.891%
4	2.267	356	366	378	rBV	511574	768938	34.79%	4.459%
5	2.418	407	413	415	rBV5	1543	1720	0.08%	0.010%
6	2.695	492	499	507	rBV7	1724	2365	0.11%	0.014%
7	2.830	527	541	554	rVB5	5187	11992	0.54%	0.070%
8	2.929	568	572	575	rVB3	772	615	0.03%	0.004%
9	2.984	587	589	594	rBV2	1034	878	0.04%	0.005%
10	3.174	640	648	651	rBV6	1320	1880	0.09%	0.011%
11	3.251	666	672	674	rBV3	886	817	0.04%	0.005%
12	3.376	706	711	717	rVB3	907	971	0.04%	0.006%
13	3.408	717	721	724	rBV2	731	676	0.03%	0.004%
14	3.457	733	736	739	rVV4	756	562	0.03%	0.003%
15	3.476	739	742	752	rVB2	963	1286	0.06%	0.007%
16	3.765	829	832	837	rVB4	1040	859	0.04%	0.005%
17	4.010	900	908	909	rBV3	2439	2418	0.11%	0.014%
18	4.170	945	958	990	rBV	224731	630110	28.50%	3.654%
19	4.395	1026	1028	1031	rBV2	846	670	0.03%	0.004%
20	4.450	1043	1045	1051	rVB6	899	615	0.03%	0.004%
21	4.518	1062	1066	1070	rVB3	856	712	0.03%	0.004%
22	4.643	1087	1105	1133	rBV3	375947	1024307	46.34%	5.940%
23	4.842	1165	1167	1173	rBV5	899	787	0.04%	0.005%
24	4.958	1200	1203	1206	rBV2	893	749	0.03%	0.004%
25	4.987	1211	1212	1216	rVV3	969	572	0.03%	0.003%
26	5.045	1227	1230	1236	rVB4	774	737	0.03%	0.004%
27	5.103	1242	1248	1250	rBV3	637	642	0.03%	0.004%
28	5.170	1265	1269	1273	rVB3	648	605	0.03%	0.004%
29	5.334	1296	1320	1340	rBV2	753494	2210544	100.00%	12.820%
30	5.604	1401	1404	1406	rBV3	1234	827	0.04%	0.005%
31	5.672	1420	1425	1429	rBV6	1925	1904	0.09%	0.011%
32	5.813	1467	1469	1475	rVB6	1705	1376	0.06%	0.008%
33	5.881	1475	1490	1519	rBV2	596482	1206964	54.60%	7.000%
34	6.125	1564	1566	1572	rVB7	1031	582	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031046.D
 Acq On : 11 Apr 2019 06:09
 Operator : JC/SP
 Sample : K2299-26
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB706

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.154	1572	1575	1577	rBV3	1219	911	0.04%	0.005%
36	6.180	1578	1583	1587	rBV6	2866	3006	0.14%	0.017%
37	6.257	1604	1607	1610	rBV4	939	686	0.03%	0.004%
38	6.325	1614	1628	1659	rVV	495808	1005789	45.50%	5.833%
39	6.508	1681	1685	1689	rVB5	1016	984	0.04%	0.006%
40	6.553	1695	1699	1701	rBV4	1289	1213	0.05%	0.007%
41	6.752	1747	1761	1778	rBV2	96477	185670	8.40%	1.077%
42	6.993	1832	1836	1837	rBV2	1023	679	0.03%	0.004%
43	7.225	1895	1908	1935	rBV2	256553	484258	21.91%	2.808%
44	7.389	1955	1959	1962	rVB6	1467	1229	0.06%	0.007%
45	7.479	1976	1987	1991	rBV5	3358	5968	0.27%	0.035%
46	7.559	1997	2012	2042	rBV	934593	1705017	77.13%	9.888%
47	7.849	2091	2102	2134	rBV2	178408	330671	14.96%	1.918%
48	8.080	2170	2174	2176	rBV2	747	562	0.03%	0.003%
49	8.173	2198	2203	2212	rBV6	3237	4501	0.20%	0.026%
50	8.251	2224	2227	2230	rVB3	944	575	0.03%	0.003%
51	8.308	2234	2245	2284	rVV	641686	1300919	58.85%	7.545%
52	8.472	2285	2296	2317	rVB4	112093	211094	9.55%	1.224%
53	8.694	2359	2365	2367	rBV3	1073	1070	0.05%	0.006%
54	8.775	2384	2390	2393	rBV6	606	695	0.03%	0.004%
55	8.797	2393	2397	2399	rBV4	901	713	0.03%	0.004%
56	8.862	2413	2417	2421	rBV4	1000	912	0.04%	0.005%
57	8.907	2426	2431	2435	rBV3	970	1077	0.05%	0.006%
58	9.042	2469	2473	2474	rBV2	1183	767	0.03%	0.004%
59	9.087	2474	2487	2507	rBV	862785	1490249	67.42%	8.643%
60	9.755	2691	2695	2698	rVV3	591	587	0.03%	0.003%
61	9.775	2698	2701	2706	rVV4	825	757	0.03%	0.004%
62	9.810	2709	2712	2717	rVB2	939	915	0.04%	0.005%
63	9.887	2734	2736	2744	rVB4	1307	1234	0.06%	0.007%
64	9.961	2747	2759	2770	rBV2	12680	22042	1.00%	0.128%
65	10.051	2779	2787	2793	rBV10	2851	5061	0.23%	0.029%
66	10.199	2830	2833	2837	rBV2	787	645	0.03%	0.004%
67	10.427	2890	2904	2931	rVV	660055	1084079	49.04%	6.287%
68	10.601	2953	2958	2967	rVB9	3118	4888	0.22%	0.028%
69	10.791	3014	3017	3021	rVB3	850	614	0.03%	0.004%
70	10.884	3042	3046	3052	rBV5	1165	1203	0.05%	0.007%
71	10.913	3052	3055	3059	rBV	789	572	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031046.D
 Acq On : 11 Apr 2019 06:09
 Operator : JC/SP
 Sample : K2299-26
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB706

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.974	3072	3074	3079	rVB3	770	645	0.03%	0.004%
73	11.070	3099	3104	3108	rBV6	944	924	0.04%	0.005%
74	11.209	3145	3147	3151	rVB3	748	613	0.03%	0.004%
75	11.318	3177	3181	3183	rBV2	760	631	0.03%	0.004%
76	11.376	3194	3199	3201	rBV4	3049	2815	0.13%	0.016%
77	11.479	3220	3231	3257	rBV	808949	1339612	60.60%	7.769%
78	11.759	3316	3318	3321	rBV2	1136	736	0.03%	0.004%
79	11.855	3336	3348	3367	rBV	857733	1437400	65.02%	8.336%
80	12.131	3431	3434	3436	rBV3	1101	819	0.04%	0.005%
81	12.328	3492	3495	3498	rBV3	1224	805	0.04%	0.005%
82	12.347	3498	3501	3506	rVV6	1501	1164	0.05%	0.007%
83	12.379	3508	3511	3514	rBV2	879	570	0.03%	0.003%
84	12.476	3534	3541	3548	rBV6	2778	4226	0.19%	0.025%
85	12.755	3625	3628	3631	rVB3	1331	790	0.04%	0.005%
86	12.816	3644	3647	3651	rVB4	1316	774	0.04%	0.004%
87	12.961	3688	3692	3697	rBV4	1096	1322	0.06%	0.008%
88	13.009	3703	3707	3710	rBV3	1493	1185	0.05%	0.007%
89	13.125	3736	3743	3746	rBV6	1988	2206	0.10%	0.013%
90	13.238	3773	3778	3781	rBV4	1264	1311	0.06%	0.008%
91	13.533	3868	3870	3872	rBV2	993	559	0.03%	0.003%
92	13.752	3934	3938	3942	rBV4	1377	1491	0.07%	0.009%
93	13.771	3942	3944	3947	rVV2	827	628	0.03%	0.004%
94	13.990	4010	4012	4017	rVB4	1133	833	0.04%	0.005%
95	14.012	4017	4019	4021	rBV	1151	705	0.03%	0.004%
96	14.311	4109	4112	4114	rBV3	1494	882	0.04%	0.005%
97	14.340	4117	4121	4124	rBV5	1120	1164	0.05%	0.007%
98	14.591	4196	4199	4208	rVB6	2200	2295	0.10%	0.013%
99	14.990	4320	4323	4324	rBV3	1615	911	0.04%	0.005%
100	15.093	4352	4355	4358	rBV4	1873	1259	0.06%	0.007%


Sum of corrected areas: 17243063

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031046.D
Acq On : 11 Apr 2019 06:09
Operator : JC/SP
Sample : K2299-26
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB706

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

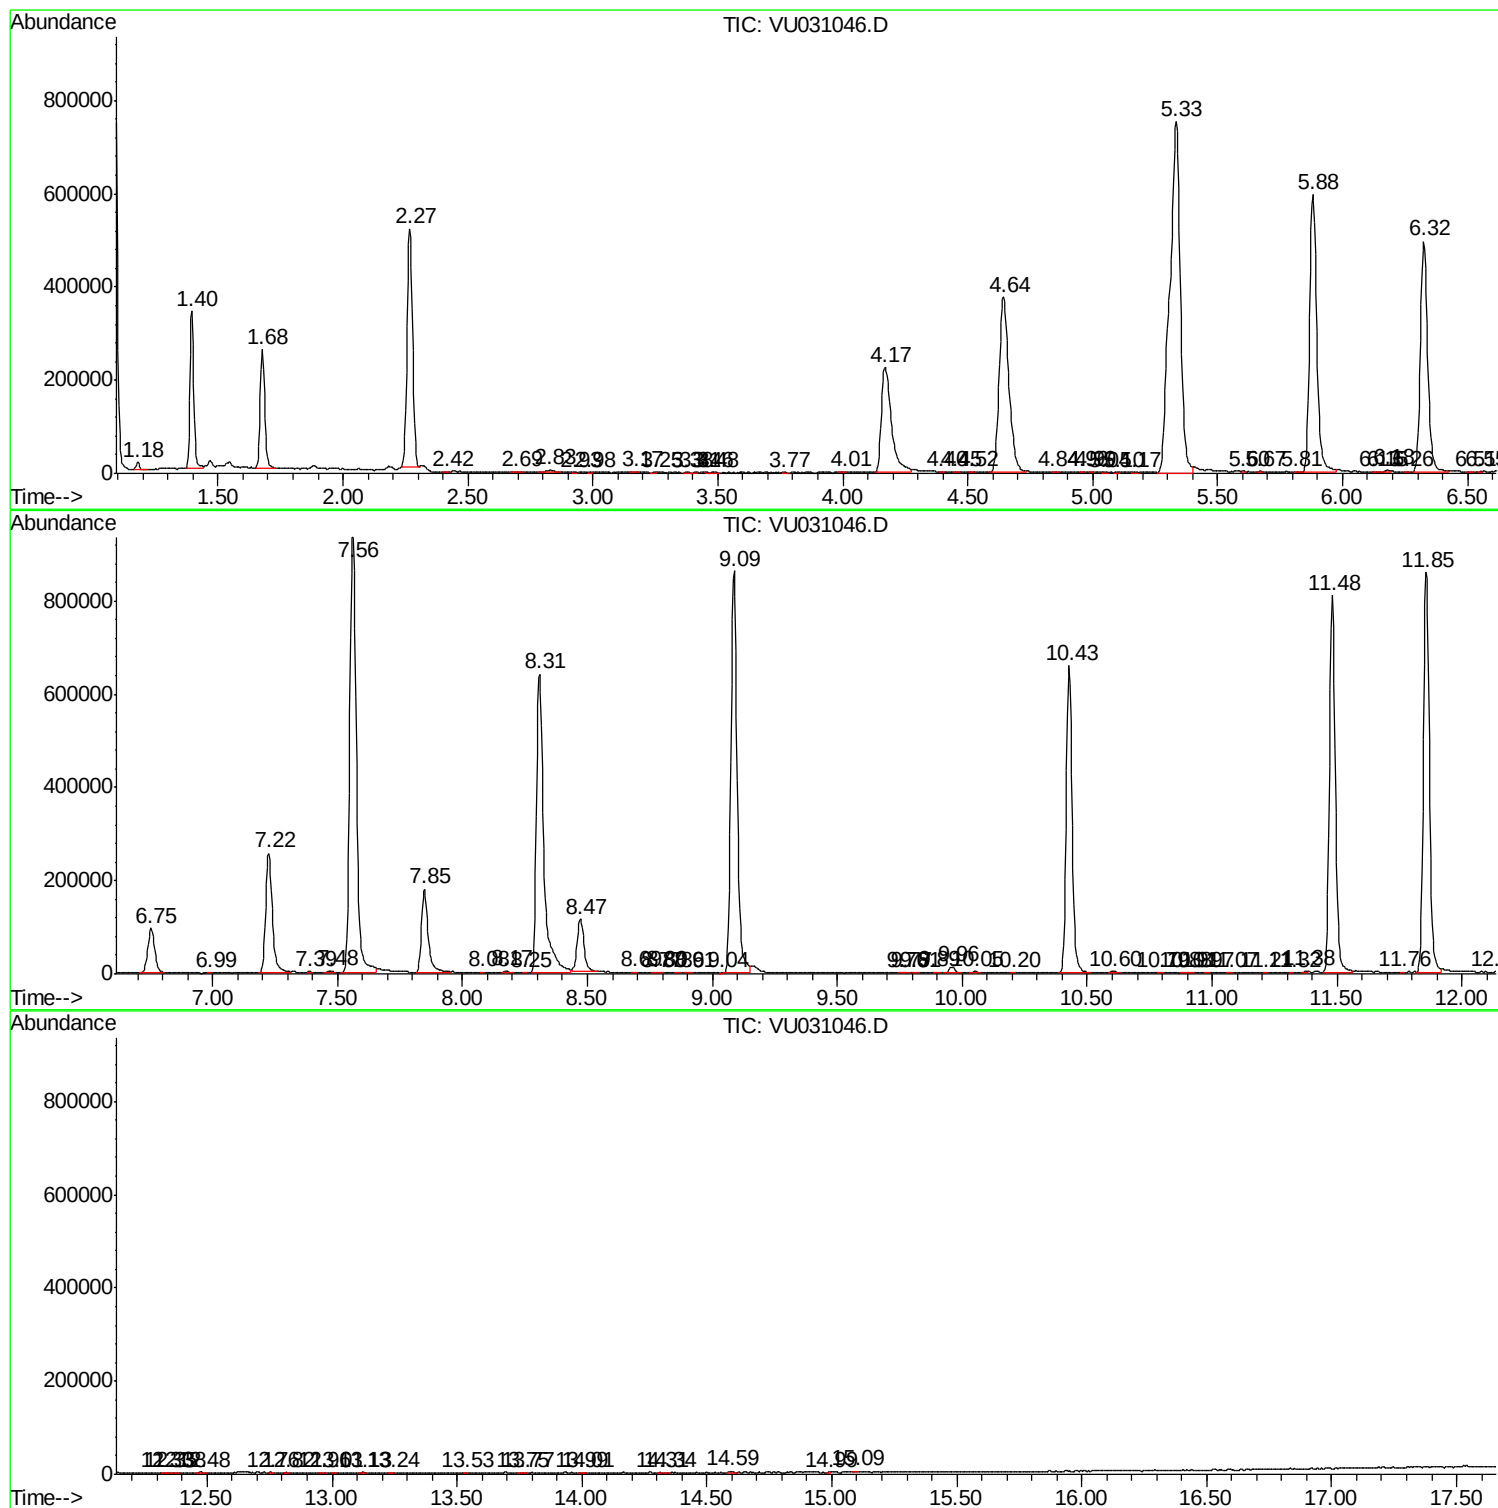

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031046.D
Acq On : 11 Apr 2019 06:09
Operator : JC/SP
Sample : K2299-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB706

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031046.D
Acq On : 11 Apr 2019 06:09
Operator : JC/SP
Sample : K2299-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB706

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc