

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031063.D
 Acq On : 11 Apr 2019 12:40
 Operator : JC/SP
 Sample : K2339-01 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB2	16681	15743	0.72%	0.097%
2	1.396	88	95	108	rBV	310263	322870	14.76%	1.992%
3	1.679	175	183	203	rVB	239269	317316	14.51%	1.958%
4	2.267	356	366	380	rBV	491905	739549	33.82%	4.564%
5	2.527	444	447	450	rBV3	849	558	0.03%	0.003%
6	2.663	487	489	492	rVB2	968	528	0.02%	0.003%
7	2.695	492	499	510	rBV5	3070	4847	0.22%	0.030%
8	2.801	528	532	533	rBV	1082	658	0.03%	0.004%
9	2.968	581	584	588	rBV2	770	591	0.03%	0.004%
10	3.029	598	603	606	rBV3	723	713	0.03%	0.004%
11	3.058	609	612	617	rVB2	789	566	0.03%	0.003%
12	3.119	628	631	636	rBV2	607	649	0.03%	0.004%
13	3.151	638	641	645	rVV2	628	596	0.03%	0.004%
14	3.280	676	681	682	rBV	690	558	0.03%	0.003%
15	3.312	686	691	694	rVB3	884	794	0.04%	0.005%
16	3.383	710	713	720	rVV4	597	549	0.03%	0.003%
17	3.531	752	759	762	rVB3	841	921	0.04%	0.006%
18	3.569	766	771	773	rBV2	686	616	0.03%	0.004%
19	3.756	825	829	833	rVB3	680	528	0.02%	0.003%
20	3.952	881	890	893	rBV3	921	1050	0.05%	0.006%
21	3.971	893	896	900	rVV2	593	528	0.02%	0.003%
22	4.058	917	923	927	rBV2	1086	867	0.04%	0.005%
23	4.170	946	958	989	rBV	206889	567302	25.94%	3.501%
24	4.511	1061	1064	1068	rBV3	856	595	0.03%	0.004%
25	4.643	1087	1105	1132	rBV	355818	864140	39.51%	5.333%
26	4.833	1159	1164	1169	rBV6	1437	1805	0.08%	0.011%
27	4.881	1174	1179	1182	rBV4	1416	1345	0.06%	0.008%
28	4.990	1210	1213	1216	rBV3	932	565	0.03%	0.003%
29	5.096	1242	1246	1249	rVV2	1090	724	0.03%	0.004%
30	5.141	1254	1260	1261	rBV3	721	677	0.03%	0.004%
31	5.334	1295	1320	1352	rBV2	741051	2186992	100.00%	13.496%
32	5.624	1408	1410	1414	rVB4	1555	839	0.04%	0.005%
33	5.675	1422	1426	1428	rBV4	989	714	0.03%	0.004%
34	5.711	1434	1437	1441	rBV5	896	791	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031063.D
 Acq On : 11 Apr 2019 12:40
 Operator : JC/SP
 Sample : K2339-01 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.740	1444	1446	1450	rVB3	1172	698	0.03%	0.004%
36	5.775	1455	1457	1460	rBV3	820	556	0.03%	0.003%
37	5.823	1469	1472	1477	rBV4	913	813	0.04%	0.005%
38	5.881	1477	1490	1517	rBV	586397	1179927	53.95%	7.281%
39	6.174	1579	1581	1587	rBV4	2111	1843	0.08%	0.011%
40	6.325	1614	1628	1657	rBV	485563	997081	45.59%	6.153%
41	6.569	1701	1704	1707	rBV4	1239	761	0.03%	0.005%
42	6.643	1724	1727	1732	rBV4	1080	1106	0.05%	0.007%
43	6.900	1805	1807	1809	rBV2	884	558	0.03%	0.003%
44	7.225	1896	1908	1933	rBV	254465	483225	22.10%	2.982%
45	7.563	2000	2013	2042	rBV	916283	1672486	76.47%	10.321%
46	7.846	2090	2101	2123	rBV	173828	320634	14.66%	1.979%
47	8.125	2186	2188	2192	rBV	1056	903	0.04%	0.006%
48	8.145	2192	2194	2197	rVV	820	545	0.02%	0.003%
49	8.180	2197	2205	2211	rVB7	2401	3171	0.14%	0.020%
50	8.231	2211	2221	2231	rVB8	8066	14433	0.66%	0.089%
51	8.309	2231	2245	2281	rBV	588478	1205150	55.11%	7.437%
52	8.579	2325	2329	2332	rBV5	1495	1430	0.07%	0.009%
53	8.646	2347	2350	2352	rBV3	809	554	0.03%	0.003%
54	8.791	2391	2395	2396	rVV2	849	526	0.02%	0.003%
55	8.823	2403	2405	2409	rVV2	751	598	0.03%	0.004%
56	8.923	2432	2436	2440	rVB4	734	659	0.03%	0.004%
57	9.087	2474	2487	2513	rBV	854805	1477846	67.57%	9.120%
58	9.501	2612	2616	2619	rBV4	982	741	0.03%	0.005%
59	9.546	2626	2630	2636	rVB6	1390	1161	0.05%	0.007%
60	9.604	2642	2648	2651	rBV	814	641	0.03%	0.004%
61	9.627	2651	2655	2658	rBV3	862	678	0.03%	0.004%
62	9.717	2680	2683	2686	rBV3	945	707	0.03%	0.004%
63	9.762	2691	2697	2700	rBV3	957	974	0.04%	0.006%
64	9.781	2700	2703	2706	rBV3	798	598	0.03%	0.004%
65	9.845	2719	2723	2729	rBV2	616	830	0.04%	0.005%
66	10.032	2779	2781	2786	rVV2	688	554	0.03%	0.003%
67	10.061	2787	2790	2793	rVB	1052	638	0.03%	0.004%
68	10.238	2843	2845	2849	rVB2	768	528	0.02%	0.003%
69	10.273	2849	2856	2859	rBV3	781	1037	0.05%	0.006%
70	10.299	2859	2864	2866	rBV2	773	832	0.04%	0.005%
71	10.347	2874	2879	2883	rBV3	854	760	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031063.D
 Acq On : 11 Apr 2019 12:40
 Operator : JC/SP
 Sample : K2339-01 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.370	2883	2886	2888	rBV2	1195	789	0.04%	0.005%
73	10.427	2892	2904	2929	rVV	653342	1063359	48.62%	6.562%
74	10.646	2969	2972	2977	rVB4	1031	881	0.04%	0.005%
75	10.968	3070	3072	3077	rVB2	903	713	0.03%	0.004%
76	10.997	3077	3081	3084	rBV2	909	745	0.03%	0.005%
77	11.080	3103	3107	3110	rBV3	1015	891	0.04%	0.005%
78	11.302	3171	3176	3181	rBV3	718	891	0.04%	0.005%
79	11.373	3194	3198	3203	rBV2	617	654	0.03%	0.004%
80	11.411	3204	3210	3214	rVV3	965	1049	0.05%	0.006%
81	11.479	3219	3231	3251	rBV	785095	1287963	58.89%	7.948%
82	11.855	3334	3348	3371	rBV	843386	1417884	64.83%	8.750%
83	12.225	3459	3463	3464	rBV3	848	638	0.03%	0.004%
84	12.476	3538	3541	3543	rBV3	1204	977	0.04%	0.006%
85	12.533	3556	3559	3563	rVB3	935	678	0.03%	0.004%
86	12.607	3579	3582	3585	rBV2	1111	814	0.04%	0.005%
87	12.865	3659	3662	3665	rBV3	1033	729	0.03%	0.004%
88	12.932	3673	3683	3686	rBV4	1133	1737	0.08%	0.011%
89	12.990	3698	3701	3706	rVB3	835	589	0.03%	0.004%
90	13.019	3706	3710	3712	rBV2	757	719	0.03%	0.004%
91	13.074	3725	3727	3731	rVB3	1070	686	0.03%	0.004%
92	13.167	3754	3756	3763	rVB3	1160	1075	0.05%	0.007%
93	13.199	3763	3766	3767	rBV2	1121	552	0.03%	0.003%
94	13.260	3781	3785	3787	rBV2	865	785	0.04%	0.005%
95	13.958	3997	4002	4004	rBV4	1129	1100	0.05%	0.007%
96	13.993	4011	4013	4016	rBV	879	622	0.03%	0.004%
97	14.058	4031	4033	4039	rVB2	1019	787	0.04%	0.005%
98	14.575	4192	4194	4196	rBV2	1116	587	0.03%	0.004%
99	14.649	4213	4217	4220	rBV4	914	871	0.04%	0.005%
100	15.167	4376	4378	4382	rBV3	1192	679	0.03%	0.004%


Sum of corrected areas: 16204710

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031063.D
Acq On : 11 Apr 2019 12:40
Operator : JC/SP
Sample : K2339-01 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

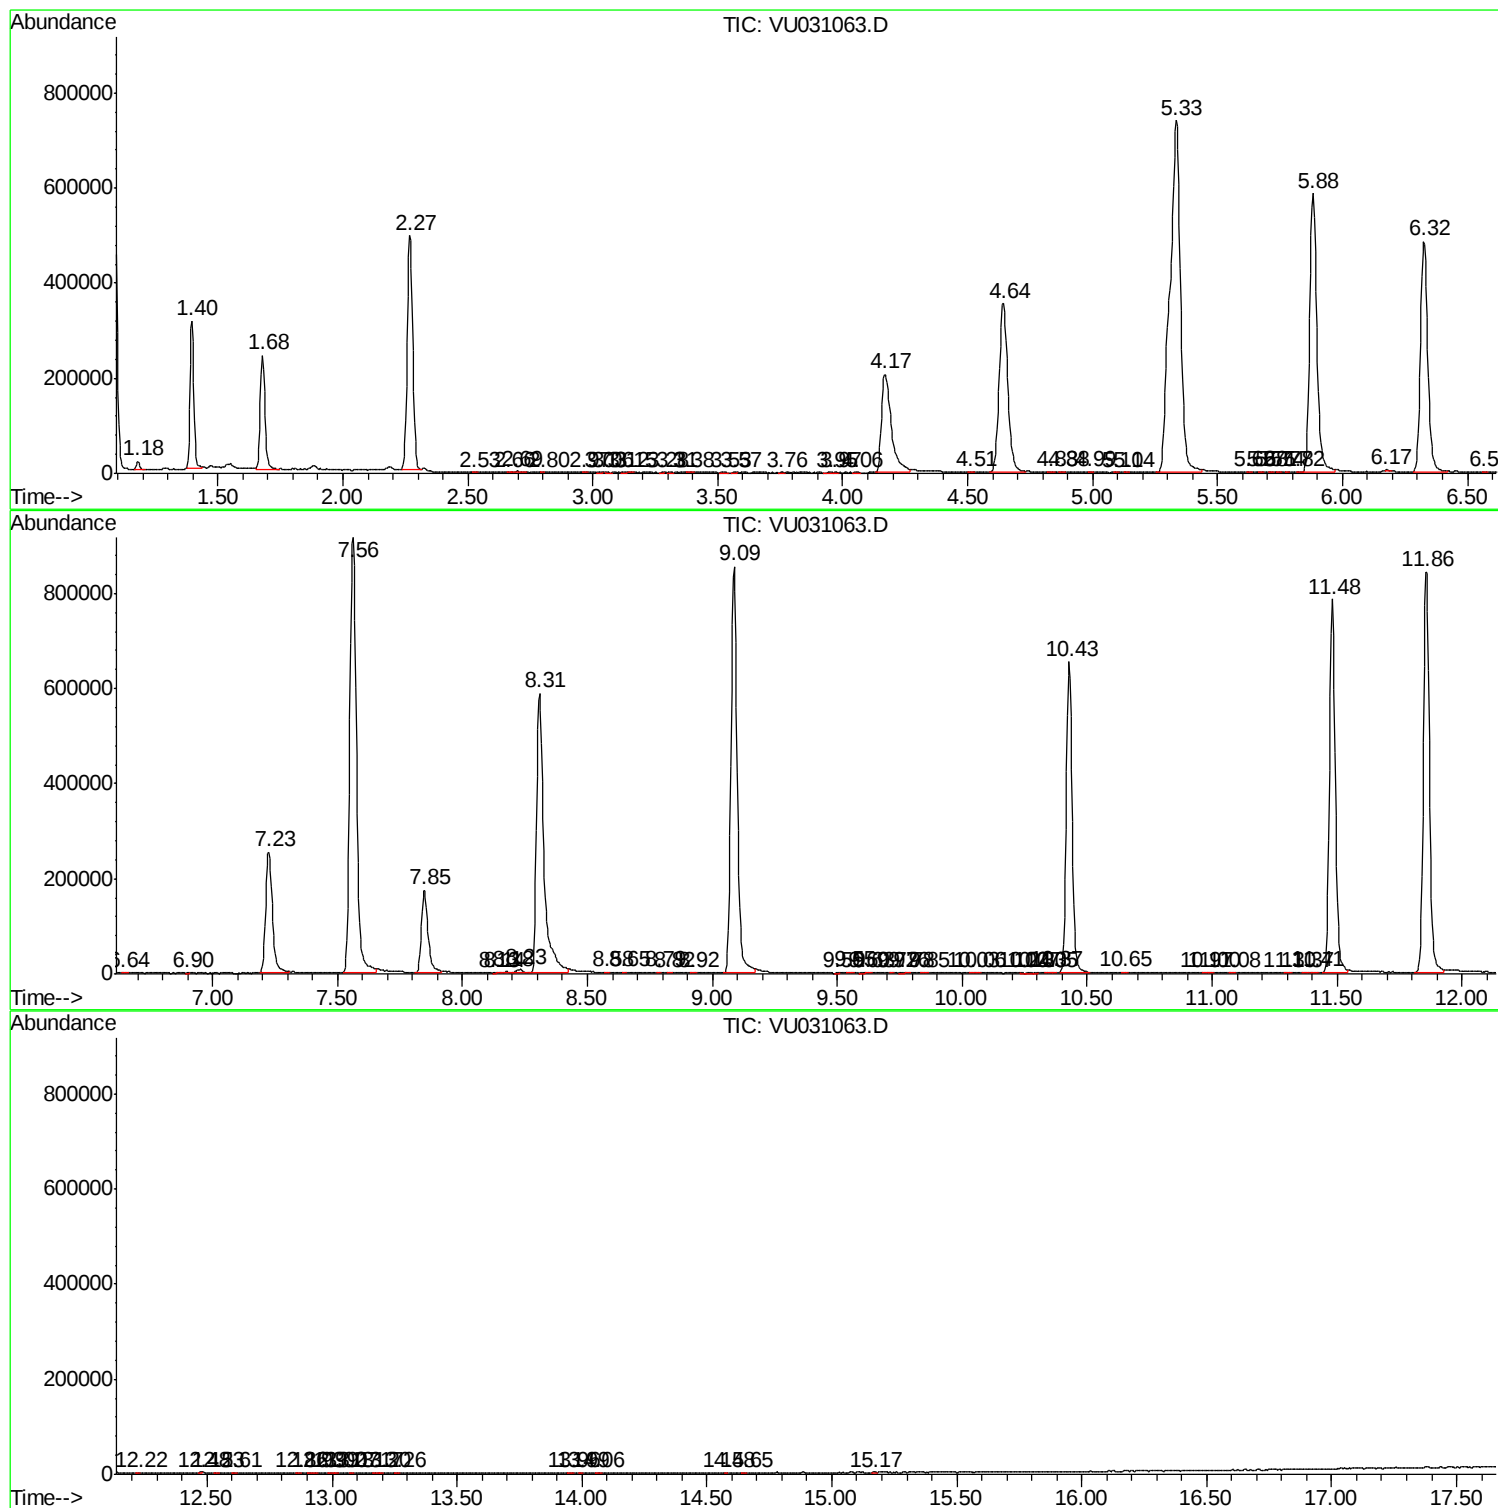

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031063.D
Acq On : 11 Apr 2019 12:40
Operator : JC/SP
Sample : K2339-01 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031063.D
Acq On : 11 Apr 2019 12:40
Operator : JC/SP
Sample : K2339-01 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC47

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc