

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031065.D
 Acq On : 11 Apr 2019 13:25
 Operator : JC/SP
 Sample : K2339-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	22	28	39	rBV	18036	17910	0.85%	0.115%
2	1.395	87	95	109	rBV	318066	329526	15.73%	2.115%
3	1.675	175	182	196	rVB	232999	297088	14.18%	1.907%
4	2.267	356	366	381	rVB	464303	697888	33.30%	4.479%
5	2.421	410	414	415	rBV3	584	476	0.02%	0.003%
6	2.566	455	459	463	rBV4	777	771	0.04%	0.005%
7	2.611	470	473	477	rBV3	800	565	0.03%	0.004%
8	2.701	493	501	506	rBV7	2302	3293	0.16%	0.021%
9	2.772	518	523	525	rBV3	1068	866	0.04%	0.006%
10	2.823	533	539	540	rBV3	1103	1014	0.05%	0.007%
11	2.900	560	563	570	rVB2	825	812	0.04%	0.005%
12	2.945	570	577	579	rBV4	1214	1171	0.06%	0.008%
13	3.016	593	599	603	rBV5	1113	1346	0.06%	0.009%
14	3.061	608	613	614	rBV2	655	524	0.03%	0.003%
15	3.402	715	719	723	rVB2	755	703	0.03%	0.005%
16	3.431	724	728	731	rBV2	730	548	0.03%	0.004%
17	3.540	760	762	767	rVB3	751	496	0.02%	0.003%
18	3.572	767	772	776	rBV3	588	521	0.02%	0.003%
19	3.707	810	814	819	rBV5	639	616	0.03%	0.004%
20	3.839	852	855	860	rBV2	835	755	0.04%	0.005%
21	4.016	904	910	913	rBV3	740	802	0.04%	0.005%
22	4.170	946	958	996	rBV2	194976	534976	25.53%	3.433%
23	4.530	1066	1070	1072	rBV4	831	717	0.03%	0.005%
24	4.643	1087	1105	1137	rBV2	335272	828927	39.56%	5.320%
25	4.932	1190	1195	1196	rBV2	613	452	0.02%	0.003%
26	5.042	1226	1229	1231	rVB2	804	492	0.02%	0.003%
27	5.074	1231	1239	1243	rBV4	926	1278	0.06%	0.008%
28	5.125	1248	1255	1257	rBV3	1201	1103	0.05%	0.007%
29	5.209	1279	1281	1288	rVB5	600	594	0.03%	0.004%
30	5.257	1292	1296	1297	rBV2	746	502	0.02%	0.003%
31	5.334	1297	1320	1345	rBV2	697492	2095531	100.00%	13.448%
32	5.559	1386	1390	1392	rBV5	1092	918	0.04%	0.006%
33	5.649	1416	1418	1422	rVB4	1204	832	0.04%	0.005%
34	5.675	1424	1426	1427	rBV2	973	471	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031065.D
 Acq On : 11 Apr 2019 13:25
 Operator : JC/SP
 Sample : K2339-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.881	1477	1490	1513	rBV	562588	1136505	54.23%	7.293%
36	6.180	1570	1583	1595	rBV10	4927	10892	0.52%	0.070%
37	6.325	1612	1628	1660	rBV	463666	960066	45.81%	6.161%
38	6.537	1691	1694	1697	rBV4	889	634	0.03%	0.004%
39	6.579	1705	1707	1711	rBV3	768	562	0.03%	0.004%
40	6.816	1779	1781	1784	rBV2	818	631	0.03%	0.004%
41	6.833	1784	1786	1793	rVV3	1079	946	0.05%	0.006%
42	6.903	1805	1808	1812	rVV2	762	657	0.03%	0.004%
43	6.961	1824	1826	1829	rVV	930	597	0.03%	0.004%
44	7.132	1875	1879	1886	rVB4	1017	1371	0.07%	0.009%
45	7.170	1888	1891	1896	rVB2	819	542	0.03%	0.003%
46	7.225	1896	1908	1928	rBV	243227	462472	22.07%	2.968%
47	7.456	1977	1980	1984	rBV4	814	789	0.04%	0.005%
48	7.562	1997	2013	2047	rBV	879386	1598743	76.29%	10.260%
49	7.845	2091	2101	2124	rBV	171283	307203	14.66%	1.971%
50	8.106	2180	2182	2187	rVB4	881	595	0.03%	0.004%
51	8.228	2210	2220	2230	rVB5	4277	8022	0.38%	0.051%
52	8.308	2234	2245	2290	rBV	583891	1184506	56.53%	7.602%
53	8.643	2347	2349	2354	rVB4	1068	607	0.03%	0.004%
54	8.723	2370	2374	2377	rVB3	791	670	0.03%	0.004%
55	8.765	2384	2387	2391	rVB3	819	507	0.02%	0.003%
56	8.791	2391	2395	2398	rBV3	691	640	0.03%	0.004%
57	8.810	2398	2401	2406	rVV4	987	850	0.04%	0.005%
58	8.839	2408	2410	2416	rVV3	757	571	0.03%	0.004%
59	8.877	2420	2422	2427	rVB2	629	472	0.02%	0.003%
60	8.900	2427	2429	2433	rBV4	744	606	0.03%	0.004%
61	9.086	2474	2487	2518	rBV	819044	1438955	68.67%	9.234%
62	9.321	2557	2560	2565	rBV2	800	771	0.04%	0.005%
63	9.392	2575	2582	2583	rBV3	1165	842	0.04%	0.005%
64	9.472	2604	2607	2613	rVB5	1422	1073	0.05%	0.007%
65	9.517	2614	2621	2625	rBV5	1005	1410	0.07%	0.009%
66	9.633	2655	2657	2661	rVB3	841	484	0.02%	0.003%
67	9.656	2661	2664	2667	rBV3	751	589	0.03%	0.004%
68	9.672	2667	2669	2674	rVB4	624	466	0.02%	0.003%
69	9.697	2674	2677	2679	rBV3	666	460	0.02%	0.003%
70	9.775	2697	2701	2703	rBV3	666	545	0.03%	0.003%
71	9.807	2708	2711	2714	rVB2	683	457	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031065.D
 Acq On : 11 Apr 2019 13:25
 Operator : JC/SP
 Sample : K2339-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	9.855	2721	2726	2732	rBV3	473	542	0.03%	0.003%
73	9.980	2762	2765	2769	rVB3	811	716	0.03%	0.005%
74	10.096	2797	2801	2805	rBV3	564	530	0.03%	0.003%
75	10.164	2818	2822	2828	rVB3	856	898	0.04%	0.006%
76	10.218	2835	2839	2842	rBV2	457	454	0.02%	0.003%
77	10.366	2881	2885	2889	rBV3	1102	979	0.05%	0.006%
78	10.427	2889	2904	2927	rBV	622672	1025484	48.94%	6.581%
79	10.614	2960	2962	2969	rVB5	1392	1254	0.06%	0.008%
80	10.762	3006	3008	3015	rVB4	658	605	0.03%	0.004%
81	10.794	3015	3018	3022	rVB2	650	577	0.03%	0.004%
82	10.820	3022	3026	3031	rBV3	1067	1092	0.05%	0.007%
83	10.881	3042	3045	3049	rVB2	888	752	0.04%	0.005%
84	10.913	3049	3055	3057	rBV3	703	780	0.04%	0.005%
85	11.022	3085	3089	3092	rVB2	606	508	0.02%	0.003%
86	11.086	3102	3109	3114	rBV7	1095	1283	0.06%	0.008%
87	11.131	3120	3123	3127	rBV4	796	525	0.03%	0.003%
88	11.315	3174	3180	3184	rBV2	786	858	0.04%	0.006%
89	11.479	3220	3231	3251	rBV	746084	1237178	59.04%	7.940%
90	11.858	3336	3349	3379	rBV	801974	1349145	64.38%	8.658%
91	12.459	3534	3536	3538	rBV2	943	606	0.03%	0.004%
92	12.549	3561	3564	3565	rBV2	891	542	0.03%	0.003%
93	12.739	3619	3623	3625	rBV2	998	739	0.04%	0.005%
94	12.807	3641	3644	3646	rBV2	798	536	0.03%	0.003%
95	12.887	3667	3669	3673	rBV4	733	600	0.03%	0.004%
96	13.170	3753	3757	3759	rBV2	808	699	0.03%	0.004%
97	13.572	3878	3882	3886	rVB2	1264	992	0.05%	0.006%
98	14.360	4123	4127	4132	rBV6	1163	1201	0.06%	0.008%
99	14.585	4194	4197	4199	rBV2	981	556	0.03%	0.004%
100	14.755	4247	4250	4252	rBV3	1210	698	0.03%	0.004%


Sum of corrected areas: 15582521

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031065.D
Acq On : 11 Apr 2019 13:25
Operator : JC/SP
Sample : K2339-03 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC55

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

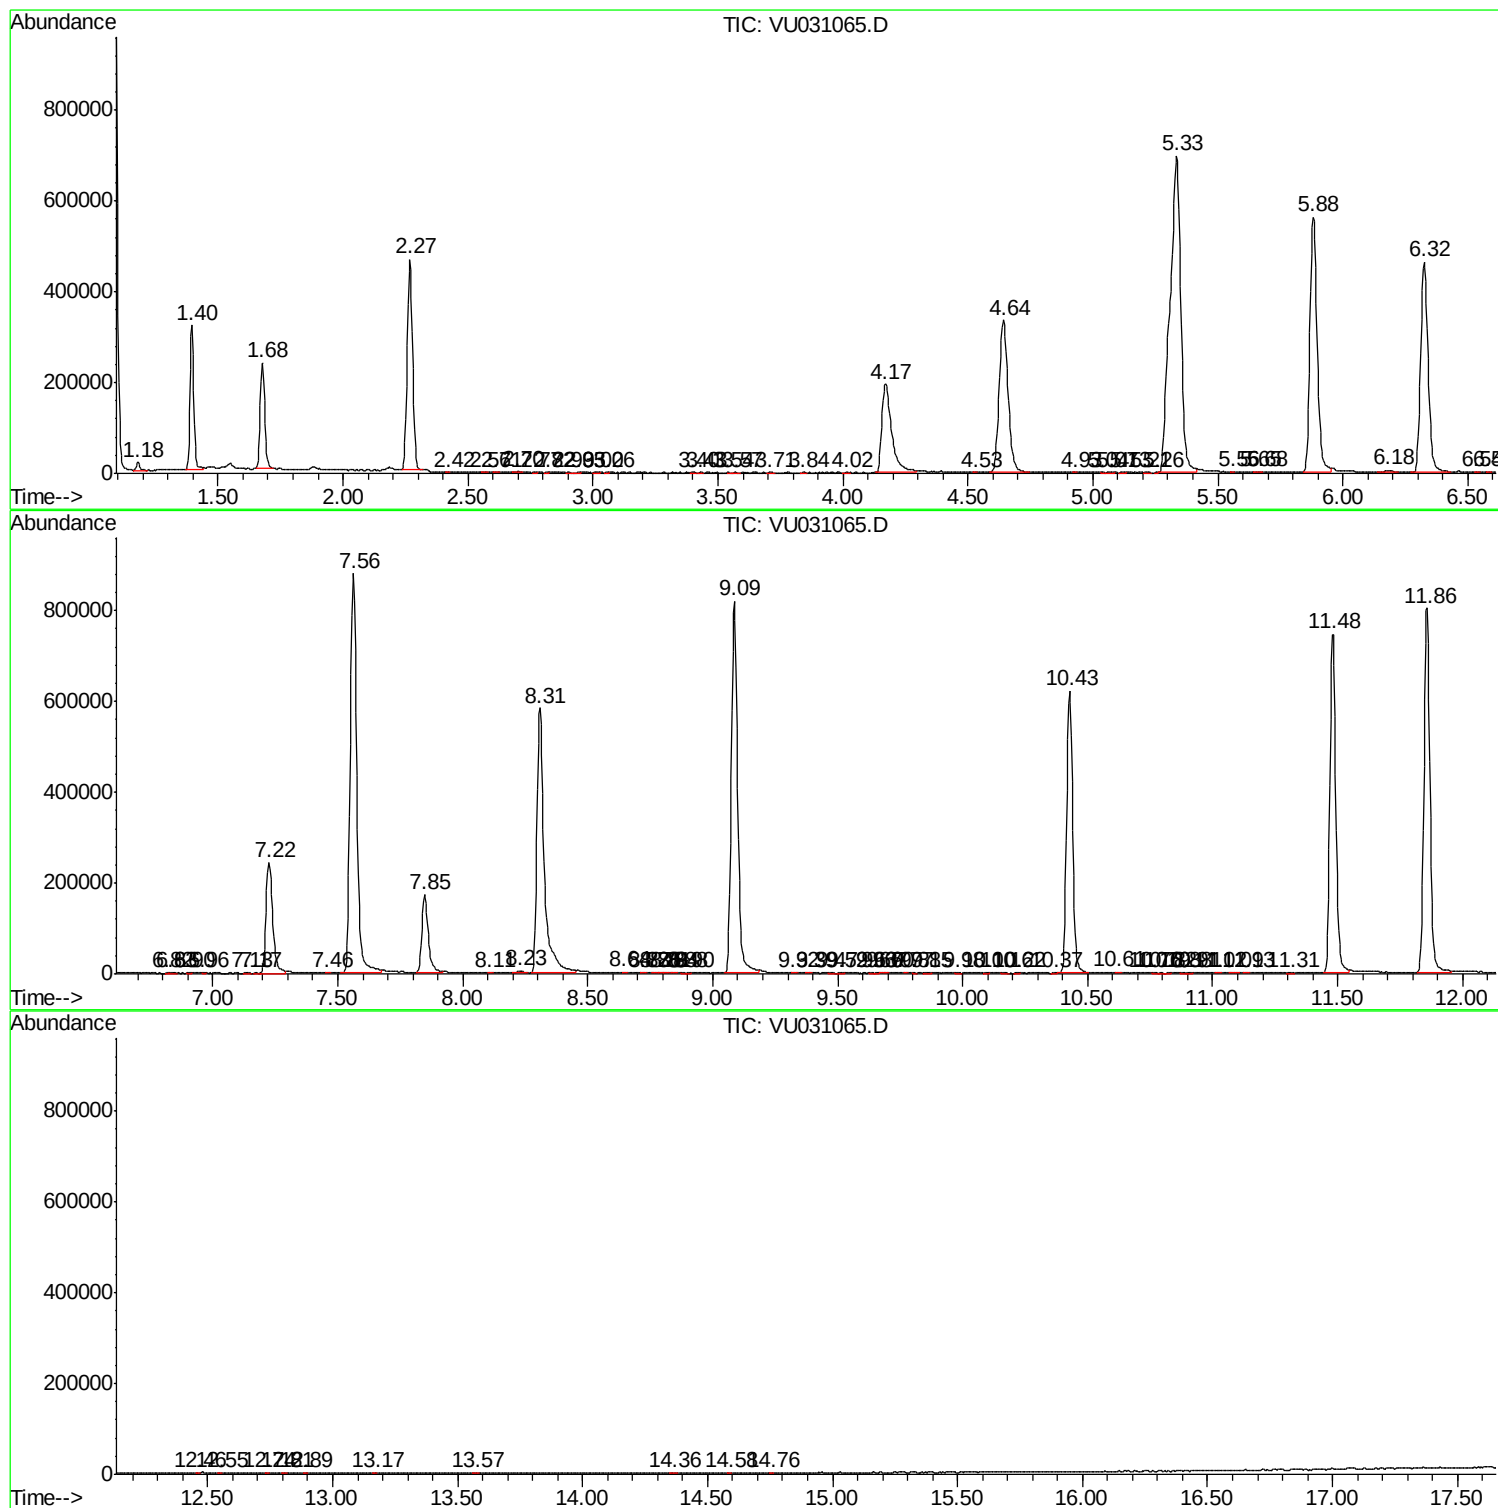

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031065.D
Acq On : 11 Apr 2019 13:25
Operator : JC/SP
Sample : K2339-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC55

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031065.D
Acq On : 11 Apr 2019 13:25
Operator : JC/SP
Sample : K2339-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC55

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc