

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031074.D
 Acq On : 11 Apr 2019 17:22
 Operator : JC/SP
 Sample : K2341-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB744

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB	19767	18130	0.97%	0.125%
2	1.396	88	95	106	rBV	240985	249111	13.28%	1.717%
3	1.675	175	182	196	rVB	199581	256608	13.68%	1.769%
4	2.267	356	366	379	rVB	392842	595943	31.77%	4.108%
5	2.633	478	480	482	rBV2	443	256	0.01%	0.002%
6	2.781	524	526	530	rBV2	749	445	0.02%	0.003%
7	2.807	531	534	535	rBV2	996	624	0.03%	0.004%
8	2.871	551	554	559	rVB4	879	742	0.04%	0.005%
9	2.977	583	587	588	rBV2	837	601	0.03%	0.004%
10	3.103	623	626	629	rBV3	940	656	0.03%	0.005%
11	3.238	666	668	672	rVB3	405	212	0.01%	0.001%
12	3.418	721	724	726	rBV2	562	357	0.02%	0.002%
13	3.576	769	773	774	rBV	931	647	0.03%	0.004%
14	3.730	818	821	824	rBV2	542	408	0.02%	0.003%
15	3.778	834	836	839	rBV	342	197	0.01%	0.001%
16	3.830	848	852	859	rBV4	846	869	0.05%	0.006%
17	3.858	859	861	863	rVB	419	179	0.01%	0.001%
18	3.878	863	867	869	rBV2	614	504	0.03%	0.003%
19	3.910	874	877	878	rBV	364	173	0.01%	0.001%
20	4.013	904	909	910	rBV2	513	417	0.02%	0.003%
21	4.042	914	918	919	rBV	285	211	0.01%	0.001%
22	4.074	926	928	932	rVB3	510	333	0.02%	0.002%
23	4.100	934	936	940	rBV3	605	424	0.02%	0.003%
24	4.170	947	958	991	rBV	201861	547212	29.17%	3.772%
25	4.640	1089	1104	1129	rBV	308474	747170	39.83%	5.151%
26	4.997	1212	1215	1217	rBV2	544	379	0.02%	0.003%
27	5.022	1221	1223	1228	rVB2	458	374	0.02%	0.003%
28	5.048	1229	1231	1233	rVB2	321	114	0.01%	0.001%
29	5.061	1233	1235	1237	rBV3	516	226	0.01%	0.002%
30	5.186	1271	1274	1278	rBV2	936	692	0.04%	0.005%
31	5.241	1287	1291	1292	rBV	399	231	0.01%	0.002%
32	5.334	1295	1320	1342	rBV2	623319	1876067	100.00%	12.933%
33	5.881	1476	1490	1512	rBV	568579	1131266	60.30%	7.799%
34	6.325	1614	1628	1654	rBV	428306	876424	46.72%	6.042%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031074.D
 Acq On : 11 Apr 2019 17:22
 Operator : JC/SP
 Sample : K2341-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB744

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.617	1715	1719	1721	rBV3	758	529	0.03%	0.004%
36	6.630	1721	1723	1726	rBV2	991	694	0.04%	0.005%
37	6.839	1785	1788	1794	rBV3	738	759	0.04%	0.005%
38	6.862	1794	1795	1796	rBV3	268	88	0.00%	0.001%
39	6.939	1816	1819	1824	rVB3	833	639	0.03%	0.004%
40	6.964	1824	1827	1833	rVB3	497	461	0.02%	0.003%
41	7.013	1840	1842	1843	rBV2	439	116	0.01%	0.001%
42	7.074	1859	1861	1862	rBV	223	93	0.00%	0.001%
43	7.180	1886	1894	1895	rBV4	612	666	0.04%	0.005%
44	7.225	1895	1908	1926	rBV	232455	422316	22.51%	2.911%
45	7.563	2001	2013	2035	rBV	769411	1366027	72.81%	9.417%
46	7.845	2086	2101	2126	rBV	157477	294895	15.72%	2.033%
47	8.308	2234	2245	2288	rBV	577262	1149226	61.26%	7.923%
48	8.836	2407	2409	2414	rVB2	746	307	0.02%	0.002%
49	8.929	2435	2438	2439	rBV2	734	447	0.02%	0.003%
50	8.993	2454	2458	2464	rVB3	1043	1045	0.06%	0.007%
51	9.022	2464	2467	2468	rBV2	744	457	0.02%	0.003%
52	9.087	2474	2487	2518	rBV	825749	1413879	75.36%	9.747%
53	9.466	2601	2605	2608	rBV3	568	552	0.03%	0.004%
54	9.620	2651	2653	2656	rBV2	598	465	0.02%	0.003%
55	9.807	2708	2711	2715	rBV2	772	638	0.03%	0.004%
56	10.096	2798	2801	2806	rBV2	735	692	0.04%	0.005%
57	10.218	2835	2839	2841	rBV3	811	587	0.03%	0.004%
58	10.324	2870	2872	2874	rVB	561	238	0.01%	0.002%
59	10.427	2891	2904	2929	rBV	605385	1003595	53.49%	6.919%
60	10.604	2950	2959	2969	rVB4	14844	24357	1.30%	0.168%
61	10.694	2984	2987	2988	rBV3	796	455	0.02%	0.003%
62	10.759	3003	3007	3008	rBV2	777	498	0.03%	0.003%
63	10.816	3016	3025	3033	rBV4	11913	18476	0.98%	0.127%
64	11.086	3105	3109	3117	rVB4	1158	1314	0.07%	0.009%
65	11.283	3166	3170	3172	rBV2	668	482	0.03%	0.003%
66	11.385	3199	3202	3206	rBV3	910	723	0.04%	0.005%
67	11.421	3208	3213	3215	rBV4	1918	1871	0.10%	0.013%
68	11.482	3220	3232	3263	rBV	747661	1244828	66.35%	8.582%
69	11.858	3337	3349	3371	rBV	738564	1243839	66.30%	8.575%
70	12.373	3506	3509	3512	rVB2	1454	818	0.04%	0.006%
71	13.000	3702	3704	3707	rBV	833	527	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031074.D
Acq On : 11 Apr 2019 17:22
Operator : JC/SP
Sample : K2341-17
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB744

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Title : VOC Analysis


Sum of corrected areas: 14505801

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031074.D
Acq On : 11 Apr 2019 17:22
Operator : JC/SP
Sample : K2341-17
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB744

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

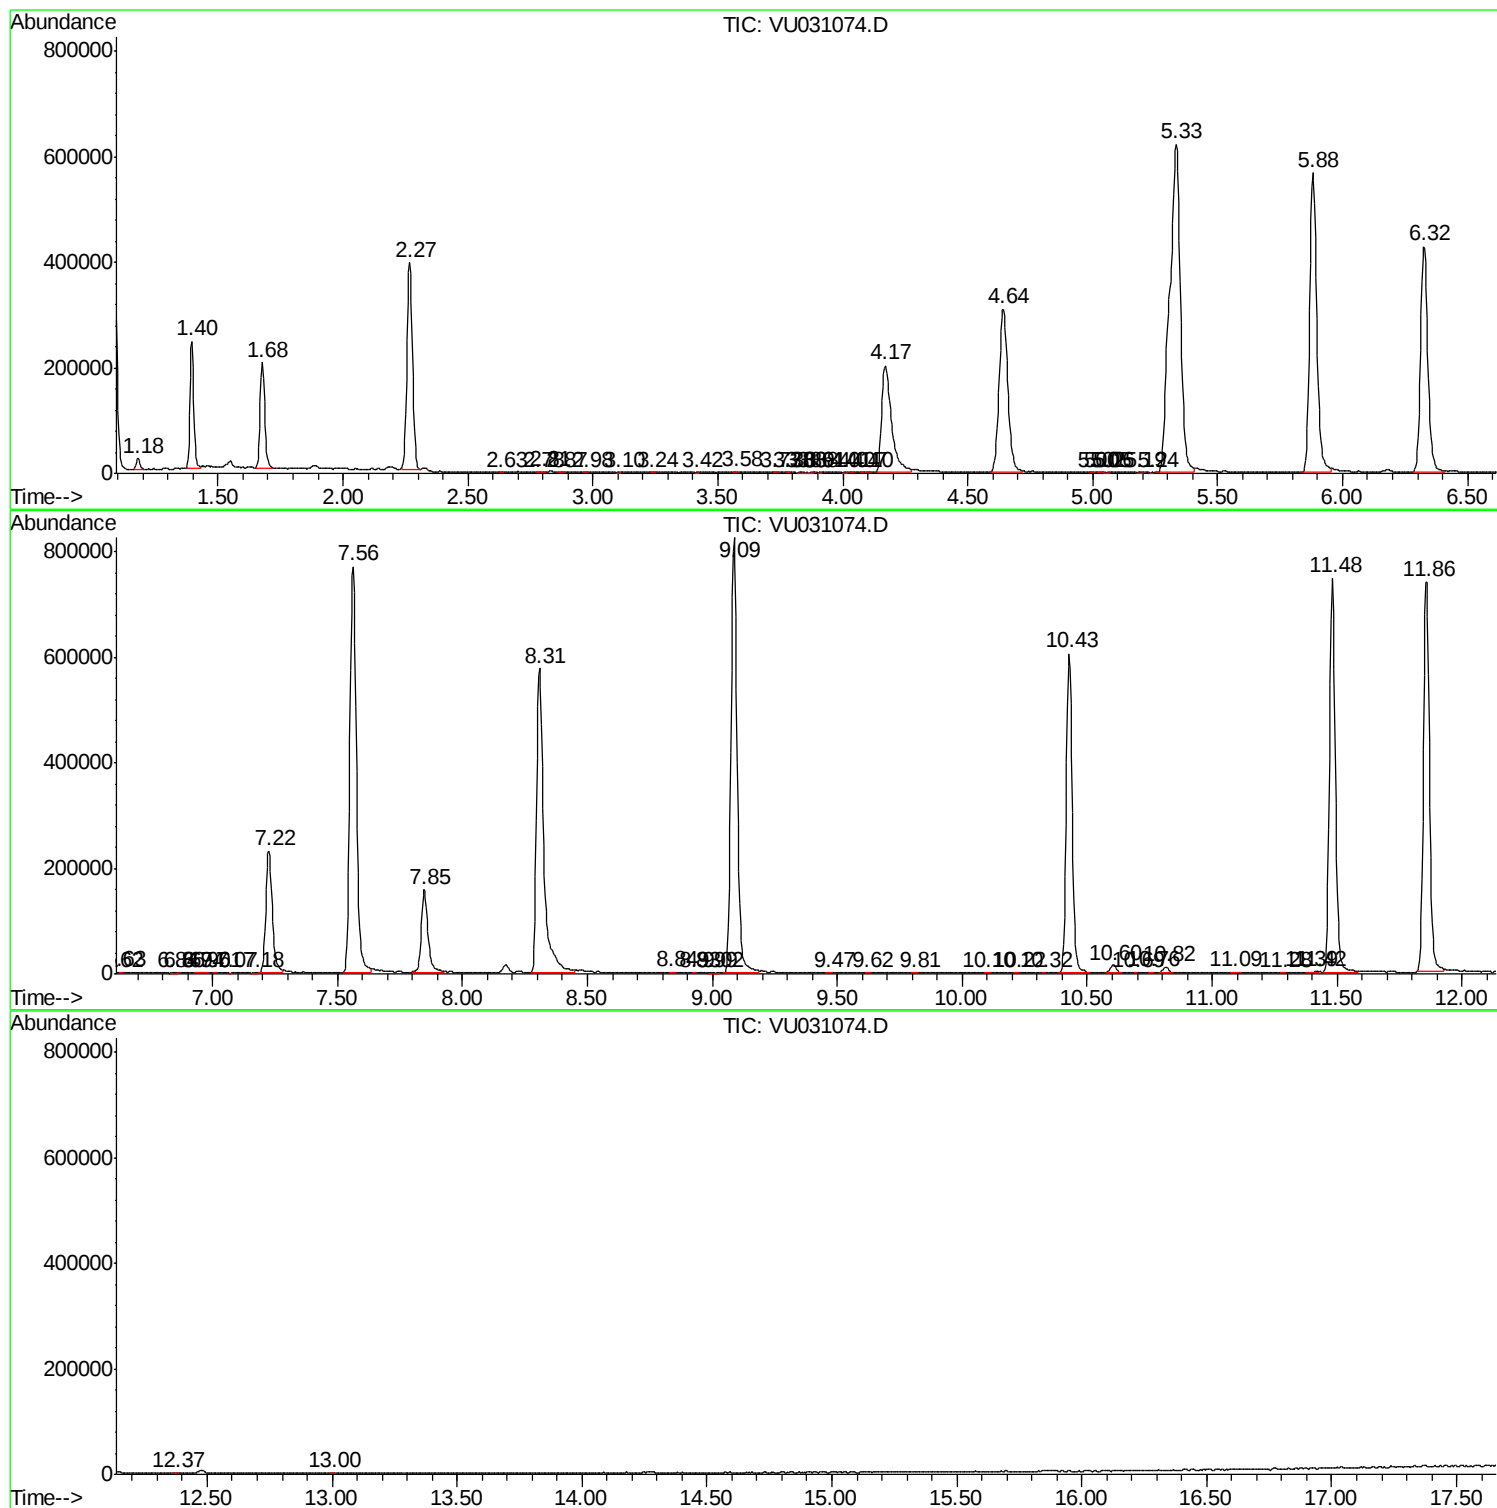

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031074.D
Acq On : 11 Apr 2019 17:22
Operator : JC/SP
Sample : K2341-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB744

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031074.D
Acq On : 11 Apr 2019 17:22
Operator : JC/SP
Sample : K2341-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB744

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc