

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031075.D
 Acq On : 11 Apr 2019 17:45
 Operator : JC/SP
 Sample : K2339-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	37	rVB3	19364	18443	0.99%	0.127%
2	1.396	88	95	105	rBV	236196	243922	13.13%	1.680%
3	1.675	175	182	197	rVB	197640	257556	13.87%	1.773%
4	2.267	356	366	378	rBV	377189	567422	30.55%	3.907%
5	2.441	411	420	439	rBV	19181	36860	1.98%	0.254%
6	2.826	533	540	541	rBV5	1811	2095	0.11%	0.014%
7	2.907	562	565	568	rBV2	575	513	0.03%	0.004%
8	2.933	569	573	576	rVV2	550	626	0.03%	0.004%
9	2.978	584	587	593	rVV4	806	735	0.04%	0.005%
10	3.093	620	623	628	rVB4	854	726	0.04%	0.005%
11	3.158	637	643	645	rBV5	772	758	0.04%	0.005%
12	3.293	681	685	687	rVV	858	572	0.03%	0.004%
13	3.305	687	689	694	rVB4	995	728	0.04%	0.005%
14	4.010	905	908	918	rVB3	801	1164	0.06%	0.008%
15	4.068	918	926	931	rBV4	1141	1187	0.06%	0.008%
16	4.170	944	958	994	rBV	199825	566656	30.51%	3.902%
17	4.402	1027	1030	1036	rVB4	1785	1243	0.07%	0.009%
18	4.498	1058	1060	1063	rVB2	1086	614	0.03%	0.004%
19	4.640	1088	1104	1134	rBV	306105	761987	41.03%	5.247%
20	4.823	1156	1161	1164	rBV5	1241	1142	0.06%	0.008%
21	4.842	1164	1167	1171	rBV4	1258	1045	0.06%	0.007%
22	5.042	1225	1229	1232	rBV3	621	517	0.03%	0.004%
23	5.119	1247	1253	1256	rVV5	579	623	0.03%	0.004%
24	5.235	1286	1289	1292	rBV2	846	617	0.03%	0.004%
25	5.334	1294	1320	1345	rBV2	617876	1857301	100.00%	12.788%
26	5.813	1467	1469	1475	rVB6	789	614	0.03%	0.004%
27	5.881	1475	1490	1517	rBV	550151	1117899	60.19%	7.697%
28	6.093	1554	1556	1559	rBV2	1089	566	0.03%	0.004%
29	6.174	1575	1581	1585	rBV7	2782	3699	0.20%	0.025%
30	6.325	1614	1628	1648	rBV	422525	857613	46.18%	5.905%
31	6.498	1679	1682	1687	rVV5	1241	1186	0.06%	0.008%
32	6.614	1714	1718	1721	rBV3	634	656	0.04%	0.005%
33	6.672	1733	1736	1740	rBV5	1010	867	0.05%	0.006%
34	6.736	1751	1756	1757	rBV2	901	674	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031075.D
 Acq On : 11 Apr 2019 17:45
 Operator : JC/SP
 Sample : K2339-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.797	1770	1775	1779	rVB2	658	645	0.03%	0.004%
36	6.974	1828	1830	1836	rVB4	871	664	0.04%	0.005%
37	7.045	1846	1852	1853	rBV2	727	650	0.03%	0.004%
38	7.058	1853	1856	1859	rVB2	970	571	0.03%	0.004%
39	7.225	1894	1908	1930	rBV2	223302	417476	22.48%	2.875%
40	7.434	1970	1973	1978	rVB4	1276	1229	0.07%	0.008%
41	7.563	1999	2013	2036	rBV	754401	1363225	73.40%	9.387%
42	7.807	2086	2089	2090	rBV2	930	520	0.03%	0.004%
43	7.845	2090	2101	2119	rVV	150858	278368	14.99%	1.917%
44	8.054	2162	2166	2173	rVB3	1197	1331	0.07%	0.009%
45	8.177	2193	2204	2213	rBV2	14980	27677	1.49%	0.191%
46	8.231	2213	2221	2227	rVB8	2889	4527	0.24%	0.031%
47	8.309	2234	2245	2282	rBV	561454	1139650	61.36%	7.847%
48	8.726	2372	2375	2378	rBV3	1141	606	0.03%	0.004%
49	8.804	2396	2399	2401	rBV2	903	615	0.03%	0.004%
50	8.836	2407	2409	2413	rVB3	808	543	0.03%	0.004%
51	8.929	2434	2438	2440	rBV2	997	662	0.04%	0.005%
52	8.977	2447	2453	2458	rBV5	571	794	0.04%	0.005%
53	9.003	2458	2461	2466	rVB3	1218	1201	0.06%	0.008%
54	9.087	2471	2487	2519	rBV	821907	1415687	76.22%	9.748%
55	9.228	2529	2531	2536	rVB4	1542	1159	0.06%	0.008%
56	9.254	2536	2539	2541	rBV3	1113	681	0.04%	0.005%
57	9.305	2552	2555	2557	rBV3	1183	734	0.04%	0.005%
58	9.376	2574	2577	2581	rBV4	955	635	0.03%	0.004%
59	9.501	2611	2616	2621	rVB3	857	981	0.05%	0.007%
60	9.527	2621	2624	2627	rBV3	879	564	0.03%	0.004%
61	9.791	2700	2706	2710	rVB5	880	800	0.04%	0.006%
62	9.910	2739	2743	2747	rBV5	730	715	0.04%	0.005%
63	9.961	2755	2759	2763	rBV2	796	677	0.04%	0.005%
64	9.997	2765	2770	2771	rBV	804	606	0.03%	0.004%
65	10.099	2799	2802	2805	rBV3	1027	695	0.04%	0.005%
66	10.202	2831	2834	2838	rVB2	899	663	0.04%	0.005%
67	10.273	2852	2856	2859	rVB3	682	621	0.03%	0.004%
68	10.331	2871	2874	2876	rBV	1036	585	0.03%	0.004%
69	10.344	2876	2878	2882	rVB2	1269	839	0.05%	0.006%
70	10.370	2882	2886	2888	rBV2	706	658	0.04%	0.005%
71	10.427	2891	2904	2931	rBV	600328	998589	53.77%	6.876%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031075.D
 Acq On : 11 Apr 2019 17:45
 Operator : JC/SP
 Sample : K2339-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.607	2949	2960	2974	rVB3	15224	26757	1.44%	0.184%
73	10.813	3017	3024	3033	rVV8	6389	9656	0.52%	0.066%
74	10.868	3039	3041	3048	rBV3	713	718	0.04%	0.005%
75	11.054	3095	3099	3104	rVB3	588	524	0.03%	0.004%
76	11.080	3104	3107	3108	rBV3	973	541	0.03%	0.004%
77	11.254	3159	3161	3168	rVB3	917	868	0.05%	0.006%
78	11.408	3207	3209	3212	rBV2	1363	902	0.05%	0.006%
79	11.479	3219	3231	3261	rBV	741225	1240910	66.81%	8.544%
80	11.855	3336	3348	3372	rVV	733248	1240829	66.81%	8.544%
81	12.418	3520	3523	3525	rBV3	1428	695	0.04%	0.005%
82	12.479	3536	3542	3551	rVB2	5684	7793	0.42%	0.054%
83	12.543	3560	3562	3567	rVB2	706	557	0.03%	0.004%
84	12.620	3583	3586	3591	rVB3	1299	719	0.04%	0.005%
85	12.820	3643	3648	3649	rBV2	837	681	0.04%	0.005%
86	12.881	3662	3667	3670	rBV2	2181	2100	0.11%	0.014%
87	12.929	3678	3682	3687	rBV3	1212	1452	0.08%	0.010%
88	13.096	3732	3734	3739	rVB3	739	540	0.03%	0.004%
89	13.308	3793	3800	3802	rBV4	763	914	0.05%	0.006%
90	13.398	3824	3828	3832	rBV3	666	699	0.04%	0.005%
91	13.466	3846	3849	3853	rBV3	795	619	0.03%	0.004%
92	13.517	3862	3865	3870	rBV3	723	556	0.03%	0.004%
93	13.771	3941	3944	3947	rBV3	663	568	0.03%	0.004%
94	14.273	4096	4100	4109	rVB6	2032	3006	0.16%	0.021%
95	14.414	4141	4144	4147	rBV3	1156	769	0.04%	0.005%
96	14.485	4163	4166	4168	rBV2	1007	608	0.03%	0.004%
97	14.540	4180	4183	4187	rBV4	1543	1333	0.07%	0.009%
98	14.877	4286	4288	4294	rVB5	1146	808	0.04%	0.006%
99	14.910	4295	4298	4300	rBV2	1419	875	0.05%	0.006%
100	14.926	4300	4303	4304	rBV	990	552	0.03%	0.004%


Sum of corrected areas: 14523218

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031075.D
Acq On : 11 Apr 2019 17:45
Operator : JC/SP
Sample : K2339-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

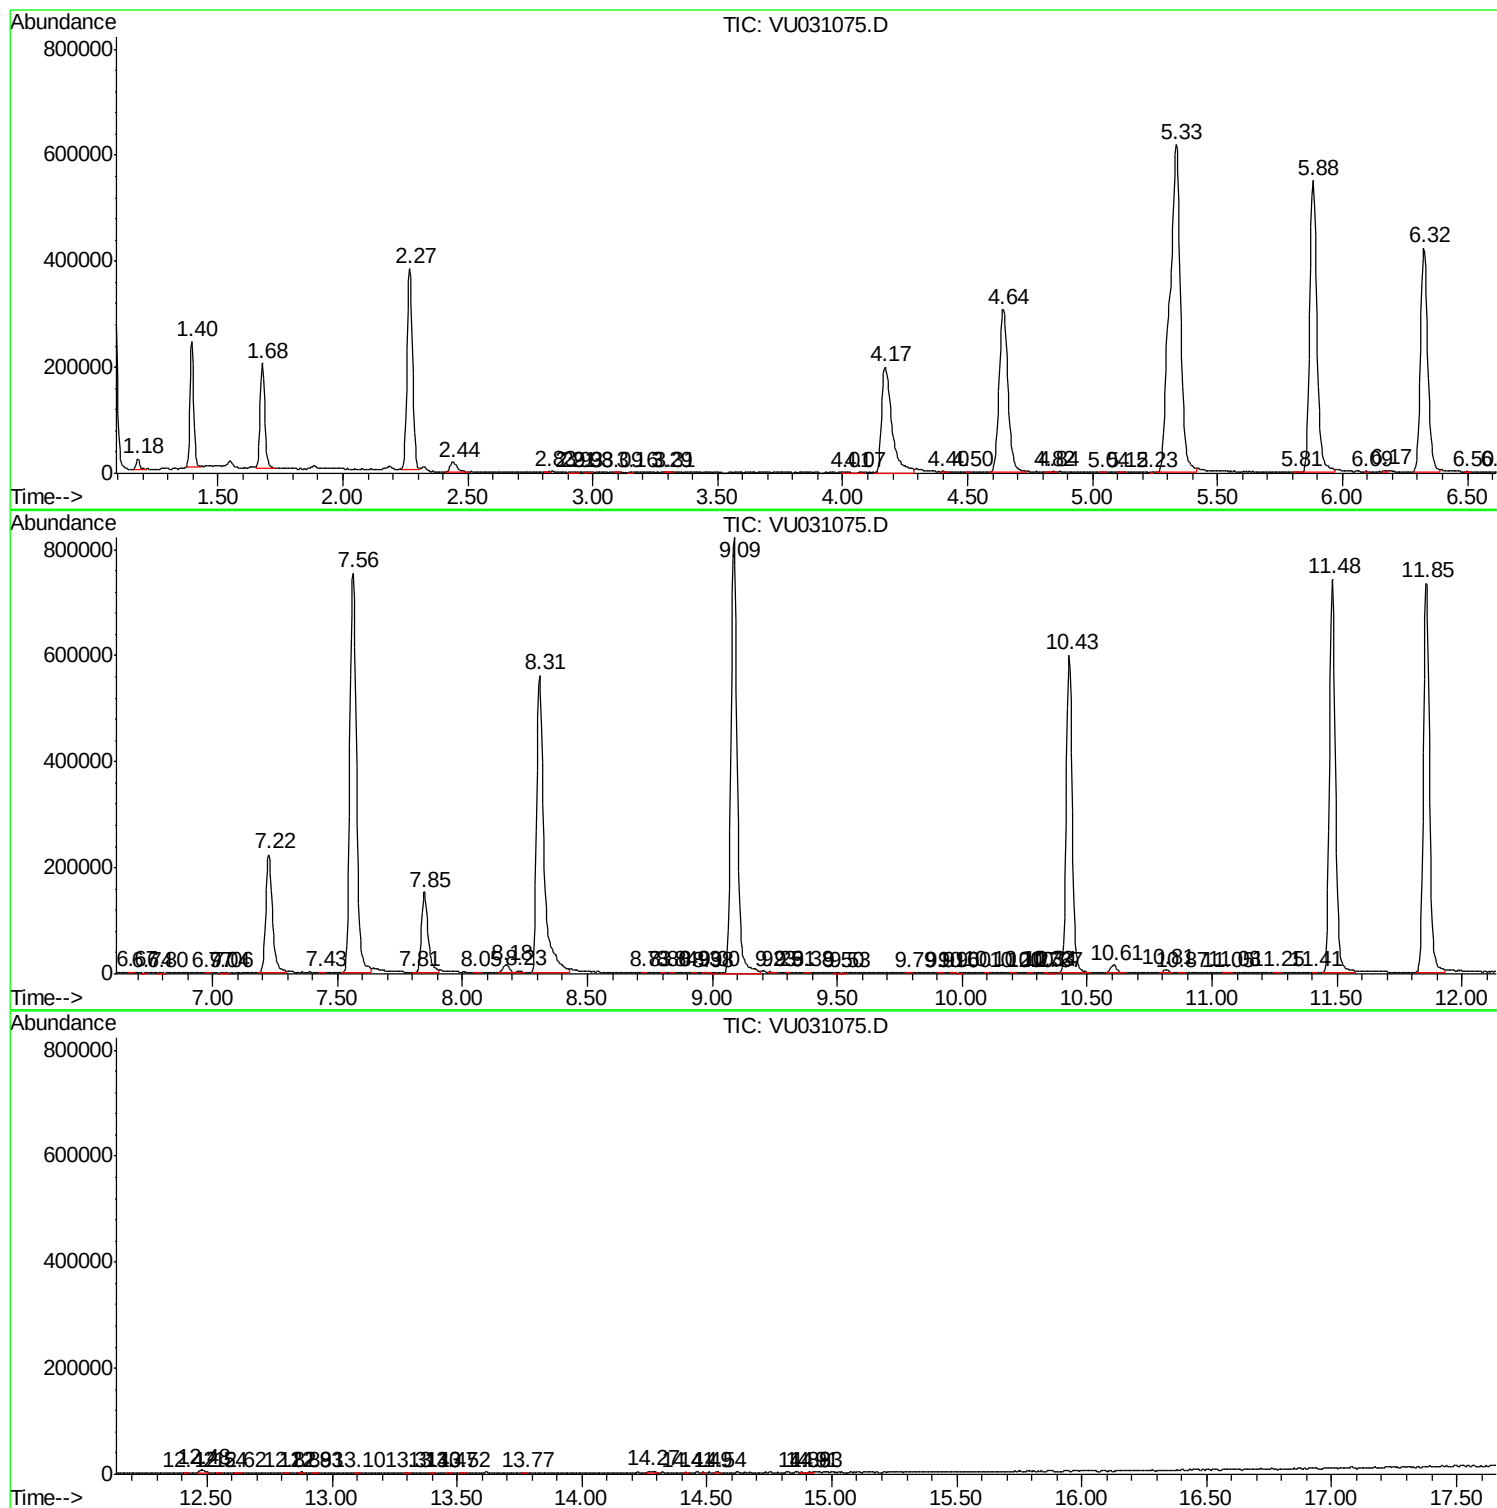

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031075.D
Acq On : 11 Apr 2019 17:45
Operator : JC/SP
Sample : K2339-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC67

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031075.D
Acq On : 11 Apr 2019 17:45
Operator : JC/SP
Sample : K2339-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 66 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC67

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc