

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031079.D
 Acq On : 11 Apr 2019 19:17
 Operator : JC/SP
 Sample : K2341-08DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB723DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	39	rVB3	19613	19837	1.09%	0.129%
2	1.396	88	95	110	rBV	236362	244687	13.40%	1.591%
3	1.470	114	118	127	rVB	11106	12937	0.71%	0.084%
4	1.679	174	183	198	rVB	193836	248784	13.63%	1.618%
5	2.267	355	366	378	rVB	388426	583772	31.98%	3.796%
6	2.441	412	420	436	rVB2	15750	27799	1.52%	0.181%
7	2.560	450	457	461	rBV5	1169	1386	0.08%	0.009%
8	2.695	492	499	500	rBV5	3094	2596	0.14%	0.017%
9	2.830	531	541	553	rBV5	2915	6378	0.35%	0.041%
10	3.084	617	620	623	rBV2	782	593	0.03%	0.004%
11	3.193	641	654	662	rBV8	3811	7902	0.43%	0.051%
12	3.280	675	681	686	rBV4	811	987	0.05%	0.006%
13	3.624	783	788	792	rVB4	803	753	0.04%	0.005%
14	3.936	881	885	889	rBV3	551	612	0.03%	0.004%
15	4.170	946	958	994	rBV2	197229	550216	30.14%	3.577%
16	4.495	1055	1059	1062	rBV4	896	729	0.04%	0.005%
17	4.518	1064	1066	1070	rVB4	934	639	0.04%	0.004%
18	4.550	1070	1076	1079	rBV4	977	966	0.05%	0.006%
19	4.643	1087	1105	1130	rBV	310021	788443	43.19%	5.126%
20	4.823	1157	1161	1164	rBV3	864	662	0.04%	0.004%
21	4.878	1170	1178	1182	rBV10	1190	1894	0.10%	0.012%
22	4.897	1182	1184	1190	rVB6	1178	1121	0.06%	0.007%
23	4.949	1196	1200	1203	rBV2	1058	869	0.05%	0.006%
24	5.051	1228	1232	1234	rBV3	850	494	0.03%	0.003%
25	5.100	1243	1247	1252	rVB5	810	799	0.04%	0.005%
26	5.129	1252	1256	1258	rBV4	867	647	0.04%	0.004%
27	5.334	1296	1320	1348	rBV2	601649	1825582	100.00%	11.870%
28	5.592	1395	1400	1403	rBV5	3337	3408	0.19%	0.022%
29	5.772	1445	1456	1464	rBV10	3322	6292	0.34%	0.041%
30	5.881	1476	1490	1514	rBV	540659	1096786	60.08%	7.131%
31	6.170	1573	1580	1581	rBV5	2897	3118	0.17%	0.020%
32	6.254	1603	1606	1610	rBV4	1205	1081	0.06%	0.007%
33	6.325	1615	1628	1653	rVV2	416005	845126	46.29%	5.495%
34	6.559	1698	1701	1706	rBV6	1226	1235	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031079.D
 Acq On : 11 Apr 2019 19:17
 Operator : JC/SP
 Sample : K2341-08DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB723DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.633	1722	1724	1726	rVB2	1407	594	0.03%	0.004%
36	6.759	1752	1763	1773	rVV2	10542	20048	1.10%	0.130%
37	6.830	1780	1785	1790	rBV3	1011	1267	0.07%	0.008%
38	6.868	1793	1797	1800	rBV3	745	528	0.03%	0.003%
39	6.971	1826	1829	1832	rBV	1069	833	0.05%	0.005%
40	7.180	1890	1894	1896	rBV2	670	517	0.03%	0.003%
41	7.225	1896	1908	1929	rBV	216035	400919	21.96%	2.607%
42	7.350	1944	1947	1952	rBV3	863	671	0.04%	0.004%
43	7.453	1975	1979	1980	rBV2	1126	720	0.04%	0.005%
44	7.563	2000	2013	2029	rBV	728875	1302869	71.37%	8.471%
45	7.849	2090	2102	2122	rBV	154608	277996	15.23%	1.807%
46	8.174	2193	2203	2206	rBV4	3711	5082	0.28%	0.033%
47	8.222	2206	2218	2235	rVV	601016	1046928	57.35%	6.807%
48	8.309	2235	2245	2285	rVV	554021	1146710	62.81%	7.456%
49	8.469	2289	2295	2314	rVB5	25458	47060	2.58%	0.306%
50	8.784	2391	2393	2396	rBV3	681	480	0.03%	0.003%
51	8.858	2412	2416	2419	rBV2	665	492	0.03%	0.003%
52	8.955	2442	2446	2449	rBV3	677	532	0.03%	0.003%
53	9.038	2467	2472	2474	rBV2	1092	894	0.05%	0.006%
54	9.087	2474	2487	2523	rBV	796826	1388282	76.05%	9.026%
55	9.289	2547	2550	2554	rBV5	766	596	0.03%	0.004%
56	9.453	2597	2601	2605	rVB3	751	578	0.03%	0.004%
57	9.527	2621	2624	2628	rVB3	802	569	0.03%	0.004%
58	9.704	2676	2679	2684	rVB2	828	632	0.03%	0.004%
59	9.746	2690	2692	2698	rVB3	809	608	0.03%	0.004%
60	9.788	2698	2705	2709	rBV6	1292	1576	0.09%	0.010%
61	9.810	2710	2712	2718	rVB5	678	595	0.03%	0.004%
62	10.051	2779	2787	2799	rBV10	1911	4513	0.25%	0.029%
63	10.196	2827	2832	2834	rBV2	466	483	0.03%	0.003%
64	10.427	2892	2904	2924	rBV	597098	971785	53.23%	6.318%
65	10.604	2950	2959	2965	rBV5	3266	5267	0.29%	0.034%
66	10.678	2978	2982	2985	rBV2	914	631	0.03%	0.004%
67	10.726	2993	2997	3002	rVB6	987	1128	0.06%	0.007%
68	10.759	3002	3007	3009	rBV3	1058	794	0.04%	0.005%
69	10.807	3016	3022	3023	rBV3	2182	1388	0.08%	0.009%
70	10.926	3055	3059	3062	rBV2	949	834	0.05%	0.005%
71	11.009	3080	3085	3088	rBV2	851	876	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031079.D
 Acq On : 11 Apr 2019 19:17
 Operator : JC/SP
 Sample : K2341-08DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB723DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	11.128	3118	3122	3123	rBV2	781	510	0.03%	0.003%
73	11.376	3191	3199	3201	rBV7	2515	2428	0.13%	0.016%
74	11.479	3220	3231	3250	rBV	740365	1209788	66.27%	7.866%
75	11.765	3317	3320	3323	rBV2	724	571	0.03%	0.004%
76	11.855	3336	3348	3372	rBV	715735	1219353	66.79%	7.928%
77	12.112	3425	3428	3434	rBV7	957	988	0.05%	0.006%
78	12.308	3484	3489	3492	rBV4	895	1165	0.06%	0.008%
79	12.415	3518	3522	3524	rVB3	845	667	0.04%	0.004%
80	12.472	3532	3540	3548	rBV7	2068	3197	0.18%	0.021%
81	12.781	3634	3636	3641	rBV3	1330	921	0.05%	0.006%
82	12.810	3641	3645	3648	rVV4	777	630	0.03%	0.004%
83	12.826	3648	3650	3655	rVV3	569	475	0.03%	0.003%
84	12.932	3679	3683	3688	rBV4	1052	970	0.05%	0.006%
85	12.990	3698	3701	3704	rBV2	830	657	0.04%	0.004%
86	13.041	3715	3717	3723	rBV3	1099	1080	0.06%	0.007%
87	13.122	3737	3742	3744	rBV2	1063	934	0.05%	0.006%
88	13.186	3758	3762	3763	rBV2	1069	558	0.03%	0.004%
89	13.443	3839	3842	3848	rBV3	953	1075	0.06%	0.007%
90	13.623	3894	3898	3904	rVV4	974	1020	0.06%	0.007%
91	13.662	3908	3910	3917	rVB2	780	662	0.04%	0.004%
92	13.726	3928	3930	3934	rBV3	779	496	0.03%	0.003%
93	13.749	3935	3937	3945	rVB5	1444	1415	0.08%	0.009%
94	13.897	3980	3983	3986	rVB3	1507	945	0.05%	0.006%
95	14.022	4019	4022	4024	rBV2	705	476	0.03%	0.003%
96	14.234	4085	4088	4093	rBV3	1134	1088	0.06%	0.007%
97	14.424	4144	4147	4151	rVB4	1335	899	0.05%	0.006%
98	14.447	4151	4154	4157	rBV3	870	674	0.04%	0.004%
99	14.861	4281	4283	4285	rBV2	1237	742	0.04%	0.005%
100	14.900	4293	4295	4298	rBV3	921	643	0.04%	0.004%


Sum of corrected areas: 15380432

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031079.D
Acq On : 11 Apr 2019 19:17
Operator : JC/SP
Sample : K2341-08DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB723DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

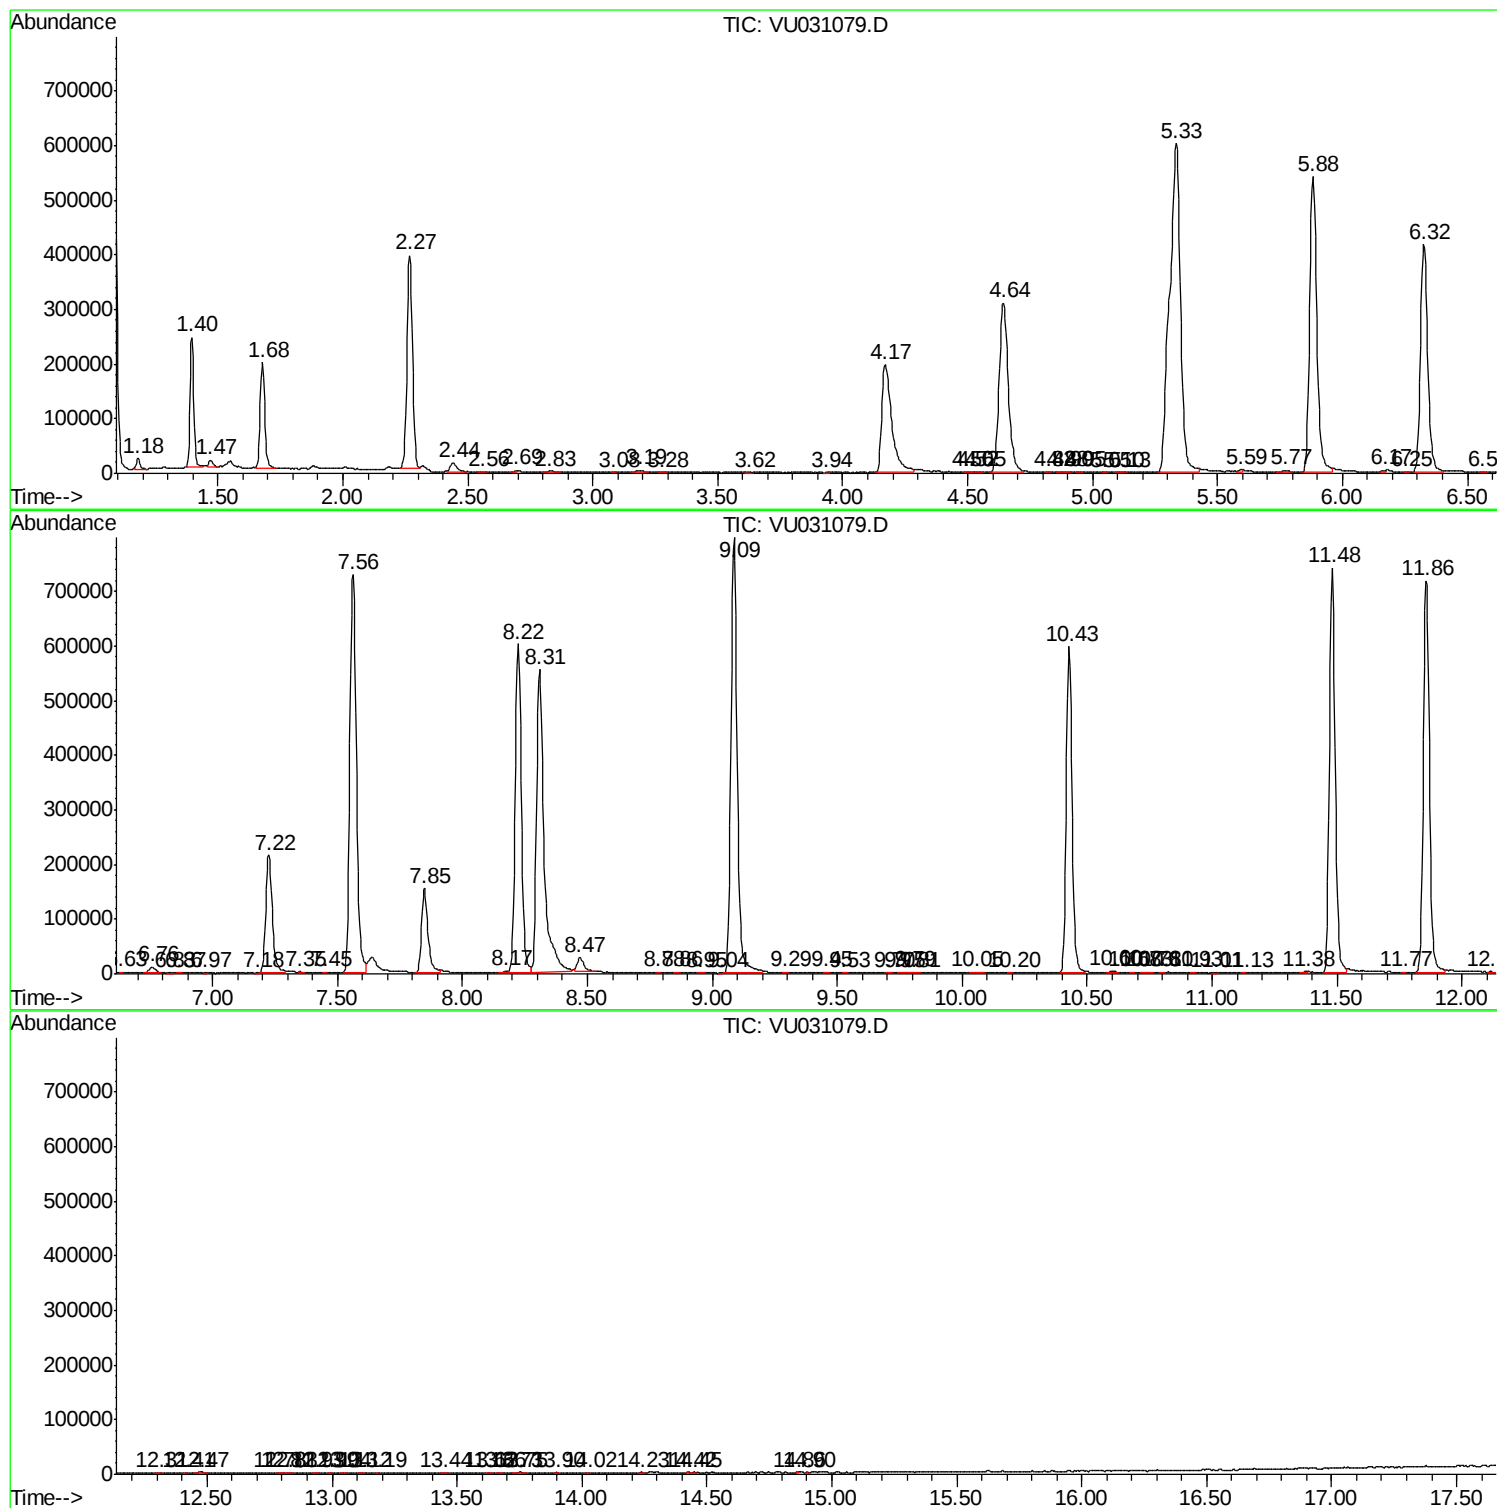

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031079.D
Acq On : 11 Apr 2019 19:17
Operator : JC/SP
Sample : K2341-08DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB723DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031079.D
Acq On : 11 Apr 2019 19:17
Operator : JC/SP
Sample : K2341-08DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 70 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB723DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc