

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031080.D
 Acq On : 11 Apr 2019 19:40
 Operator : JC/SP
 Sample : K2299-22DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6Z8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB	20755	20728	1.11%	0.132%
2	1.395	88	95	108	rBV	264613	272829	14.56%	1.742%
3	1.675	174	182	196	rVB	188186	253979	13.56%	1.622%
4	2.267	355	366	379	rBV	391122	601074	32.08%	3.838%
5	2.357	392	394	401	rVB6	1690	1410	0.08%	0.009%
6	2.437	411	419	428	rBV2	6246	10559	0.56%	0.067%
7	2.694	490	499	507	rBV7	3434	6398	0.34%	0.041%
8	2.823	534	539	542	rBV5	2544	2914	0.16%	0.019%
9	2.977	580	587	590	rBV5	2649	3252	0.17%	0.021%
10	3.804	840	844	852	rBV3	692	827	0.04%	0.005%
11	3.971	891	896	903	rVB4	915	1248	0.07%	0.008%
12	4.170	945	958	963	rBV	213878	424873	22.68%	2.713%
13	4.550	1073	1076	1080	rBV4	821	777	0.04%	0.005%
14	4.640	1086	1104	1132	rBV	311598	773350	41.28%	4.939%
15	4.881	1174	1179	1181	rBV6	973	945	0.05%	0.006%
16	4.939	1191	1197	1201	rBV4	1138	930	0.05%	0.006%
17	4.974	1203	1208	1209	rBV3	1673	1240	0.07%	0.008%
18	5.006	1215	1218	1224	rVB5	1728	1336	0.07%	0.009%
19	5.109	1245	1250	1255	rVB4	827	822	0.04%	0.005%
20	5.334	1297	1320	1342	rBV2	621162	1873550	100.00%	11.964%
21	5.550	1383	1387	1388	rBV2	1099	780	0.04%	0.005%
22	5.704	1432	1435	1438	rBV3	886	886	0.05%	0.006%
23	5.749	1444	1449	1454	rBV5	843	990	0.05%	0.006%
24	5.881	1477	1490	1516	rBV	553173	1109753	59.23%	7.087%
25	6.183	1568	1584	1605	rBV	364359	725882	38.74%	4.635%
26	6.325	1614	1628	1649	rBV	431260	870159	46.44%	5.557%
27	6.530	1689	1692	1696	rBV3	1702	1357	0.07%	0.009%
28	6.607	1713	1716	1721	rVB6	1009	768	0.04%	0.005%
29	6.897	1804	1806	1810	rVV4	841	744	0.04%	0.005%
30	7.032	1844	1848	1852	rVB3	853	697	0.04%	0.004%
31	7.128	1874	1878	1882	rBV4	838	683	0.04%	0.004%
32	7.225	1896	1908	1925	rBV	225946	415747	22.19%	2.655%
33	7.431	1967	1972	1973	rBV3	914	754	0.04%	0.005%
34	7.562	1999	2013	2031	rBV	755106	1349316	72.02%	8.617%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031080.D
 Acq On : 11 Apr 2019 19:40
 Operator : JC/SP
 Sample : K2299-22DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6Z8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	7.849	2091	2102	2122	rBV	157941	290213	15.49%	1.853%
36	8.019	2152	2155	2160	rVB5	1049	795	0.04%	0.005%
37	8.115	2180	2185	2190	rBV4	1159	1046	0.06%	0.007%
38	8.170	2190	2202	2208	rBV4	3696	4781	0.26%	0.031%
39	8.225	2208	2219	2233	rBV3	81452	136920	7.31%	0.874%
40	8.308	2235	2245	2280	rBV	577615	1154895	61.64%	7.375%
41	8.765	2385	2387	2392	rVB5	1015	789	0.04%	0.005%
42	8.845	2408	2412	2416	rBV3	946	883	0.05%	0.006%
43	8.935	2437	2440	2444	rBV3	932	658	0.04%	0.004%
44	8.968	2444	2450	2452	rBV3	1193	1238	0.07%	0.008%
45	8.980	2452	2454	2461	rVB4	674	742	0.04%	0.005%
46	9.086	2474	2487	2512	rBV	812120	1395184	74.47%	8.910%
47	9.250	2533	2538	2542	rBV6	2778	3384	0.18%	0.022%
48	9.440	2595	2597	2606	rVB3	815	897	0.05%	0.006%
49	9.820	2713	2715	2724	rVB3	798	676	0.04%	0.004%
50	9.868	2727	2730	2734	rBV2	675	672	0.04%	0.004%
51	9.903	2734	2741	2744	rVB4	919	1041	0.06%	0.007%
52	9.980	2760	2765	2767	rBV2	862	712	0.04%	0.005%
53	10.038	2775	2783	2786	rBV4	961	1107	0.06%	0.007%
54	10.167	2812	2823	2833	rBV6	6623	11856	0.63%	0.076%
55	10.292	2857	2862	2865	rBV4	1094	922	0.05%	0.006%
56	10.427	2891	2904	2927	rBV	613446	1009354	53.87%	6.446%
57	10.701	2985	2989	2993	rBV6	1067	913	0.05%	0.006%
58	10.749	3000	3004	3009	rVB3	940	721	0.04%	0.005%
59	10.813	3019	3024	3026	rBV4	1767	1708	0.09%	0.011%
60	10.861	3035	3039	3045	rVB4	906	771	0.04%	0.005%
61	10.894	3045	3049	3054	rBV3	975	1062	0.06%	0.007%
62	10.974	3065	3074	3084	rVV3	6634	10222	0.55%	0.065%
63	11.019	3084	3088	3093	rVB2	825	767	0.04%	0.005%
64	11.321	3177	3182	3190	rVB3	4252	5966	0.32%	0.038%
65	11.479	3219	3231	3256	rBV	760452	1239326	66.15%	7.914%
66	11.691	3293	3297	3302	rBV6	843	953	0.05%	0.006%
67	11.765	3311	3320	3331	rBV4	15893	31434	1.68%	0.201%
68	11.855	3336	3348	3369	rBV	761967	1290835	68.90%	8.243%
69	12.128	3429	3433	3435	rBV3	1180	881	0.05%	0.006%
70	12.147	3436	3439	3442	rVV4	1589	1262	0.07%	0.008%
71	12.202	3452	3456	3459	rBV4	1154	973	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031080.D
 Acq On : 11 Apr 2019 19:40
 Operator : JC/SP
 Sample : K2299-22DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6Z8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	12.250	3465	3471	3477	rBV4	7267	9734	0.52%	0.062%
73	12.353	3495	3503	3510	rBV2	12261	17912	0.96%	0.114%
74	12.453	3529	3534	3535	rBV3	1105	715	0.04%	0.005%
75	12.492	3544	3546	3551	rVB4	1581	1019	0.05%	0.007%
76	12.537	3558	3560	3565	rVB5	1708	1306	0.07%	0.008%
77	12.559	3565	3567	3578	rVB5	1114	1327	0.07%	0.008%
78	12.646	3589	3594	3601	rBV2	4939	6097	0.33%	0.039%
79	12.701	3604	3611	3622	rVB3	10101	16451	0.88%	0.105%
80	12.781	3633	3636	3637	rBV2	1479	958	0.05%	0.006%
81	12.877	3660	3666	3669	rBV6	1506	1517	0.08%	0.010%
82	12.919	3674	3679	3682	rBV4	1325	1365	0.07%	0.009%
83	12.967	3688	3694	3695	rBV4	3900	3949	0.21%	0.025%
84	13.061	3721	3723	3725	rBV2	1226	765	0.04%	0.005%
85	13.125	3734	3743	3753	rBV4	15727	26587	1.42%	0.170%
86	13.286	3784	3793	3806	rBV4	25024	38885	2.08%	0.248%
87	13.456	3843	3846	3853	rVB7	3272	3351	0.18%	0.021%
88	13.508	3857	3862	3874	rVV7	4004	6481	0.35%	0.041%
89	13.575	3879	3883	3887	rBV6	2412	2607	0.14%	0.017%
90	13.749	3925	3937	3961	rBV	22728	58249	3.11%	0.372%
91	13.948	3992	3999	4009	rBV9	6764	9330	0.50%	0.060%
92	14.003	4014	4016	4020	rBV4	1411	1148	0.06%	0.007%
93	14.135	4054	4057	4058	rBV2	1400	692	0.04%	0.004%
94	14.353	4112	4125	4138	rBV2	9901	21528	1.15%	0.137%
95	14.475	4158	4163	4165	rBV3	2300	2304	0.12%	0.015%
96	14.546	4179	4185	4194	rVB9	4145	6852	0.37%	0.044%
97	14.681	4217	4227	4236	rBV9	9814	18403	0.98%	0.118%
98	14.752	4247	4249	4256	rVB5	1614	1163	0.06%	0.007%
99	14.893	4287	4293	4299	rBV5	7924	12030	0.64%	0.077%
100	15.067	4334	4347	4363	rBV2	18904	48585	2.59%	0.310%


Sum of corrected areas: 15659426

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031080.D
Acq On : 11 Apr 2019 19:40
Operator : JC/SP
Sample : K2299-22DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6Z8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

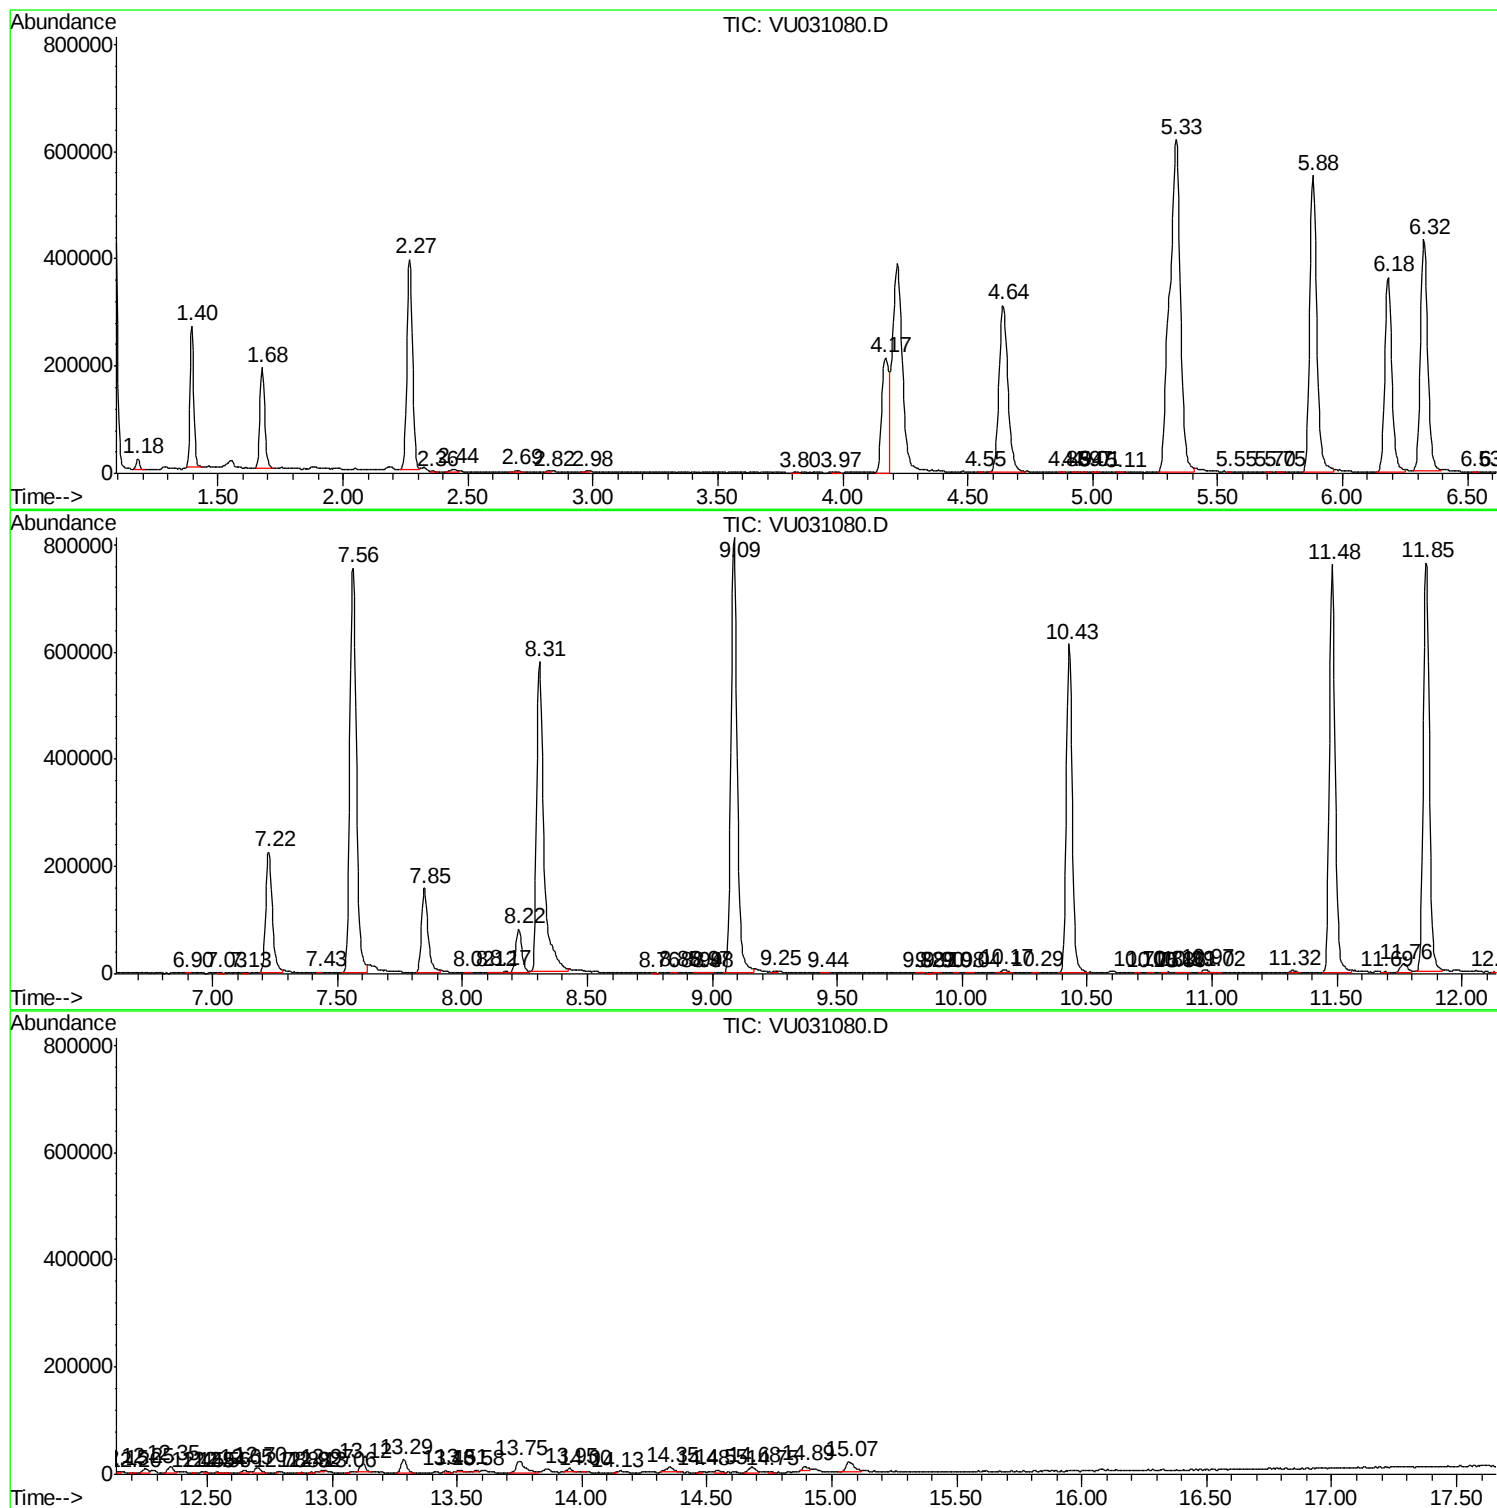

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031080.D
Acq On : 11 Apr 2019 19:40
Operator : JC/SP
Sample : K2299-22DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6Z8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031080.D
Acq On : 11 Apr 2019 19:40
Operator : JC/SP
Sample : K2299-22DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6Z8DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc