

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031082.D
 Acq On : 11 Apr 2019 20:25
 Operator : JC/SP
 Sample : K2341-07DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB722DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	37	rVB	19331	18856	1.01%	0.120%
2	1.396	87	95	108	rBV	233684	255717	13.74%	1.625%
3	1.675	174	182	196	rBV	189162	243878	13.11%	1.550%
4	2.267	355	366	379	rVB	377771	577190	31.02%	3.668%
5	2.380	398	401	404	rBV2	969	528	0.03%	0.003%
6	2.441	415	420	438	rVB4	3636	5744	0.31%	0.037%
7	2.675	490	493	494	rVV2	920	545	0.03%	0.003%
8	2.701	495	501	510	rVB7	2992	5162	0.28%	0.033%
9	2.749	512	516	519	rBV4	723	527	0.03%	0.003%
10	2.823	535	539	541	rBV3	1152	933	0.05%	0.006%
11	2.897	558	562	566	rVB4	745	505	0.03%	0.003%
12	2.974	580	586	588	rBV5	2426	2252	0.12%	0.014%
13	3.161	641	644	647	rVB2	1237	855	0.05%	0.005%
14	3.267	670	677	680	rBV5	675	664	0.04%	0.004%
15	3.595	773	779	784	rVB3	775	1064	0.06%	0.007%
16	3.637	784	792	797	rBV2	672	737	0.04%	0.005%
17	3.804	839	844	846	rBV2	801	575	0.03%	0.004%
18	3.868	860	864	868	rBV2	504	521	0.03%	0.003%
19	3.900	868	874	877	rBV4	512	515	0.03%	0.003%
20	3.933	881	884	887	rBV3	678	506	0.03%	0.003%
21	3.952	887	890	897	rVB	698	490	0.03%	0.003%
22	3.984	897	900	904	rBV2	658	600	0.03%	0.004%
23	4.170	945	958	966	rBV	206219	478308	25.71%	3.040%
24	4.415	1032	1034	1038	rBV4	1105	855	0.05%	0.005%
25	4.643	1088	1105	1134	rVV2	303093	760228	40.86%	4.831%
26	4.881	1177	1179	1187	rVB5	1272	1408	0.08%	0.009%
27	4.961	1199	1204	1208	rBV4	889	813	0.04%	0.005%
28	5.019	1220	1222	1229	rVB5	718	686	0.04%	0.004%
29	5.077	1237	1240	1243	rVB2	875	564	0.03%	0.004%
30	5.158	1262	1265	1269	rBV3	781	624	0.03%	0.004%
31	5.209	1275	1281	1285	rVB2	1145	1234	0.07%	0.008%
32	5.334	1295	1320	1351	rBV3	611569	1860710	100.00%	11.824%
33	5.559	1386	1390	1394	rBV6	1501	1187	0.06%	0.008%
34	5.682	1426	1428	1432	rVB4	778	665	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031082.D
 Acq On : 11 Apr 2019 20:25
 Operator : JC/SP
 Sample : K2341-07DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB722DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.756	1445	1451	1453	rBV4	872	809	0.04%	0.005%
36	5.881	1475	1490	1519	rBV	548203	1112179	59.77%	7.068%
37	6.183	1570	1584	1610	rBV3	112954	232643	12.50%	1.478%
38	6.325	1614	1628	1658	rBV	426469	872150	46.87%	5.542%
39	6.447	1662	1666	1667	rBV4	1348	905	0.05%	0.006%
40	6.666	1731	1734	1740	rVB5	947	851	0.05%	0.005%
41	6.865	1792	1796	1799	rBV2	592	583	0.03%	0.004%
42	6.881	1799	1801	1804	rVB	789	505	0.03%	0.003%
43	6.903	1804	1808	1809	rBV	750	523	0.03%	0.003%
44	7.051	1849	1854	1859	rBV2	798	915	0.05%	0.006%
45	7.225	1888	1908	1938	rBV	223113	423319	22.75%	2.690%
46	7.418	1964	1968	1972	rBV5	897	837	0.04%	0.005%
47	7.563	1999	2013	2029	rBV	728109	1319705	70.92%	8.386%
48	7.846	2090	2101	2127	rBV	156460	285923	15.37%	1.817%
49	8.032	2158	2159	2163	rVB2	1534	734	0.04%	0.005%
50	8.061	2163	2168	2170	rBV4	871	751	0.04%	0.005%
51	8.177	2196	2204	2205	rBV4	2461	2990	0.16%	0.019%
52	8.222	2206	2218	2235	rVV	721927	1244495	66.88%	7.908%
53	8.309	2235	2245	2288	rVB	565728	1141276	61.34%	7.252%
54	8.675	2356	2359	2363	rVB4	1153	773	0.04%	0.005%
55	8.794	2394	2396	2402	rBV3	962	888	0.05%	0.006%
56	8.849	2410	2413	2417	rVB4	783	603	0.03%	0.004%
57	8.868	2417	2419	2424	rVB2	763	564	0.03%	0.004%
58	8.910	2429	2432	2435	rBV5	866	603	0.03%	0.004%
59	9.029	2466	2469	2474	rBV3	1058	1055	0.06%	0.007%
60	9.087	2474	2487	2513	rBV	797673	1381545	74.25%	8.779%
61	9.440	2593	2597	2600	rVB2	1005	613	0.03%	0.004%
62	9.521	2618	2622	2624	rBV3	804	566	0.03%	0.004%
63	9.598	2644	2646	2650	rVB3	1020	754	0.04%	0.005%
64	9.646	2655	2661	2666	rBV3	959	1264	0.07%	0.008%
65	9.788	2702	2705	2708	rBV2	867	586	0.03%	0.004%
66	9.887	2731	2736	2743	rVB3	759	897	0.05%	0.006%
67	9.929	2743	2749	2751	rBV3	574	641	0.03%	0.004%
68	9.993	2767	2769	2774	rVB	790	567	0.03%	0.004%
69	10.022	2775	2778	2781	rVV3	889	571	0.03%	0.004%
70	10.061	2785	2790	2797	rVB3	731	957	0.05%	0.006%
71	10.099	2797	2802	2806	rBV3	1076	1082	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031082.D
 Acq On : 11 Apr 2019 20:25
 Operator : JC/SP
 Sample : K2341-07DL 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB722DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.360	2873	2883	2885	rBV3	1026	1287	0.07%	0.008%
73	10.427	2890	2904	2932	rBV	616259	1000258	53.76%	6.356%
74	10.569	2943	2948	2950	rBV3	1078	961	0.05%	0.006%
75	10.743	2998	3002	3005	rBV	686	548	0.03%	0.003%
76	10.781	3010	3014	3018	rBV4	727	706	0.04%	0.004%
77	10.813	3020	3024	3029	rBV3	1868	1582	0.09%	0.010%
78	11.222	3148	3151	3154	rVB3	927	567	0.03%	0.004%
79	11.283	3164	3170	3175	rBV3	646	767	0.04%	0.005%
80	11.402	3204	3207	3209	rBV	999	607	0.03%	0.004%
81	11.482	3219	3232	3251	rBV	731691	1200010	64.49%	7.626%
82	11.855	3336	3348	3377	rBV	738355	1246635	67.00%	7.922%
83	12.177	3445	3448	3449	rBV3	1351	723	0.04%	0.005%
84	12.238	3464	3467	3471	rBV3	1147	1033	0.06%	0.007%
85	12.273	3476	3478	3485	rVB4	1196	1007	0.05%	0.006%
86	12.360	3499	3505	3509	rBV6	1160	1161	0.06%	0.007%
87	12.479	3532	3542	3547	rBV9	1904	3567	0.19%	0.023%
88	12.759	3623	3629	3632	rBV4	1067	1145	0.06%	0.007%
89	12.816	3645	3647	3655	rBV4	759	662	0.04%	0.004%
90	12.861	3658	3661	3663	rBV	947	638	0.03%	0.004%
91	13.019	3705	3710	3713	rBV4	615	650	0.03%	0.004%
92	13.183	3758	3761	3766	rVB4	1187	889	0.05%	0.006%
93	13.215	3766	3771	3777	rBV4	979	1421	0.08%	0.009%
94	13.263	3781	3786	3788	rBV2	967	865	0.05%	0.005%
95	13.366	3812	3818	3823	rBV3	1678	2128	0.11%	0.014%
96	13.652	3904	3907	3909	rBV2	1074	724	0.04%	0.005%
97	13.685	3915	3917	3920	rBV2	790	577	0.03%	0.004%
98	13.733	3930	3932	3935	rBV2	904	570	0.03%	0.004%
99	14.894	4289	4293	4298	rBV4	1244	1499	0.08%	0.010%
100	15.157	4372	4375	4377	rBV3	1107	906	0.05%	0.006%


Sum of corrected areas: 15736361

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031082.D
Acq On : 11 Apr 2019 20:25
Operator : JC/SP
Sample : K2341-07DL 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB722DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

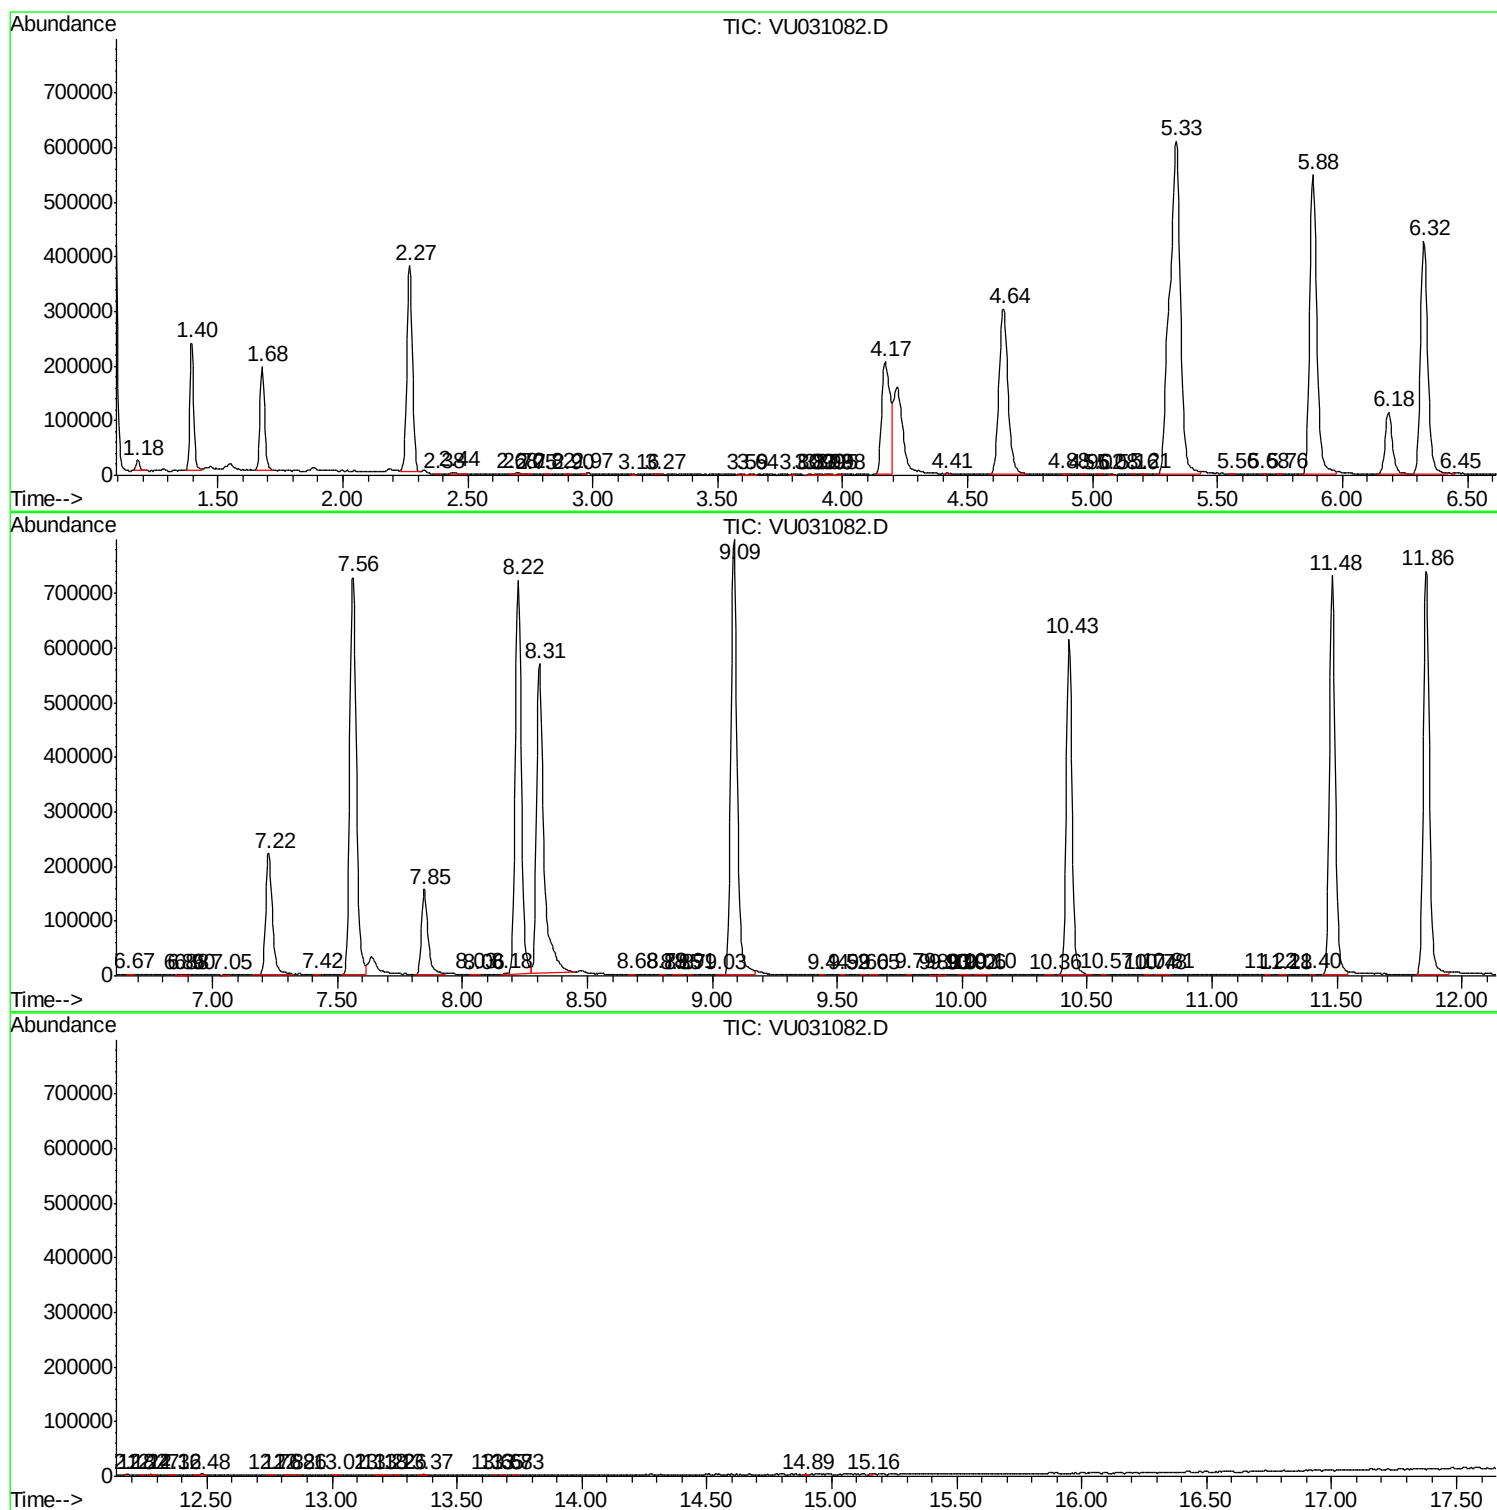

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031082.D
Acq On : 11 Apr 2019 20:25
Operator : JC/SP
Sample : K2341-07DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB722DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031082.D
Acq On : 11 Apr 2019 20:25
Operator : JC/SP
Sample : K2341-07DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB722DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc