

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031090.D
 Acq On : 11 Apr 2019 23:28
 Operator : JC/SP
 Sample : K2340-12ME
 Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF177ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.174	21	26	33	rVB	17194	16921	0.90%	0.111%
2	1.283	53	60	67	rBV4	10716	22635	1.21%	0.148%
3	1.392	87	94	110	rVB	202732	244545	13.04%	1.602%
4	1.637	165	170	180	rBV	203697	226099	12.06%	1.482%
5	2.235	346	356	370	rVB	394247	606088	32.32%	3.972%
6	2.682	483	495	497	rBV8	3790	5611	0.30%	0.037%
7	2.807	528	534	535	rBV	1171	1006	0.05%	0.007%
8	2.823	536	539	542	rVV3	1661	1436	0.08%	0.009%
9	2.926	568	571	574	rBV2	560	462	0.02%	0.003%
10	3.000	591	594	598	rVB	915	597	0.03%	0.004%
11	3.045	606	608	611	rBV2	836	464	0.02%	0.003%
12	3.074	614	617	620	rVB2	803	527	0.03%	0.003%
13	3.138	635	637	645	rVB5	796	687	0.04%	0.005%
14	3.280	675	681	693	rVB6	1324	2417	0.13%	0.016%
15	3.354	693	704	707	rBV3	939	1566	0.08%	0.010%
16	3.534	752	760	763	rBV2	843	738	0.04%	0.005%
17	4.087	928	932	935	rBV3	744	452	0.02%	0.003%
18	4.122	939	943	948	rBV3	699	676	0.04%	0.004%
19	4.187	950	963	1008	rBV2	152996	564004	30.07%	3.696%
20	4.524	1065	1068	1070	rBV2	1025	749	0.04%	0.005%
21	4.547	1073	1075	1080	rVB4	1101	587	0.03%	0.004%
22	4.640	1086	1104	1131	rBV	284750	745800	39.77%	4.887%
23	4.762	1139	1142	1146	rBV4	757	504	0.03%	0.003%
24	4.836	1161	1165	1166	rBV2	716	543	0.03%	0.004%
25	4.862	1171	1173	1176	rVV3	755	535	0.03%	0.004%
26	5.113	1246	1251	1254	rBV2	981	796	0.04%	0.005%
27	5.135	1254	1258	1262	rVV4	816	664	0.04%	0.004%
28	5.154	1262	1264	1266	rVB	1090	563	0.03%	0.004%
29	5.196	1274	1277	1280	rBV3	930	648	0.03%	0.004%
30	5.328	1294	1318	1348	rBV2	633316	1875350	100.00%	12.289%
31	5.611	1398	1406	1412	rBV10	2881	5395	0.29%	0.035%
32	5.669	1422	1424	1429	rVB5	1262	858	0.05%	0.006%
33	5.707	1432	1436	1440	rVB5	628	480	0.03%	0.003%
34	5.878	1476	1489	1524	rBV2	528851	1126305	60.06%	7.380%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031090.D
 Acq On : 11 Apr 2019 23:28
 Operator : JC/SP
 Sample : K2340-12ME
 Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF177ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	6.154	1571	1575	1576	rBV	1699	1057	0.06%	0.007%
36	6.238	1596	1601	1603	rBV4	1873	1868	0.10%	0.012%
37	6.325	1614	1628	1655	rVB	408245	859214	45.82%	5.630%
38	6.460	1667	1670	1678	rVB6	1377	1853	0.10%	0.012%
39	6.588	1708	1710	1714	rVB2	630	482	0.03%	0.003%
40	6.685	1737	1740	1744	rVB2	816	555	0.03%	0.004%
41	6.717	1746	1750	1752	rBV2	772	477	0.03%	0.003%
42	6.900	1802	1807	1810	rVV6	1220	1374	0.07%	0.009%
43	6.961	1823	1826	1830	rVB4	902	755	0.04%	0.005%
44	6.987	1830	1834	1841	rVB6	1353	1102	0.06%	0.007%
45	7.045	1849	1852	1857	rVB4	862	691	0.04%	0.005%
46	7.161	1883	1888	1891	rBV5	901	658	0.04%	0.004%
47	7.225	1895	1908	1936	rBV	205495	418130	22.30%	2.740%
48	7.421	1965	1969	1971	rBV3	917	870	0.05%	0.006%
49	7.453	1976	1979	1987	rVB4	698	535	0.03%	0.004%
50	7.559	1999	2012	2034	rBV	734650	1353835	72.19%	8.871%
51	7.849	2091	2102	2127	rBV	141045	286940	15.30%	1.880%
52	7.974	2138	2141	2143	rVB3	843	473	0.03%	0.003%
53	8.109	2181	2183	2187	rBV3	528	450	0.02%	0.003%
54	8.170	2199	2202	2207	rBV4	1032	1060	0.06%	0.007%
55	8.222	2207	2218	2237	rBV	189254	328894	17.54%	2.155%
56	8.321	2237	2249	2280	rBV	627665	1237636	65.99%	8.110%
57	8.601	2334	2336	2342	rVB5	1718	1398	0.07%	0.009%
58	8.640	2346	2348	2351	rVV2	961	605	0.03%	0.004%
59	8.656	2351	2353	2356	rVB3	1175	616	0.03%	0.004%
60	8.817	2400	2403	2410	rBV4	1021	1100	0.06%	0.007%
61	8.897	2424	2428	2434	rVB2	879	725	0.04%	0.005%
62	9.090	2474	2488	2518	rBV	787350	1434434	76.49%	9.399%
63	9.350	2566	2569	2572	rBV2	878	662	0.04%	0.004%
64	9.447	2590	2599	2605	rBV4	966	1559	0.08%	0.010%
65	9.492	2610	2613	2616	rBV2	738	537	0.03%	0.004%
66	9.845	2719	2723	2730	rVB3	878	865	0.05%	0.006%
67	10.003	2768	2772	2775	rBV	635	658	0.04%	0.004%
68	10.048	2783	2786	2791	rBV3	546	533	0.03%	0.003%
69	10.154	2815	2819	2821	rBV3	1487	1128	0.06%	0.007%
70	10.218	2837	2839	2845	rVB3	680	640	0.03%	0.004%
71	10.257	2845	2851	2852	rBV2	742	638	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031090.D
 Acq On : 11 Apr 2019 23:28
 Operator : JC/SP
 Sample : K2340-12ME
 Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 81 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF177ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.353	2877	2881	2885	rBV3	1166	819	0.04%	0.005%
73	10.431	2890	2905	2927	rBV	683481	1106886	59.02%	7.253%
74	10.579	2949	2951	2952	rBV2	1066	490	0.03%	0.003%
75	10.710	2988	2992	2997	rBV4	822	889	0.05%	0.006%
76	10.800	3017	3020	3023	rBV2	718	471	0.03%	0.003%
77	10.948	3063	3066	3071	rVB2	1001	708	0.04%	0.005%
78	11.308	3175	3178	3181	rBV2	724	653	0.03%	0.004%
79	11.357	3189	3193	3195	rBV2	615	538	0.03%	0.004%
80	11.482	3218	3232	3255	rBV	829536	1355325	72.27%	8.881%
81	11.858	3336	3349	3373	rBV	819084	1366334	72.86%	8.953%
82	12.231	3462	3465	3467	rBV2	864	577	0.03%	0.004%
83	12.321	3491	3493	3500	rBV4	785	611	0.03%	0.004%
84	12.479	3531	3542	3549	rVV2	4250	7560	0.40%	0.050%
85	12.553	3562	3565	3568	rBV	1017	594	0.03%	0.004%
86	12.636	3588	3591	3596	rVB4	782	597	0.03%	0.004%
87	12.720	3613	3617	3620	rVB2	963	802	0.04%	0.005%
88	12.739	3620	3623	3626	rBV2	1004	690	0.04%	0.005%
89	12.990	3696	3701	3706	rBV3	910	906	0.05%	0.006%
90	13.016	3706	3709	3712	rBV	1044	872	0.05%	0.006%
91	13.231	3773	3776	3779	rVB2	910	636	0.03%	0.004%
92	13.299	3793	3797	3802	rBV3	856	955	0.05%	0.006%
93	13.344	3809	3811	3815	rVB3	909	634	0.03%	0.004%
94	13.929	3988	3993	3996	rBV4	1516	1489	0.08%	0.010%
95	14.273	4095	4100	4109	rBV4	4120	5379	0.29%	0.035%
96	14.379	4129	4133	4137	rBV3	799	948	0.05%	0.006%
97	14.411	4141	4143	4150	rBV3	841	796	0.04%	0.005%
98	14.488	4163	4167	4168	rBV2	1131	794	0.04%	0.005%
99	14.913	4296	4299	4302	rBV2	826	567	0.03%	0.004%
100	14.945	4306	4309	4311	rVB2	988	581	0.03%	0.004%


Sum of corrected areas: 15260816

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031090.D
Acq On : 11 Apr 2019 23:28
Operator : JC/SP
Sample : K2340-12ME
Misc : 5.71µ/5mL/100µL/5.0mL/MSVOA_U/MEOH
ALS Vial : 81 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF177ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

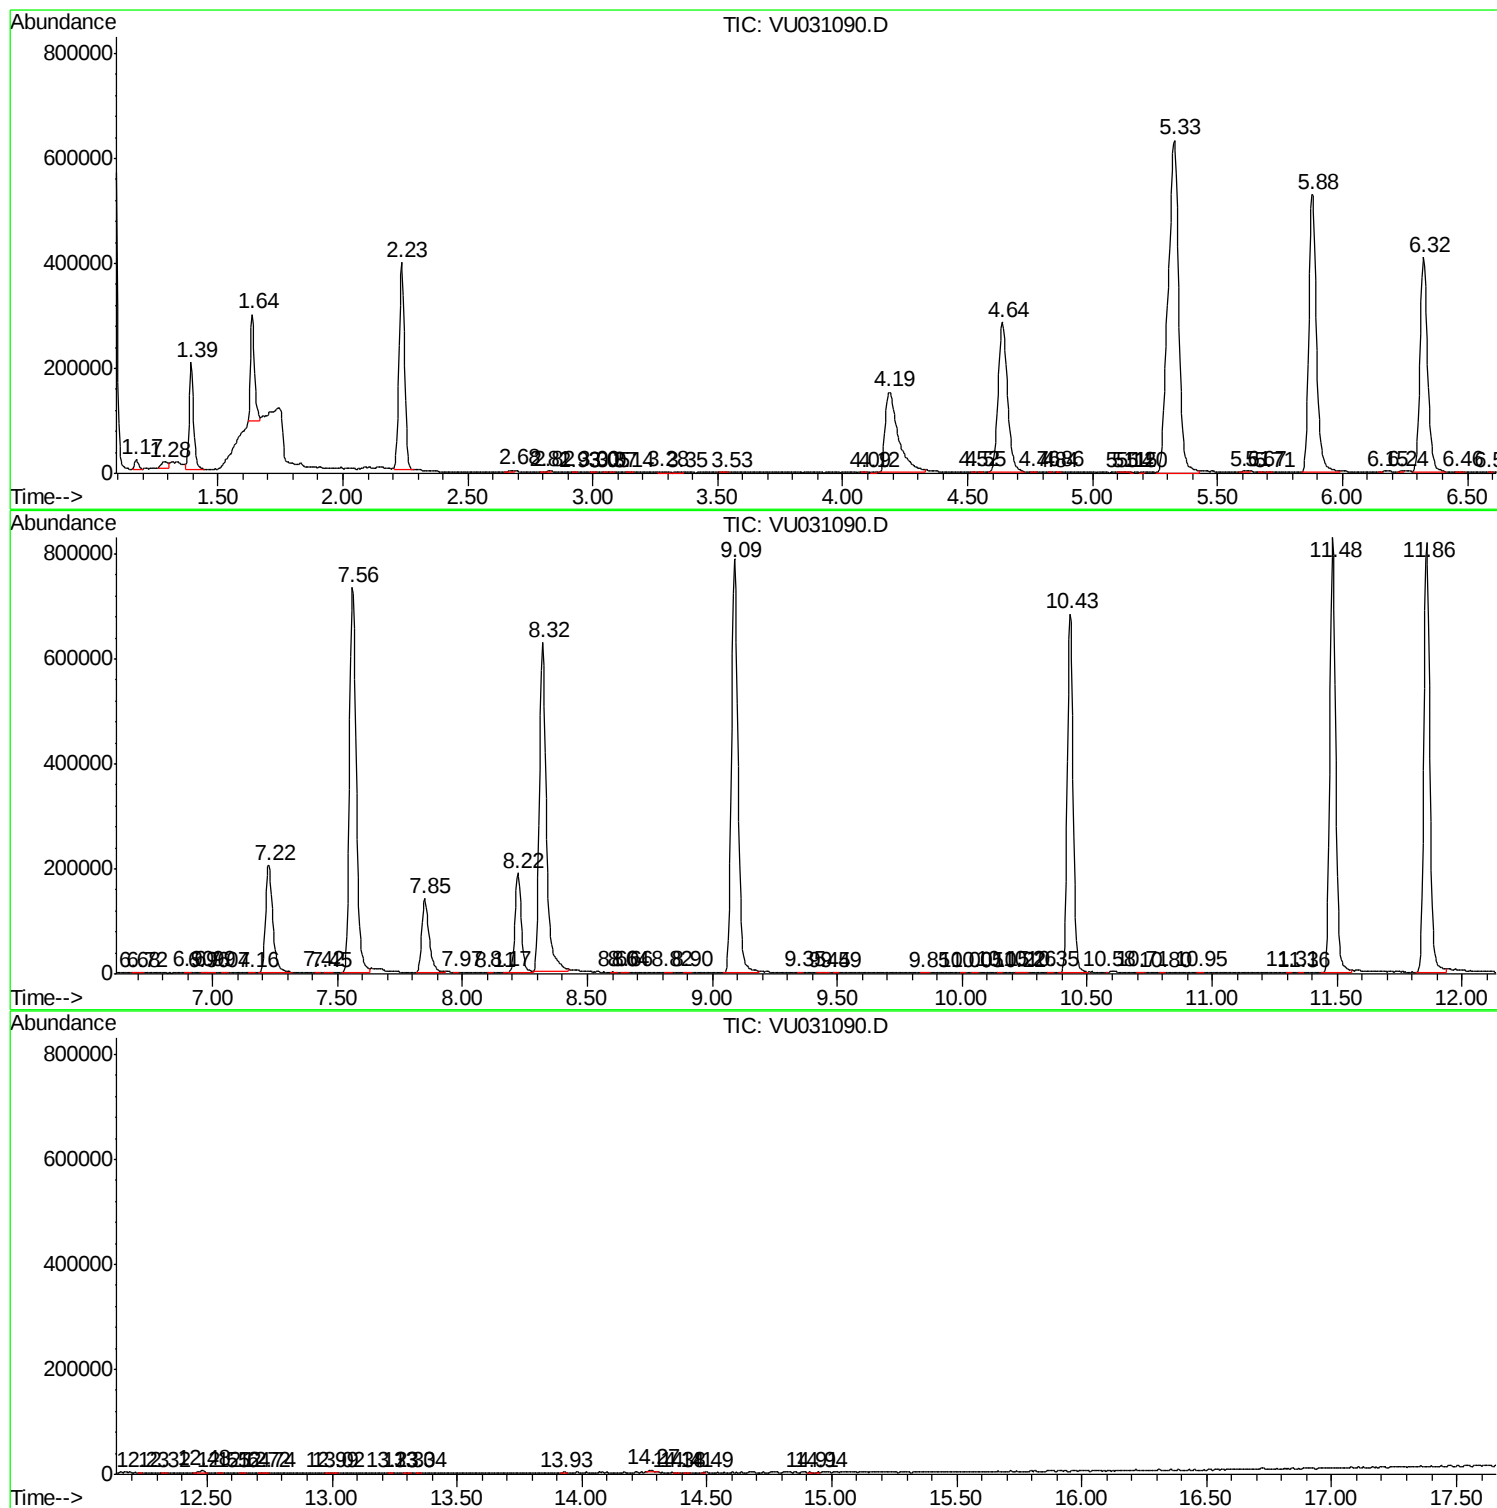

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031090.D
Acq On : 11 Apr 2019 23:28
Operator : JC/SP
Sample : K2340-12ME
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 81 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF177ME

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031090.D
Acq On : 11 Apr 2019 23:28
Operator : JC/SP
Sample : K2340-12ME
Misc : 5.71g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 81 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF177ME

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc