

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031095.D
 Acq On : 12 Apr 2019 01:46
 Operator : JC/SP
 Sample : K2339-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	22	28	38	rBV	43511	43414	2.27%	0.278%
2	1.254	47	51	58	rBV2	14279	14655	0.77%	0.094%
3	1.396	87	95	110	rBV	274864	296875	15.54%	1.903%
4	1.470	111	118	129	rVV	97810	110431	5.78%	0.708%
5	1.679	175	183	195	rVB	213417	272664	14.27%	1.748%
6	2.267	353	366	376	rBV	409495	642348	33.62%	4.118%
7	2.318	376	382	398	rVB	55355	88866	4.65%	0.570%
8	2.441	410	420	440	rVB	29439	57966	3.03%	0.372%
9	2.650	482	485	486	rBV3	929	510	0.03%	0.003%
10	2.701	492	501	510	rVB3	8395	14815	0.78%	0.095%
11	2.794	524	530	531	rBV4	936	791	0.04%	0.005%
12	2.826	531	540	556	rVB5	4475	9555	0.50%	0.061%
13	2.926	567	571	574	rVB5	1416	1159	0.06%	0.007%
14	2.949	574	578	585	rBV4	1315	1972	0.10%	0.013%
15	2.984	585	589	591	rVB2	717	545	0.03%	0.003%
16	3.183	639	651	663	rBV6	3644	7558	0.40%	0.048%
17	3.293	681	685	688	rVV4	838	653	0.03%	0.004%
18	3.630	786	790	794	rVB4	1026	897	0.05%	0.006%
19	3.662	794	800	802	rBV2	592	582	0.03%	0.004%
20	3.682	804	806	810	rVV2	966	640	0.03%	0.004%
21	3.736	819	823	826	rBV4	523	419	0.02%	0.003%
22	3.968	889	895	896	rBV3	1957	1560	0.08%	0.010%
23	4.093	929	934	938	rVB4	1134	1050	0.05%	0.007%
24	4.170	942	958	988	rBV	203663	573308	30.00%	3.676%
25	4.489	1053	1057	1059	rBV4	998	761	0.04%	0.005%
26	4.569	1079	1082	1084	rBV3	814	504	0.03%	0.003%
27	4.640	1088	1104	1137	rBV	319402	772192	40.41%	4.951%
28	4.990	1209	1213	1217	rBV5	1072	1157	0.06%	0.007%
29	5.167	1265	1268	1272	rBV2	548	561	0.03%	0.004%
30	5.225	1282	1286	1288	rBV3	542	442	0.02%	0.003%
31	5.334	1297	1320	1340	rBV2	640662	1910834	100.00%	12.250%
32	5.572	1392	1394	1396	rBV3	1162	417	0.02%	0.003%
33	5.617	1407	1408	1418	rVB7	1172	1251	0.07%	0.008%
34	5.666	1420	1423	1426	rBV3	854	658	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031095.D
 Acq On : 12 Apr 2019 01:46
 Operator : JC/SP
 Sample : K2339-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.752	1446	1450	1451	rBV2	588	456	0.02%	0.003%
36	5.881	1476	1490	1517	rBV	627218	1257415	65.80%	8.061%
37	6.103	1557	1559	1563	rVB	862	460	0.02%	0.003%
38	6.174	1573	1581	1582	rBV6	5113	5239	0.27%	0.034%
39	6.325	1613	1628	1649	rBV	436748	881821	46.15%	5.653%
40	6.553	1693	1699	1702	rBV6	2301	2960	0.15%	0.019%
41	6.627	1720	1722	1725	rVB4	1371	666	0.03%	0.004%
42	6.784	1768	1771	1775	rVB4	970	659	0.03%	0.004%
43	6.875	1796	1799	1801	rBV4	859	601	0.03%	0.004%
44	7.170	1888	1891	1896	rVB2	787	616	0.03%	0.004%
45	7.225	1896	1908	1932	rBV	219888	420506	22.01%	2.696%
46	7.408	1962	1965	1968	rBV2	858	765	0.04%	0.005%
47	7.563	2000	2013	2031	rBV	780112	1387290	72.60%	8.894%
48	7.849	2091	2102	2122	rBV	148704	277176	14.51%	1.777%
49	8.173	2190	2203	2215	rBV6	13165	26598	1.39%	0.171%
50	8.222	2215	2218	2227	rVB6	1683	2163	0.11%	0.014%
51	8.309	2234	2245	2282	rBV2	564082	1170926	61.28%	7.507%
52	8.743	2376	2380	2382	rBV3	900	565	0.03%	0.004%
53	8.768	2385	2388	2392	rVB3	820	496	0.03%	0.003%
54	8.797	2396	2397	2401	rBV4	702	479	0.03%	0.003%
55	8.961	2445	2448	2451	rBV4	972	706	0.04%	0.005%
56	8.987	2451	2456	2459	rVV4	955	789	0.04%	0.005%
57	9.042	2468	2473	2474	rBV2	594	545	0.03%	0.003%
58	9.087	2474	2487	2512	rBV	937038	1588041	83.11%	10.181%
59	9.376	2573	2577	2579	rBV2	1821	1626	0.09%	0.010%
60	9.389	2579	2581	2584	rVB4	1297	927	0.05%	0.006%
61	9.649	2653	2662	2675	rVV4	12911	22383	1.17%	0.143%
62	9.752	2685	2694	2697	rBV4	1709	2673	0.14%	0.017%
63	9.932	2742	2750	2759	rBV9	5042	9557	0.50%	0.061%
64	10.038	2777	2783	2791	rBV8	5419	9074	0.47%	0.058%
65	10.148	2813	2817	2821	rBV3	995	981	0.05%	0.006%
66	10.167	2821	2823	2831	rVB6	1028	899	0.05%	0.006%
67	10.263	2847	2853	2856	rBV4	1120	902	0.05%	0.006%
68	10.321	2867	2871	2874	rBV2	624	484	0.03%	0.003%
69	10.427	2884	2904	2927	rBV	621312	1013488	53.04%	6.498%
70	10.607	2948	2960	2970	rVB2	10518	18660	0.98%	0.120%
71	10.652	2970	2974	2977	rVB3	1122	717	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031095.D
 Acq On : 12 Apr 2019 01:46
 Operator : JC/SP
 Sample : K2339-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFC47

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.672	2977	2980	2983	rBV4	976	759	0.04%	0.005%
73	10.739	2994	3001	3008	rBV5	1339	1974	0.10%	0.013%
74	10.952	3064	3067	3070	rBV2	1170	806	0.04%	0.005%
75	10.987	3076	3078	3082	rVB2	765	490	0.03%	0.003%
76	11.077	3104	3106	3109	rVB	866	449	0.02%	0.003%
77	11.218	3147	3150	3156	rBV4	698	582	0.03%	0.004%
78	11.289	3166	3172	3173	rBV2	831	745	0.04%	0.005%
79	11.324	3178	3183	3186	rBV2	1296	1100	0.06%	0.007%
80	11.479	3219	3231	3258	rBV	844674	1366522	71.51%	8.761%
81	11.791	3325	3328	3331	rBV4	1078	733	0.04%	0.005%
82	11.855	3336	3348	3367	rBV	749059	1263349	66.12%	8.099%
83	12.479	3538	3542	3549	rVB3	3333	3638	0.19%	0.023%
84	12.636	3588	3591	3593	rBV3	1014	715	0.04%	0.005%
85	12.675	3600	3603	3606	rBV3	897	862	0.05%	0.006%
86	12.739	3619	3623	3625	rBV4	1396	1192	0.06%	0.008%
87	12.858	3657	3660	3662	rBV4	1073	799	0.04%	0.005%
88	12.871	3662	3664	3669	rVB4	947	640	0.03%	0.004%
89	12.987	3697	3700	3702	rBV3	763	515	0.03%	0.003%
90	13.035	3712	3715	3718	rVB2	1090	647	0.03%	0.004%
91	13.086	3728	3731	3737	rBV3	611	616	0.03%	0.004%
92	13.144	3746	3749	3752	rBV2	904	602	0.03%	0.004%
93	13.183	3757	3761	3762	rBV3	755	533	0.03%	0.003%
94	13.357	3812	3815	3817	rBV2	1151	892	0.05%	0.006%
95	13.595	3886	3889	3892	rBV	794	628	0.03%	0.004%
96	13.955	3997	4001	4003	rBV4	1674	1364	0.07%	0.009%
97	14.299	4106	4108	4111	rVB2	1486	847	0.04%	0.005%
98	14.427	4145	4148	4150	rBV3	1356	781	0.04%	0.005%
99	14.784	4256	4259	4261	rBV2	1333	683	0.04%	0.004%
100	15.106	4353	4359	4363	rBV4	1788	2261	0.12%	0.014%


Sum of corrected areas: 15598043

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031095.D
Acq On : 12 Apr 2019 01:46
Operator : JC/SP
Sample : K2339-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 87 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC47

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

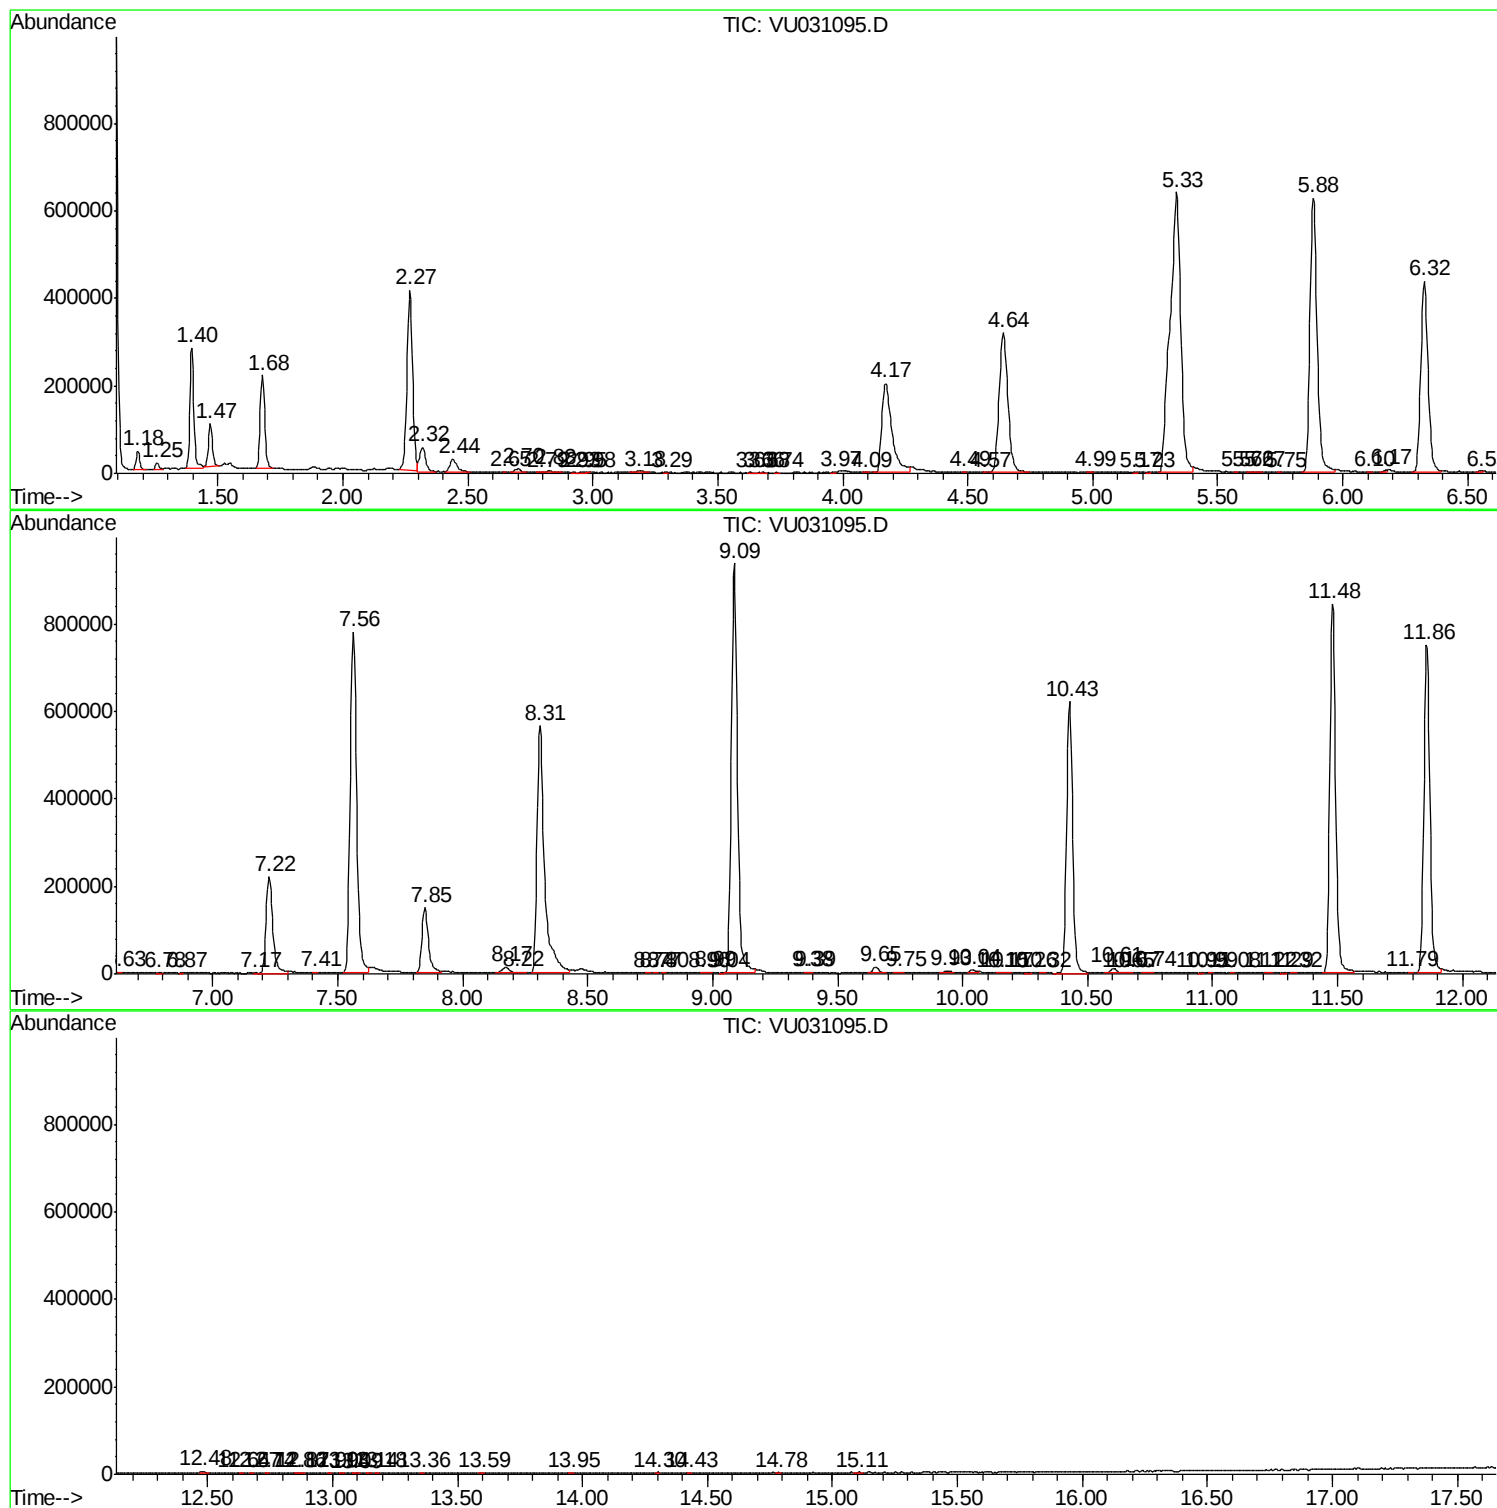

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031095.D
Acq On : 12 Apr 2019 01:46
Operator : JC/SP
Sample : K2339-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 87 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC47

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031095.D
Acq On : 12 Apr 2019 01:46
Operator : JC/SP
Sample : K2339-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 87 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFC47

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc