

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031098.D
 Acq On : 12 Apr 2019 02:55
 Operator : JC/SP
 Sample : K2354-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2T4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	88	95	107	rBV	258002	267765	14.06%	1.633%
2	1.675	175	182	199	rVB	203352	265926	13.96%	1.622%
3	2.267	356	366	380	rVB	400239	628332	32.98%	3.833%
4	2.508	439	441	442	rBV	622	309	0.02%	0.002%
5	2.559	453	457	462	rBV4	1515	1642	0.09%	0.010%
6	2.965	580	583	587	rVB2	845	731	0.04%	0.004%
7	3.010	589	597	601	rVV5	1395	2107	0.11%	0.013%
8	3.048	605	609	611	rBV3	597	442	0.02%	0.003%
9	3.109	626	628	631	rBV2	698	403	0.02%	0.002%
10	3.212	659	660	663	rVB	1005	257	0.01%	0.002%
11	3.228	663	665	669	rVB2	719	372	0.02%	0.002%
12	3.254	671	673	675	rBV	343	108	0.01%	0.001%
13	3.267	675	677	679	rVB	382	168	0.01%	0.001%
14	3.280	679	681	683	rBV	451	286	0.02%	0.002%
15	3.373	708	710	716	rVB4	596	358	0.02%	0.002%
16	3.495	743	748	755	rBV3	788	948	0.05%	0.006%
17	3.543	761	763	768	rVB	811	703	0.04%	0.004%
18	3.572	768	772	773	rBV	387	249	0.01%	0.002%
19	3.588	773	777	781	rVV2	622	657	0.03%	0.004%
20	3.611	781	784	786	rVV	804	481	0.03%	0.003%
21	3.624	786	788	791	rVV2	696	465	0.02%	0.003%
22	3.649	794	796	801	rVV4	692	614	0.03%	0.004%
23	3.691	805	809	811	rBV2	846	628	0.03%	0.004%
24	3.723	814	819	822	rBV2	599	694	0.04%	0.004%
25	3.791	835	840	842	rVB2	583	473	0.02%	0.003%
26	3.817	842	848	849	rBV3	464	354	0.02%	0.002%
27	3.842	854	856	857	rBV3	268	93	0.00%	0.001%
28	3.868	863	864	865	rBV3	316	118	0.01%	0.001%
29	3.910	874	877	883	rVB3	845	684	0.04%	0.004%
30	3.945	883	888	890	rBV	931	620	0.03%	0.004%
31	3.977	895	898	899	rBV2	427	277	0.01%	0.002%
32	4.006	904	907	909	rVB2	329	153	0.01%	0.001%
33	4.022	909	912	913	rBV2	422	259	0.01%	0.002%
34	4.058	918	923	926	rBV4	675	674	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031098.D
 Acq On : 12 Apr 2019 02:55
 Operator : JC/SP
 Sample : K2354-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2T4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	4.170	945	958	994	rBV2	194799	541865	28.44%	3.306%
36	4.643	1089	1105	1134	rBV	307157	759076	39.85%	4.631%
37	5.170	1267	1269	1271	rVB	293	118	0.01%	0.001%
38	5.196	1272	1277	1279	rBV2	626	597	0.03%	0.004%
39	5.225	1284	1286	1289	rBV	694	433	0.02%	0.003%
40	5.334	1296	1320	1350	rBV2	627491	1905005	100.00%	11.621%
41	5.743	1444	1447	1450	rBV4	1185	832	0.04%	0.005%
42	5.881	1476	1490	1520	rBV	610897	1245994	65.41%	7.601%
43	6.273	1610	1612	1614	rBV2	986	564	0.03%	0.003%
44	6.325	1614	1628	1650	rVV	438411	872941	45.82%	5.325%
45	6.736	1752	1756	1757	rBV	503	305	0.02%	0.002%
46	6.820	1777	1782	1785	rBV2	1011	908	0.05%	0.006%
47	6.839	1785	1788	1791	rVV2	614	507	0.03%	0.003%
48	6.987	1831	1834	1836	rBV2	347	263	0.01%	0.002%
49	7.009	1838	1841	1843	rBV2	474	346	0.02%	0.002%
50	7.064	1856	1858	1864	rVB3	790	618	0.03%	0.004%
51	7.090	1864	1866	1868	rBV	667	284	0.01%	0.002%
52	7.119	1873	1875	1878	rVB3	629	361	0.02%	0.002%
53	7.135	1878	1880	1882	rBV2	479	235	0.01%	0.001%
54	7.225	1896	1908	1933	rBV	212706	408677	21.45%	2.493%
55	7.511	1995	1997	2000	rBV3	733	331	0.02%	0.002%
56	7.562	2000	2013	2050	rBV	760400	1393738	73.16%	8.502%
57	7.849	2092	2102	2127	rBV	152570	280795	14.74%	1.713%
58	8.222	2205	2218	2235	rBV	873281	1501470	78.82%	9.160%
59	8.308	2236	2245	2280	rVB2	555914	1129049	59.27%	6.888%
60	8.816	2400	2403	2406	rBV2	788	550	0.03%	0.003%
61	8.903	2427	2430	2433	rVB2	566	369	0.02%	0.002%
62	8.919	2433	2435	2436	rBV	447	147	0.01%	0.001%
63	8.932	2436	2439	2442	rBV	825	639	0.03%	0.004%
64	8.974	2450	2452	2455	rBV2	555	334	0.02%	0.002%
65	8.990	2455	2457	2460	rBV2	447	256	0.01%	0.002%
66	9.086	2474	2487	2513	rBV	914760	1566541	82.23%	9.557%
67	9.363	2571	2573	2576	rBV2	630	364	0.02%	0.002%
68	9.533	2622	2626	2631	rBV3	818	893	0.05%	0.005%
69	9.614	2649	2651	2655	rBV2	414	355	0.02%	0.002%
70	9.646	2659	2661	2664	rBV3	541	411	0.02%	0.003%
71	9.739	2684	2690	2695	rBV3	836	1324	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031098.D
 Acq On : 12 Apr 2019 02:55
 Operator : JC/SP
 Sample : K2354-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 90 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2T4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	9.906	2739	2742	2744	rBV	176	110	0.01%	0.001%
73	9.993	2766	2769	2772	rVB3	738	442	0.02%	0.003%
74	10.019	2772	2777	2779	rBV3	1126	908	0.05%	0.006%
75	10.128	2808	2811	2813	rVB2	602	276	0.01%	0.002%
76	10.154	2817	2819	2821	rBV	360	182	0.01%	0.001%
77	10.231	2841	2843	2845	rBV2	403	185	0.01%	0.001%
78	10.427	2892	2904	2925	rBV	609124	995548	52.26%	6.073%
79	10.723	2994	2996	2999	rBV2	750	394	0.02%	0.002%
80	10.816	3022	3025	3027	rBV	724	506	0.03%	0.003%
81	11.032	3088	3092	3098	rBV4	971	1035	0.05%	0.006%
82	11.064	3098	3102	3107	rBV4	758	990	0.05%	0.006%
83	11.482	3219	3232	3258	rBV	800708	1345184	70.61%	8.206%
84	11.858	3336	3349	3373	rBV	735351	1250004	65.62%	7.626%
85	12.446	3530	3532	3535	rBV2	1245	727	0.04%	0.004%


Sum of corrected areas: 16392336

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031098.D
Acq On : 12 Apr 2019 02:55
Operator : JC/SP
Sample : K2354-13 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 90 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2T4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

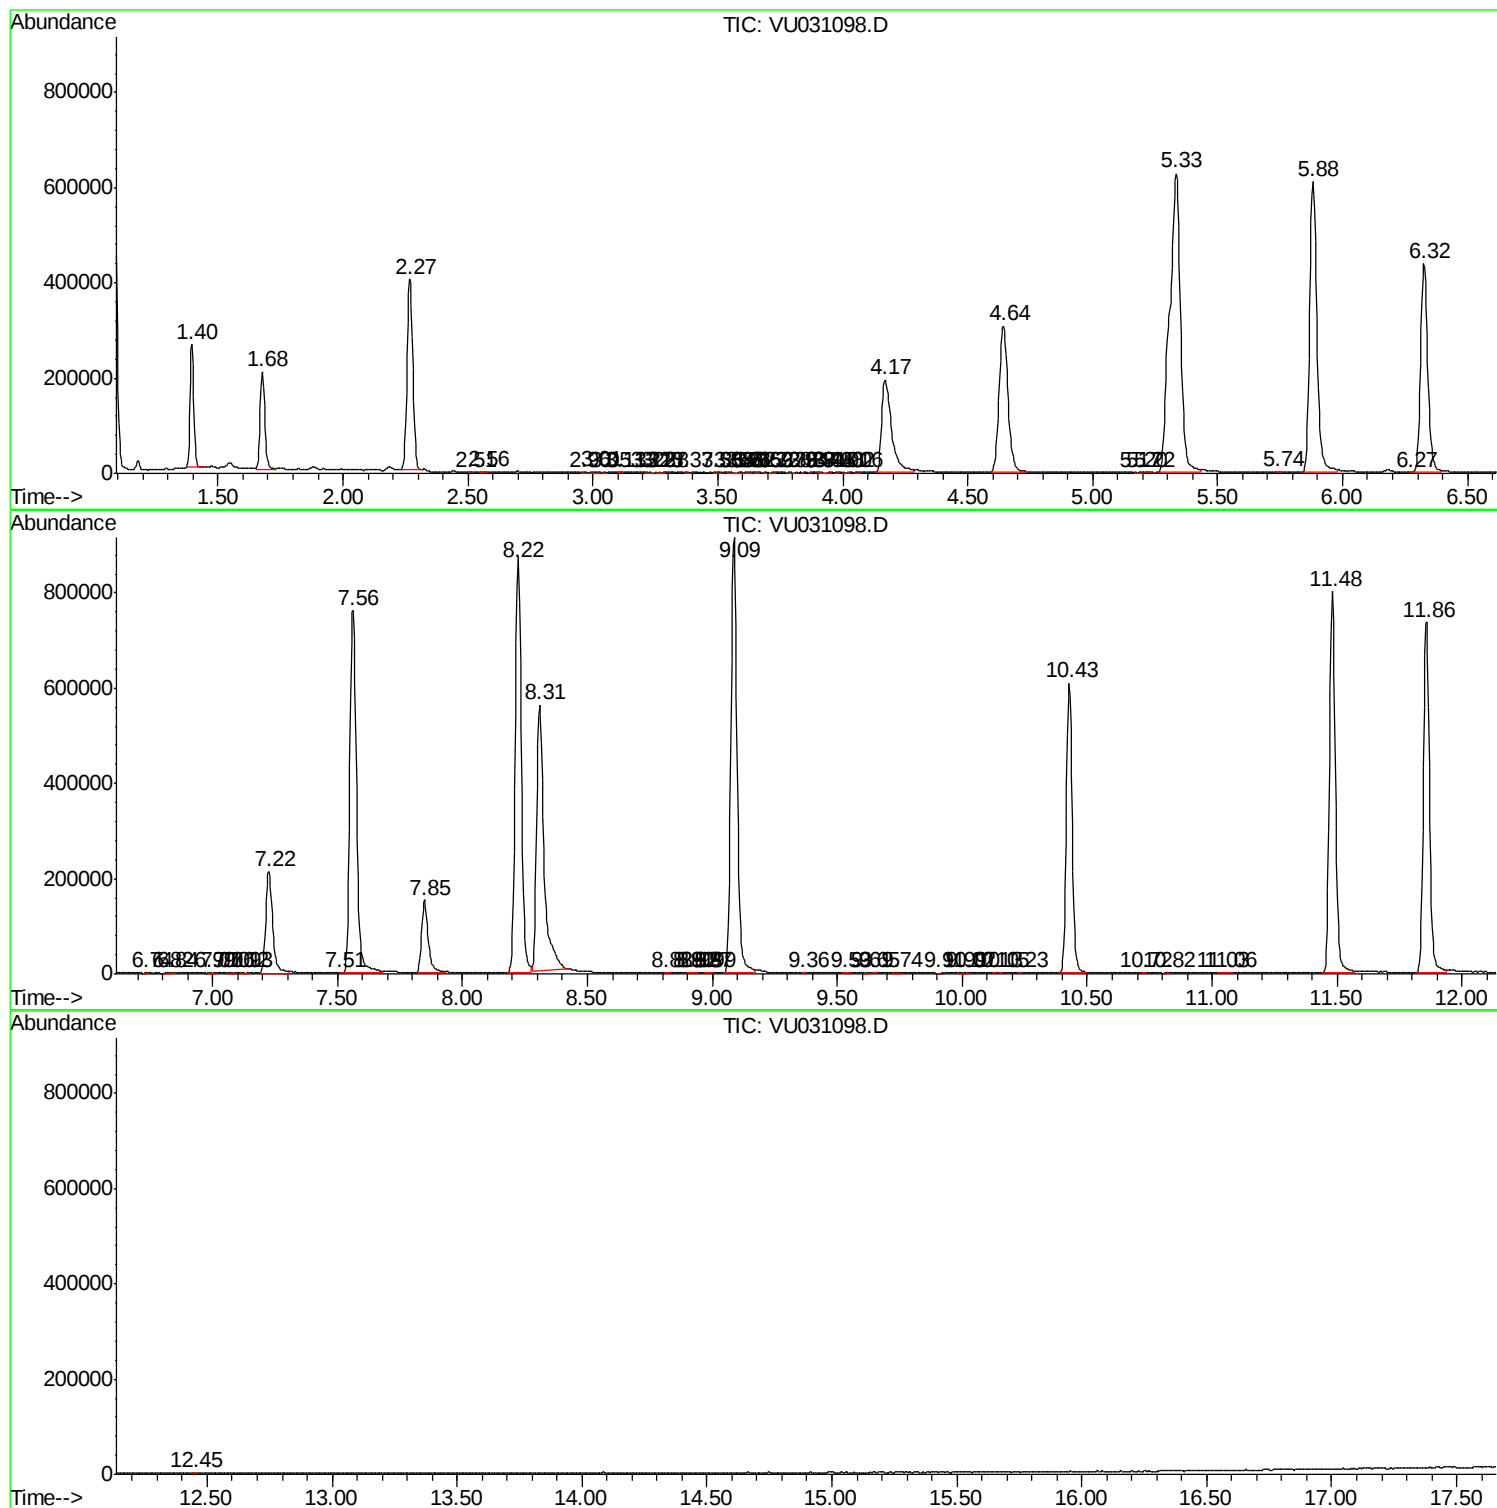

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031098.D
Acq On : 12 Apr 2019 02:55
Operator : JC/SP
Sample : K2354-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 90 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2T4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031098.D
Acq On : 12 Apr 2019 02:55
Operator : JC/SP
Sample : K2354-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 90 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2T4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc