

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031112.D
 Acq On : 12 Apr 2019 08:15
 Operator : JC/SP
 Sample : K2341-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 104 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB734

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rVB2	17418	16136	0.87%	0.110%
2	1.396	88	95	106	rBV	236316	246141	13.34%	1.679%
3	1.675	175	182	198	rVB	192013	248173	13.45%	1.693%
4	2.267	357	366	380	rVB	388570	588395	31.90%	4.014%
5	2.794	526	530	531	rBV2	787	420	0.02%	0.003%
6	2.894	558	561	565	rBV2	715	482	0.03%	0.003%
7	2.971	583	585	588	rBV4	701	496	0.03%	0.003%
8	3.096	619	624	626	rBV	490	494	0.03%	0.003%
9	3.135	632	636	637	rBV	524	336	0.02%	0.002%
10	3.222	661	663	665	rBV	334	129	0.01%	0.001%
11	3.347	699	702	705	rBV2	756	478	0.03%	0.003%
12	3.392	712	716	718	rBV	560	478	0.03%	0.003%
13	3.431	725	728	731	rVB2	764	478	0.03%	0.003%
14	3.447	731	733	735	rBV2	690	397	0.02%	0.003%
15	3.492	743	747	748	rBV2	389	277	0.02%	0.002%
16	3.640	790	793	800	rVB3	794	757	0.04%	0.005%
17	3.672	800	803	805	rBV	313	184	0.01%	0.001%
18	3.691	805	809	816	rVB3	545	755	0.04%	0.005%
19	3.730	816	821	824	rBV2	1010	869	0.05%	0.006%
20	3.756	828	829	831	rVB2	545	127	0.01%	0.001%
21	3.794	837	841	845	rVB3	729	668	0.04%	0.005%
22	3.817	845	848	850	rBV	512	332	0.02%	0.002%
23	3.913	876	878	880	rBV2	296	85	0.00%	0.001%
24	3.926	880	882	883	rVB	252	59	0.00%	0.000%
25	3.936	883	885	887	rBV	548	212	0.01%	0.001%
26	3.948	887	889	892	rBV2	485	235	0.01%	0.002%
27	3.990	899	902	904	rBV2	613	457	0.02%	0.003%
28	4.016	908	910	913	rVB3	565	325	0.02%	0.002%
29	4.042	913	918	923	rBV4	456	608	0.03%	0.004%
30	4.096	930	935	936	rBV	481	358	0.02%	0.002%
31	4.170	942	958	998	rBV2	189930	603854	32.73%	4.120%
32	4.643	1089	1105	1130	rBV	301497	739125	40.07%	5.043%
33	4.871	1171	1176	1179	rBV3	1239	1433	0.08%	0.010%
34	4.974	1205	1208	1211	rBV3	450	355	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031112.D
 Acq On : 12 Apr 2019 08:15
 Operator : JC/SP
 Sample : K2341-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 104 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB734

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.022	1221	1223	1225	rBV2	546	250	0.01%	0.002%
36	5.087	1241	1243	1246	rVB2	504	215	0.01%	0.001%
37	5.109	1246	1250	1252	rBV	600	507	0.03%	0.003%
38	5.157	1263	1265	1267	rVB	195	89	0.00%	0.001%
39	5.180	1267	1272	1273	rBV2	461	369	0.02%	0.003%
40	5.190	1273	1275	1279	rBV3	588	491	0.03%	0.003%
41	5.228	1284	1287	1290	rBV2	903	604	0.03%	0.004%
42	5.251	1292	1294	1297	rBV	574	345	0.02%	0.002%
43	5.334	1297	1320	1356	rBV2	612819	1844772	100.00%	12.586%
44	5.669	1421	1424	1428	rBV4	1254	1326	0.07%	0.009%
45	5.881	1477	1490	1519	rBV	602126	1224701	66.39%	8.355%
46	6.267	1606	1610	1613	rBV3	1075	954	0.05%	0.007%
47	6.325	1614	1628	1654	rBV	423000	857789	46.50%	5.852%
48	6.653	1727	1730	1732	rBV3	761	478	0.03%	0.003%
49	6.669	1732	1735	1739	rBV2	843	763	0.04%	0.005%
50	6.707	1744	1747	1748	rBV2	645	367	0.02%	0.003%
51	6.733	1754	1755	1758	rBV	301	137	0.01%	0.001%
52	6.762	1758	1764	1767	rBV3	1250	1090	0.06%	0.007%
53	6.884	1799	1802	1803	rBV	957	480	0.03%	0.003%
54	6.932	1815	1817	1820	rBV2	462	358	0.02%	0.002%
55	6.981	1829	1832	1833	rBV	479	240	0.01%	0.002%
56	7.006	1838	1840	1843	rVB	608	313	0.02%	0.002%
57	7.022	1843	1845	1846	rBV2	292	145	0.01%	0.001%
58	7.061	1852	1857	1863	rVB5	803	931	0.05%	0.006%
59	7.099	1863	1869	1874	rBV3	614	963	0.05%	0.007%
60	7.157	1882	1887	1890	rBV3	807	644	0.03%	0.004%
61	7.183	1892	1895	1896	rBV	524	288	0.02%	0.002%
62	7.225	1896	1908	1930	rBV	205691	386841	20.97%	2.639%
63	7.562	1999	2013	2038	rBV	726995	1340589	72.67%	9.146%
64	7.849	2091	2102	2129	rBV	143301	268999	14.58%	1.835%
65	8.106	2180	2182	2184	rBV2	550	200	0.01%	0.001%
66	8.148	2192	2195	2196	rBV2	629	382	0.02%	0.003%
67	8.308	2234	2245	2286	rBV	533777	1123378	60.90%	7.664%
68	8.688	2361	2363	2366	rBV4	565	287	0.02%	0.002%
69	8.707	2366	2369	2372	rVB2	1235	732	0.04%	0.005%
70	8.788	2391	2394	2397	rBV2	949	598	0.03%	0.004%
71	8.945	2441	2443	2446	rBV2	890	566	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031112.D
Acq On : 12 Apr 2019 08:15
Operator : JC/SP
Sample : K2341-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 104 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB734

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Title : VOC Analysis

72	9.087	2475	2487	2518	rBV	889126	1553168	84.19%	10.596%
73	9.495	2612	2614	2620	rVB5	1191	1036	0.06%	0.007%
74	9.521	2620	2622	2626	rBV	826	637	0.03%	0.004%
75	9.951	2754	2756	2758	rBV	489	254	0.01%	0.002%
76	10.312	2865	2868	2871	rBV	1088	687	0.04%	0.005%
77	10.427	2892	2904	2928	rBV	591513	981222	53.19%	6.694%
78	10.730	2995	2998	3002	rBV2	571	397	0.02%	0.003%
79	10.881	3042	3045	3048	rVB2	866	440	0.02%	0.003%
80	10.913	3052	3055	3058	rBV3	710	555	0.03%	0.004%
81	11.328	3182	3184	3186	rBV	560	308	0.02%	0.002%
82	11.479	3219	3231	3257	rBV	814962	1343534	72.83%	9.166%
83	11.855	3336	3348	3377	rBV	733477	1258684	68.23%	8.587%
84	12.717	3614	3616	3619	rBV3	1211	606	0.03%	0.004%


Sum of corrected areas: 14657817

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031112.D
Acq On : 12 Apr 2019 08:15
Operator : JC/SP
Sample : K2341-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 104 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB734

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

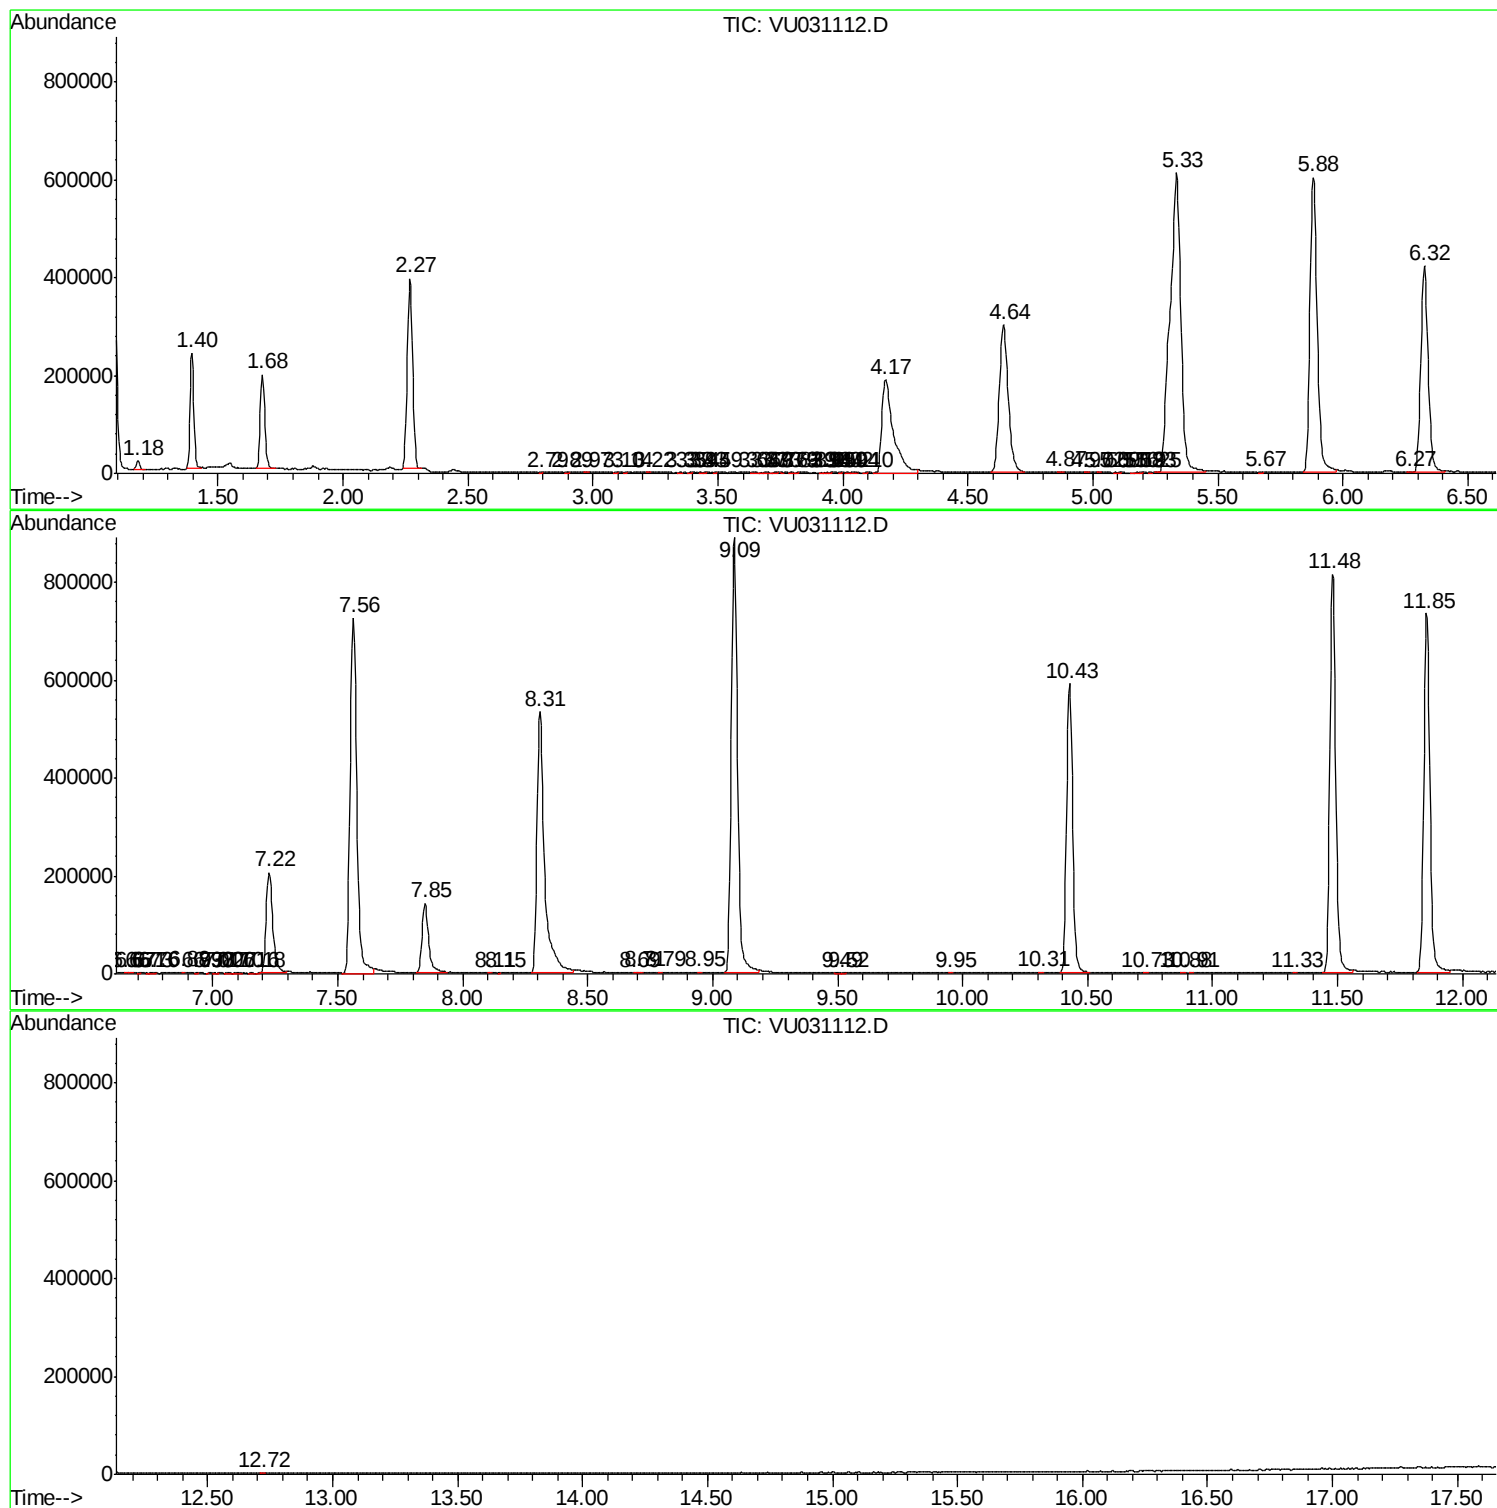

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031112.D
Acq On : 12 Apr 2019 08:15
Operator : JC/SP
Sample : K2341-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 104 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB734

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031112.D
Acq On : 12 Apr 2019 08:15
Operator : JC/SP
Sample : K2341-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 104 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB734

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc