

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031123.D
 Acq On : 12 Apr 2019 12:27
 Operator : JC/SP
 Sample : K2353-07DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 115 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ63DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	38	rVB	16684	17342	0.86%	0.113%
2	1.396	87	95	109	rBV	346889	363900	17.96%	2.370%
3	1.675	174	182	195	rVB	234723	305685	15.08%	1.991%
4	2.267	355	366	381	rVB	508017	765141	37.76%	4.984%
5	2.434	415	418	420	rBV3	1087	865	0.04%	0.006%
6	2.482	431	433	437	rVB3	782	524	0.03%	0.003%
7	2.621	471	476	477	rBV2	835	641	0.03%	0.004%
8	2.698	491	500	510	rVB7	3168	4973	0.25%	0.032%
9	2.762	515	520	524	rVB3	677	735	0.04%	0.005%
10	2.862	548	551	555	rVB3	762	562	0.03%	0.004%
11	2.891	555	560	564	rBV3	742	889	0.04%	0.006%
12	2.926	568	571	577	rVB5	575	658	0.03%	0.004%
13	2.981	579	588	598	rBV7	3961	8024	0.40%	0.052%
14	3.080	616	619	627	rVB2	896	990	0.05%	0.006%
15	3.125	629	633	636	rVB3	670	527	0.03%	0.003%
16	3.193	652	654	658	rVB2	1043	556	0.03%	0.004%
17	3.270	672	678	680	rBV	683	672	0.03%	0.004%
18	3.309	685	690	697	rBV2	1102	1280	0.06%	0.008%
19	3.386	712	714	723	rVB4	1088	871	0.04%	0.006%
20	3.624	782	788	790	rBV2	750	720	0.04%	0.005%
21	3.659	794	799	803	rBV3	1049	840	0.04%	0.005%
22	3.823	846	850	853	rBV2	786	530	0.03%	0.003%
23	3.907	873	876	879	rVB2	1018	633	0.03%	0.004%
24	3.965	889	894	896	rVV2	632	509	0.03%	0.003%
25	4.106	930	938	944	rBV4	848	1488	0.07%	0.010%
26	4.174	946	959	962	rBV	194301	351090	17.32%	2.287%
27	4.453	1043	1046	1048	rBV3	926	572	0.03%	0.004%
28	4.511	1061	1064	1065	rBV	859	540	0.03%	0.004%
29	4.643	1087	1105	1127	rBV	320982	789360	38.95%	5.142%
30	4.791	1148	1151	1155	rBV3	652	579	0.03%	0.004%
31	4.874	1173	1177	1180	rBV4	1326	1409	0.07%	0.009%
32	4.984	1207	1211	1214	rBV3	1039	789	0.04%	0.005%
33	5.000	1214	1216	1222	rVB4	732	631	0.03%	0.004%
34	5.067	1234	1237	1239	rVV2	1123	821	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031123.D
 Acq On : 12 Apr 2019 12:27
 Operator : JC/SP
 Sample : K2353-07DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 115 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ63DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

35	5.161	1260	1266	1268	rBV4	937	717	0.04%	0.005%
36	5.334	1294	1320	1348	rBV3	689423	2026546	100.00%	13.200%
37	5.588	1396	1399	1404	rVB4	1407	1105	0.05%	0.007%
38	5.682	1425	1428	1432	rVB3	1479	1035	0.05%	0.007%
39	5.701	1432	1434	1438	rBV2	709	517	0.03%	0.003%
40	5.730	1438	1443	1446	rBV3	835	713	0.04%	0.005%
41	5.788	1459	1461	1465	rVB3	826	503	0.02%	0.003%
42	5.881	1474	1490	1510	rBV	611528	1212679	59.84%	7.899%
43	6.074	1546	1550	1554	rBV4	1615	1637	0.08%	0.011%
44	6.186	1575	1585	1602	rVB4	7340	16194	0.80%	0.105%
45	6.325	1613	1628	1649	rBV	443770	900700	44.45%	5.867%
46	6.505	1680	1684	1686	rVB2	1302	1065	0.05%	0.007%
47	6.527	1688	1691	1694	rVB5	892	514	0.03%	0.003%
48	6.608	1714	1716	1723	rVB4	925	756	0.04%	0.005%
49	6.636	1723	1725	1727	rBV2	799	489	0.02%	0.003%
50	6.968	1823	1828	1830	rBV3	667	504	0.02%	0.003%
51	6.993	1833	1836	1841	rVV2	580	498	0.02%	0.003%
52	7.058	1853	1856	1860	rVV2	490	491	0.02%	0.003%
53	7.157	1883	1887	1889	rBV	682	488	0.02%	0.003%
54	7.225	1895	1908	1934	rBV	242499	441606	21.79%	2.876%
55	7.399	1959	1962	1968	rBV5	691	756	0.04%	0.005%
56	7.562	1997	2013	2050	rBV	858993	1560319	76.99%	10.163%
57	7.845	2090	2101	2125	rBV2	166737	304444	15.02%	1.983%
58	8.228	2211	2220	2230	rBV3	12322	22271	1.10%	0.145%
59	8.308	2234	2245	2288	rBV	543991	1115677	55.05%	7.267%
60	8.627	2339	2344	2346	rBV4	1039	1072	0.05%	0.007%
61	8.662	2353	2355	2360	rVB4	935	683	0.03%	0.004%
62	9.087	2474	2487	2516	rBV	891826	1538248	75.90%	10.020%
63	9.431	2592	2594	2598	rVB	872	595	0.03%	0.004%
64	9.543	2626	2629	2633	rVV3	844	732	0.04%	0.005%
65	9.598	2643	2646	2652	rVV3	678	597	0.03%	0.004%
66	9.627	2653	2655	2659	rVB2	986	657	0.03%	0.004%
67	9.730	2683	2687	2692	rBV3	884	843	0.04%	0.005%
68	9.897	2734	2739	2743	rVB3	856	942	0.05%	0.006%
69	10.022	2775	2778	2781	rVV2	734	639	0.03%	0.004%
70	10.038	2781	2783	2788	rVV4	818	800	0.04%	0.005%
71	10.074	2788	2794	2798	rVV2	862	1185	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU041119\
 Data File : VU031123.D
 Acq On : 12 Apr 2019 12:27
 Operator : JC/SP
 Sample : K2353-07DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 115 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETJ63DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis

72	10.103	2801	2803	2808	rVB2	1027	610	0.03%	0.004%
73	10.164	2819	2822	2824	rBV2	719	495	0.02%	0.003%
74	10.270	2851	2855	2857	rBV2	880	619	0.03%	0.004%
75	10.305	2862	2866	2869	rVB4	949	752	0.04%	0.005%
76	10.427	2886	2904	2928	rBV	580722	961750	47.46%	6.265%
77	10.984	3072	3077	3079	rBV2	830	715	0.04%	0.005%
78	11.115	3115	3118	3123	rBV2	734	723	0.04%	0.005%
79	11.331	3182	3185	3188	rVB3	787	504	0.02%	0.003%
80	11.479	3218	3231	3255	rBV	799323	1318057	65.04%	8.585%
81	11.855	3336	3348	3373	rBV	745853	1267621	62.55%	8.257%
82	12.427	3523	3526	3529	rBV5	862	595	0.03%	0.004%
83	12.501	3547	3549	3553	rVB2	1088	828	0.04%	0.005%
84	12.537	3553	3560	3563	rBV4	1251	1604	0.08%	0.010%
85	12.765	3629	3631	3636	rVB2	762	496	0.02%	0.003%
86	12.842	3652	3655	3658	rVV2	805	518	0.03%	0.003%
87	12.858	3658	3660	3664	rVB2	1053	537	0.03%	0.003%
88	12.926	3677	3681	3684	rBV2	971	909	0.04%	0.006%
89	13.028	3709	3713	3715	rBV3	825	775	0.04%	0.005%
90	13.520	3862	3866	3871	rVB4	886	900	0.04%	0.006%
91	13.549	3872	3875	3878	rBV2	713	589	0.03%	0.004%
92	13.823	3957	3960	3962	rBV2	856	576	0.03%	0.004%
93	13.955	3997	4001	4006	rBV3	1122	1209	0.06%	0.008%
94	14.266	4094	4098	4101	rBV2	830	726	0.04%	0.005%
95	14.340	4118	4121	4126	rBV2	933	769	0.04%	0.005%
96	14.710	4233	4236	4238	rBV2	1105	723	0.04%	0.005%
97	15.012	4327	4330	4333	rBV3	1334	1069	0.05%	0.007%
98	15.051	4340	4342	4345	rBV3	1130	863	0.04%	0.006%
99	15.562	4499	4501	4503	rBV3	1577	863	0.04%	0.006%
100	16.417	4765	4767	4770	rBV3	2344	1294	0.06%	0.008%


Sum of corrected areas: 15352252

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU041119\
Data File : VU031123.D
Acq On : 12 Apr 2019 12:27
Operator : JC/SP
Sample : K2353-07DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 115 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ63DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

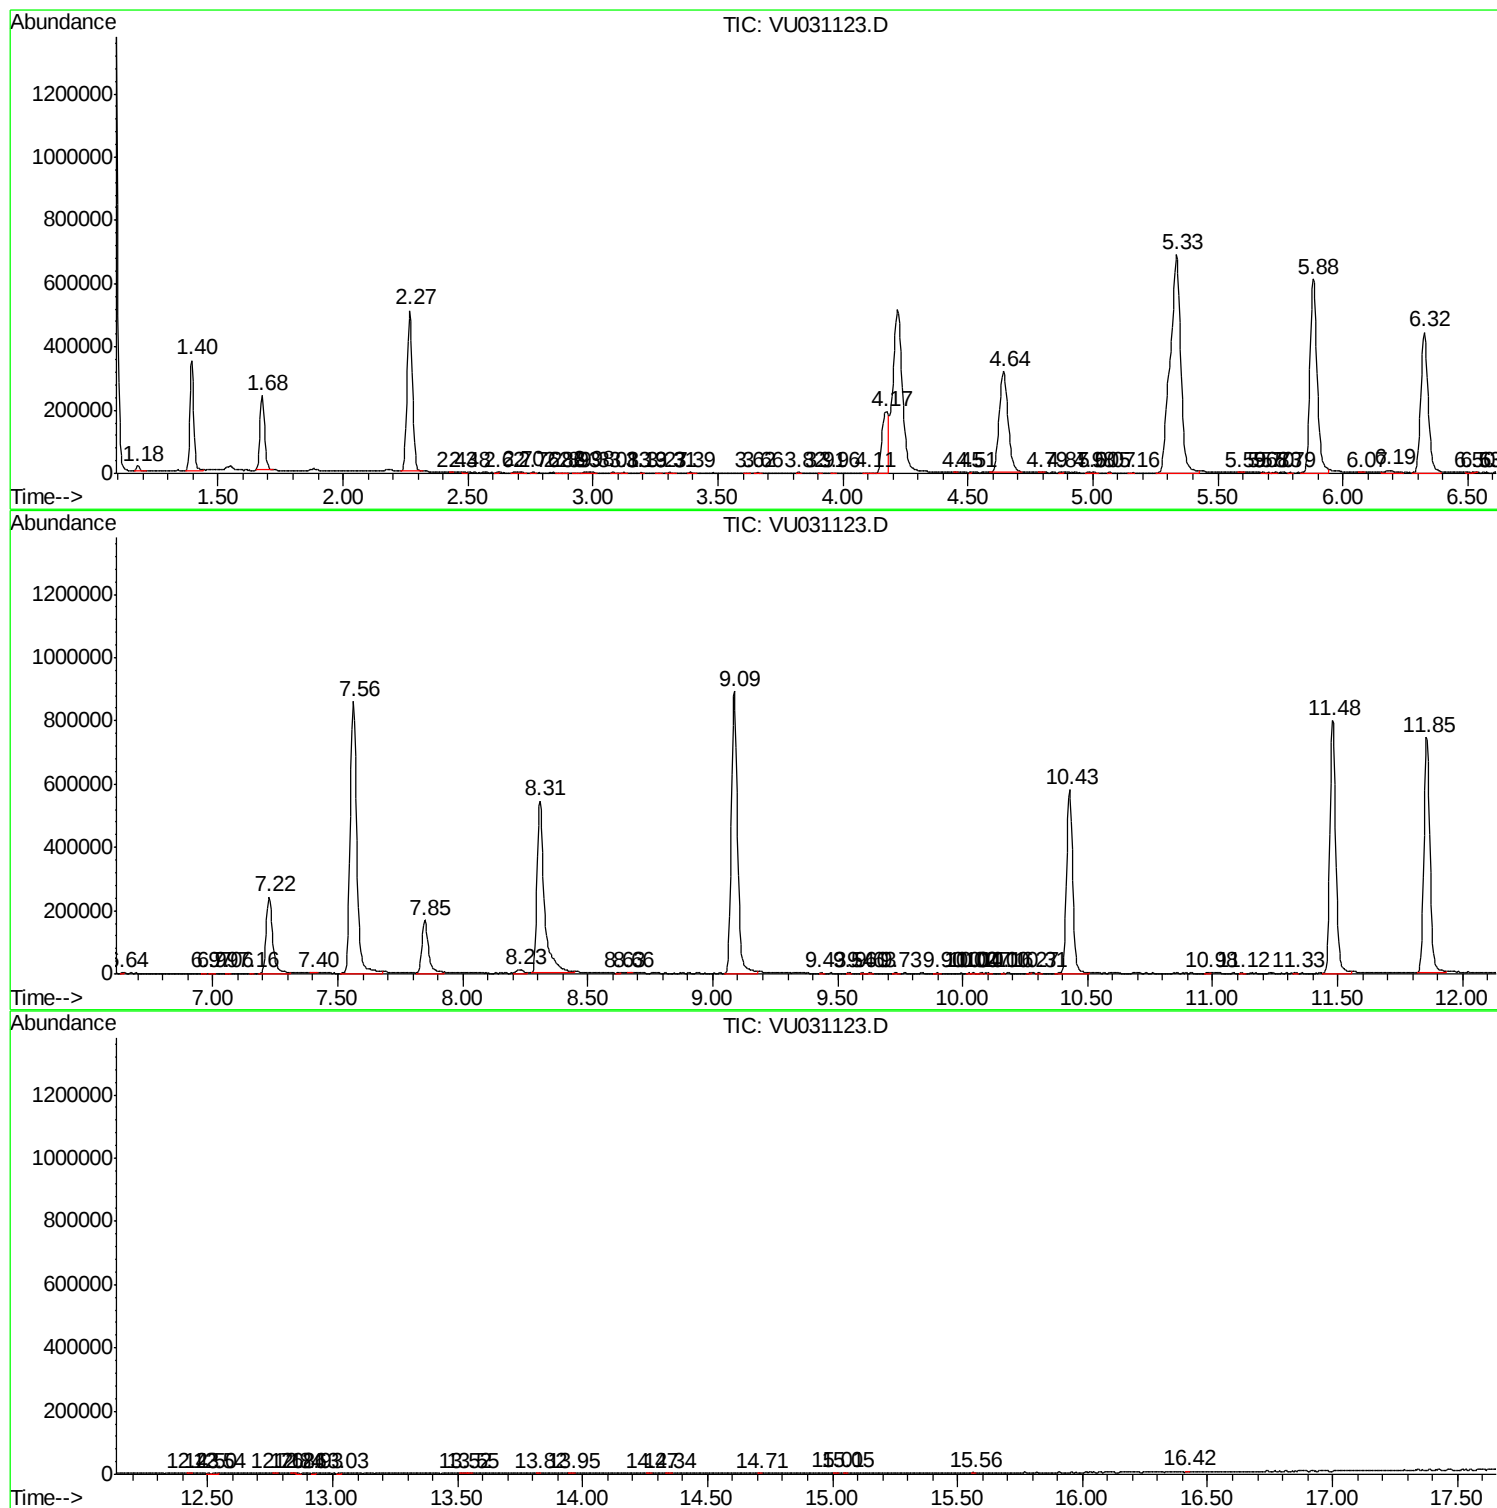

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031123.D
Acq On : 12 Apr 2019 12:27
Operator : JC/SP
Sample : K2353-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 115 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ63DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU041119\
Data File : VU031123.D
Acq On : 12 Apr 2019 12:27
Operator : JC/SP
Sample : K2353-07DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 115 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETJ63DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc