


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU041119\
 Data File : VU031012.D
 Acq On : 10 Apr 2019 15:38
 Operator : JC/SP
 Sample : BFB54
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB54

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM040519WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 15 01:39:53 2019

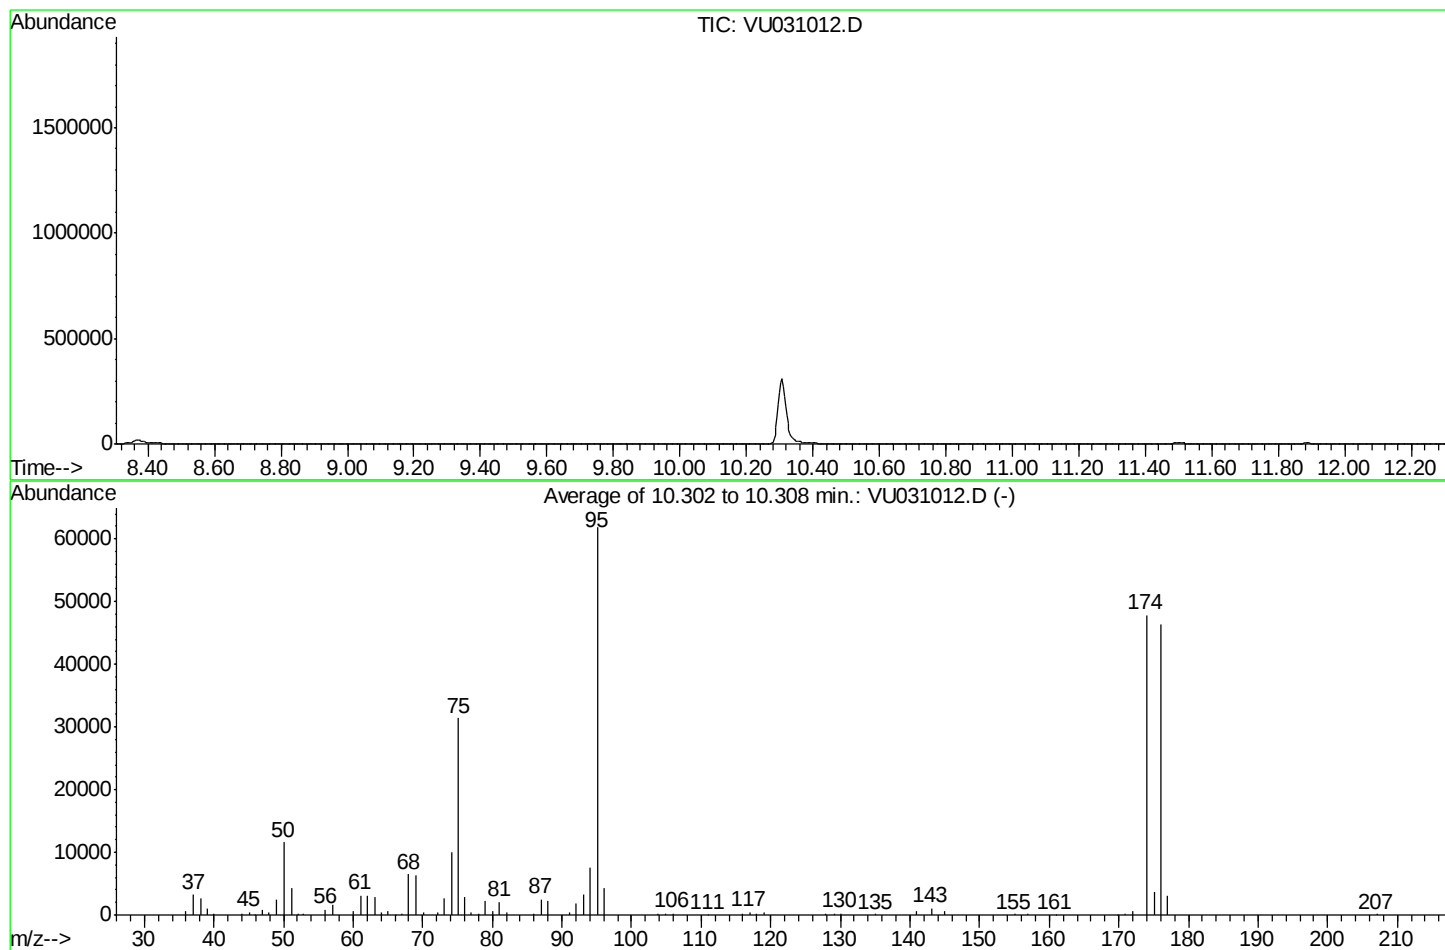

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	11567	PASS
75	95	30	80	50.7	31384	PASS
95	95	100	100	100.0	61848	PASS
96	95	5	9	6.8	4204	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.3	47821	PASS
175	174	5	9	7.8	3709	PASS
176	174	95	101	96.9	46328	PASS
177	176	5	9	6.8	3138	PASS

Scan 2854 (10.266 min): VU031012.D
BFB54

m/z	Abundance
40.00	400.0
44.00	811.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
36.00	655.0
37.00	3290.0
38.10	2687.0
39.10	1098.0
40.00	529.0
44.00	1087.0
45.10	456.0
45.90	105.0
47.00	772.0
48.00	507.0
49.10	2414.0
50.10	11428.0
51.10	4095.0
52.00	128.0
52.20	129.0
52.80	127.0
56.00	669.0
57.00	1591.0
60.00	582.0
61.10	3096.0
62.00	3178.0
63.10	2844.0
64.00	395.0
64.90	648.0
67.00	261.0
68.00	6569.0
69.10	6345.0
70.20	399.0
72.20	449.0
73.10	2277.0
74.10	10315.0
75.10	30816.0
76.10	2790.0
77.10	240.0
77.90	272.0
78.90	2293.0
80.00	736.0
81.00	2196.0
82.00	516.0
86.00	368.0
87.00	2470.0
88.00	2268.0
91.00	181.0
92.00	1845.0
93.10	3250.0
94.00	7867.0
95.10	62704.0
96.10	4209.0
103.80	329.0
104.90	160.0
105.90	248.0
111.00	132.0
115.90	259.0
117.00	497.0
117.90	220.0
119.00	403.0
127.90	241.0
129.10	225.0
130.00	289.0
135.00	116.0
140.90	670.0
143.00	1205.0
145.00	535.0
155.10	199.0
157.00	110.0
160.90	133.0
170.90	119.0
172.00	685.0
174.00	49288.0
175.10	3957.0
176.00	46856.0
177.00	3143.0
207.00	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
36.00	479.0
37.10	3027.0
38.10	2682.0
39.00	1076.0
39.90	514.0
44.00	902.0
45.10	554.0
45.90	100.0
47.00	683.0
47.90	460.0
49.00	2283.0
50.00	11486.0
51.10	4337.0
52.20	161.0
52.80	154.0
56.00	940.0
57.00	1610.0
60.00	637.0
61.10	2976.0
62.00	2957.0
63.00	2656.0
64.00	416.0
65.10	627.0
67.10	224.0
68.00	6149.0
69.10	6177.0
70.20	594.0
72.10	218.0
73.00	3051.0
74.10	9738.0
75.10	30904.0
76.00	2734.0
77.00	394.0
78.00	130.0
79.00	2308.0
80.00	461.0
81.00	1989.0
82.10	470.0
86.00	156.0
87.00	2568.0
88.00	2084.0
91.00	418.0
92.00	1677.0
93.10	3314.0
94.00	6978.0
95.10	58984.0
96.10	4010.0
104.00	124.0
105.00	175.0
106.00	351.0
116.00	313.0
117.00	428.0
118.00	362.0
119.00	541.0
127.90	265.0
130.00	244.0
135.10	189.0
140.90	625.0
143.10	1020.0
145.00	571.0
155.00	109.0
157.00	121.0
169.70	109.0
171.00	159.0
172.10	567.0
174.00	44944.0
175.10	3413.0
176.10	44200.0
177.00	3020.0
207.10	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54

m/z	Abundance
36.00	614.0
37.00	3244.0
38.10	2909.0
39.10	1048.0
39.90	564.0
44.00	1017.0
45.00	491.0
47.00	782.0
48.00	507.0
49.00	2540.0
50.10	11787.0
51.10	4503.0
52.20	171.0
52.80	168.0
56.00	861.0
57.00	1577.0
60.00	668.0
61.10	3147.0
62.00	3036.0
63.10	2794.0
64.00	403.0
65.00	655.0
66.10	104.0
67.10	238.0
68.00	6807.0
69.10	6339.0
70.20	526.0
72.20	360.0
73.00	2634.0
74.10	10217.0
75.10	32432.0
76.10	2839.0
77.00	343.0
77.90	178.0
79.00	2366.0
80.00	601.0
81.00	2174.0
82.10	541.0
86.00	290.0
87.00	2585.0
88.00	2163.0
91.00	355.0
92.00	1950.0
93.10	3555.0
94.00	7961.0
95.10	63856.0
96.10	4395.0
103.80	191.0
105.00	197.0
106.00	317.0
111.00	100.0
116.00	301.0
117.00	548.0
118.00	287.0
119.00	530.0
127.90	281.0
129.10	139.0
130.00	295.0
135.00	143.0
140.90	668.0
143.00	1161.0
145.00	615.0
155.10	147.0
157.00	143.0
160.90	138.0
171.00	138.0
172.00	705.0
174.00	49232.0
175.10	3757.0
176.00	47928.0
177.00	3253.0
207.10	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB54