




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047922.D
 Acq On : 11 Apr 2022 21:51
 Operator : SY/MD
 Sample : N2293-04ME
 Misc : 6.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNN4ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

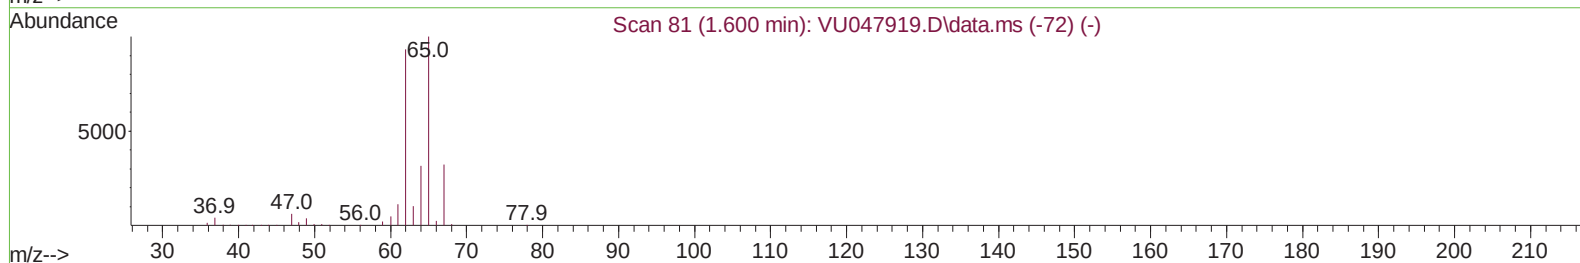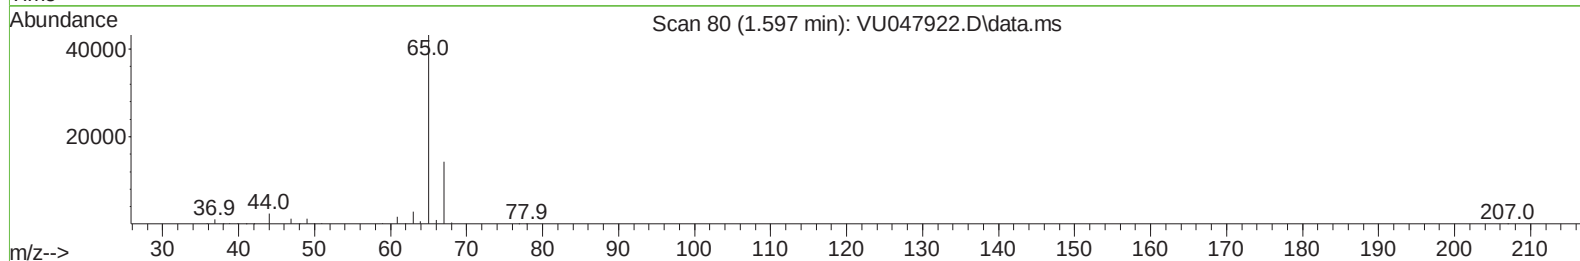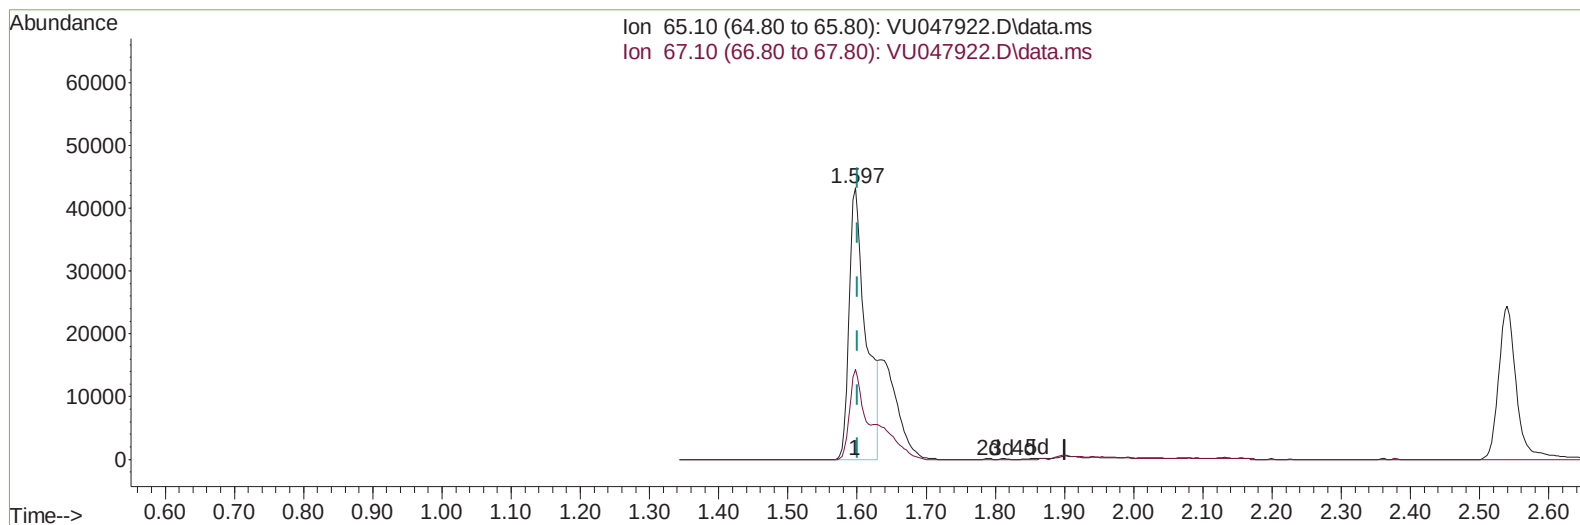

TIC: VU047922.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.597min (-0.003) 22.44 ug/L

response 72238

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.70	28.15
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047922.D
 Acq On : 11 Apr 2022 21:51
 Operator : SY/MD
 Sample : N2293-04ME
 Misc : 6.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNN4ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

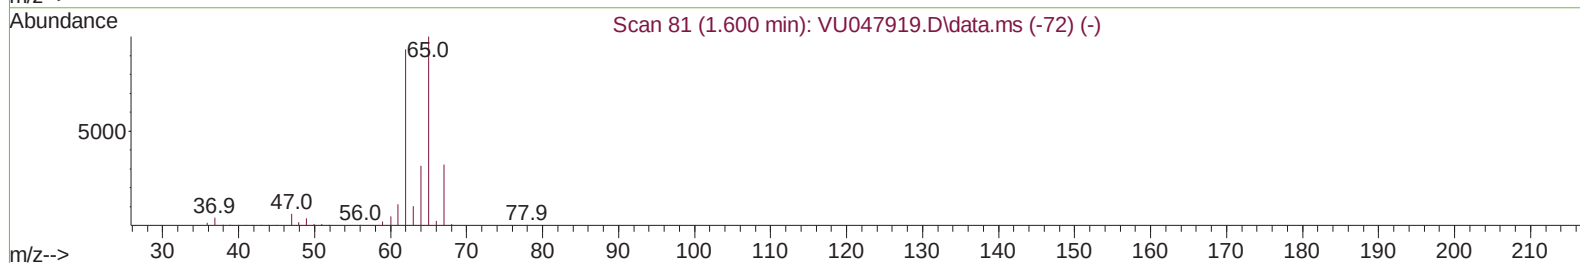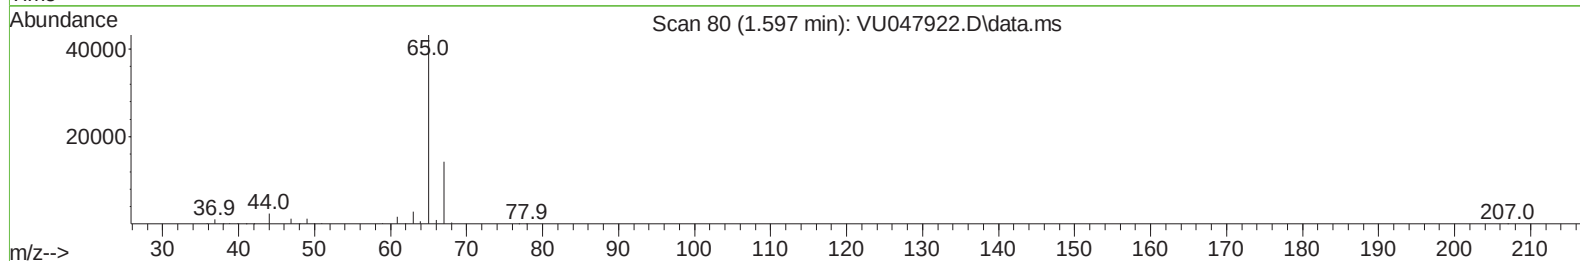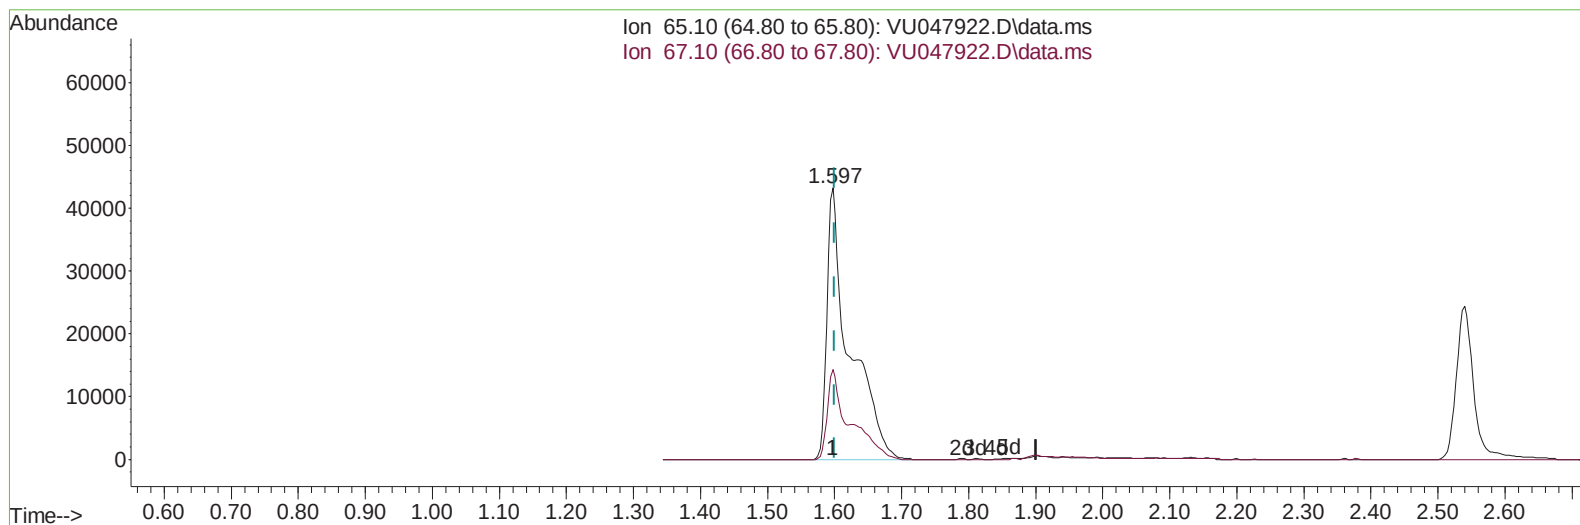

TIC: VU047922.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.597min (-0.003) 31.51 ug/L m

response 101415

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.70	20.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047922.D
 Acq On : 11 Apr 2022 21:51
 Operator : SY/MD
 Sample : N2293-04ME
 Misc : 6.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNN4ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

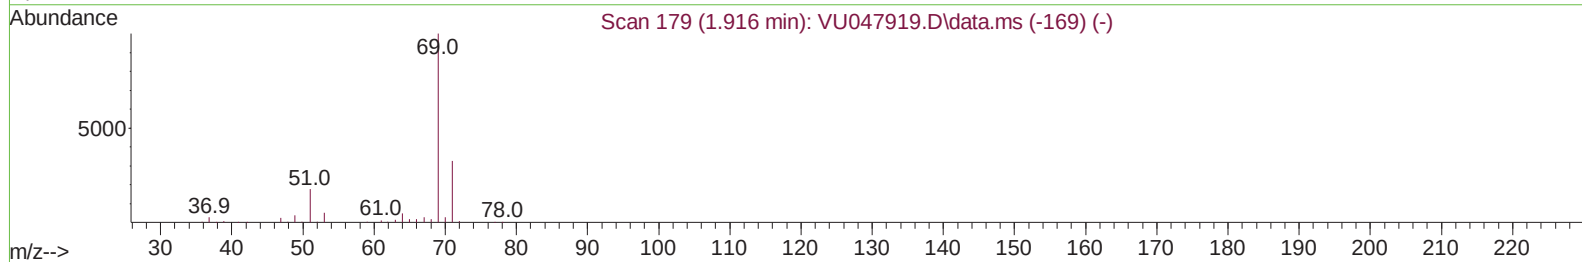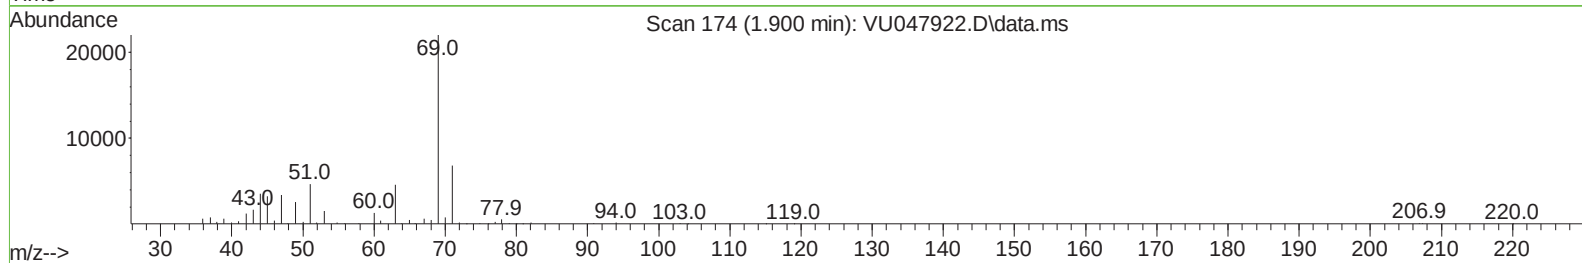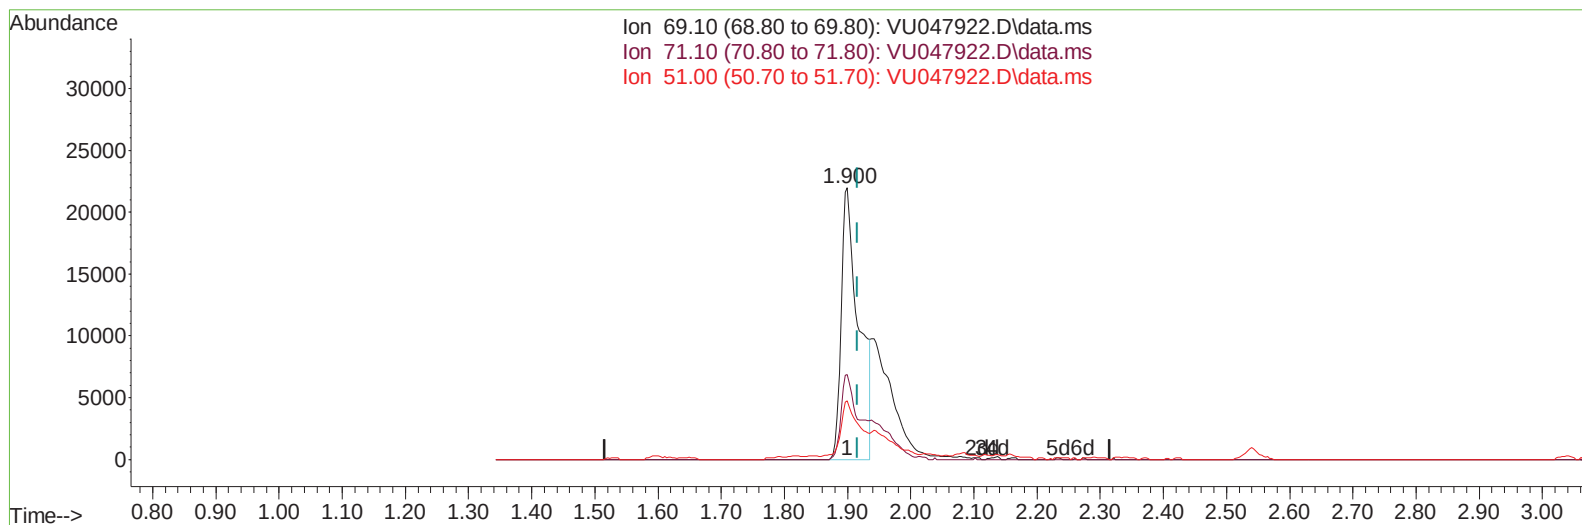

TIC: VU047922.D\data.ms

(7) Chloroethane-d5 (S)

1.900min (-0.016) 16.66 ug/L

response 42280

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	24.52
51.00	24.50	21.38
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047922.D
 Acq On : 11 Apr 2022 21:51
 Operator : SY/MD
 Sample : N2293-04ME
 Misc : 6.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNN4ME

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

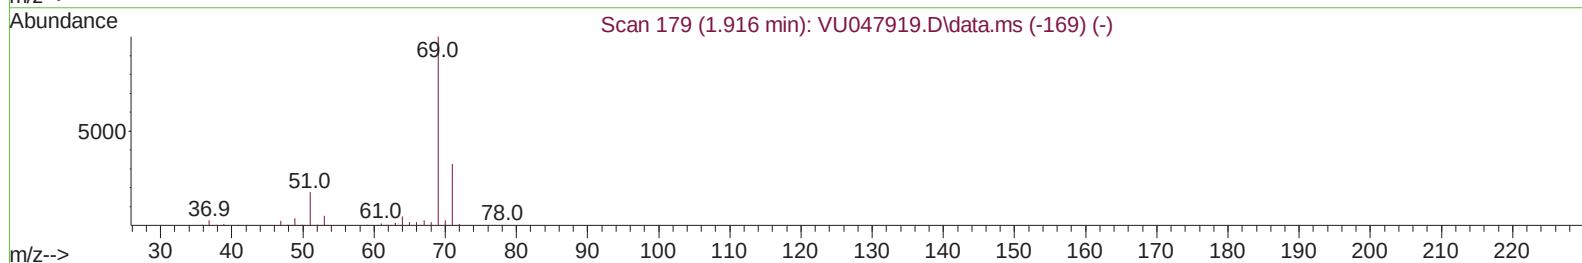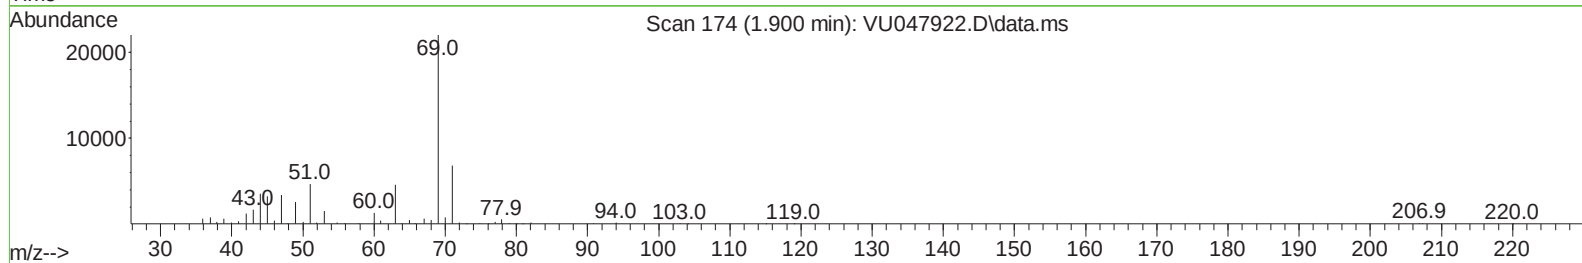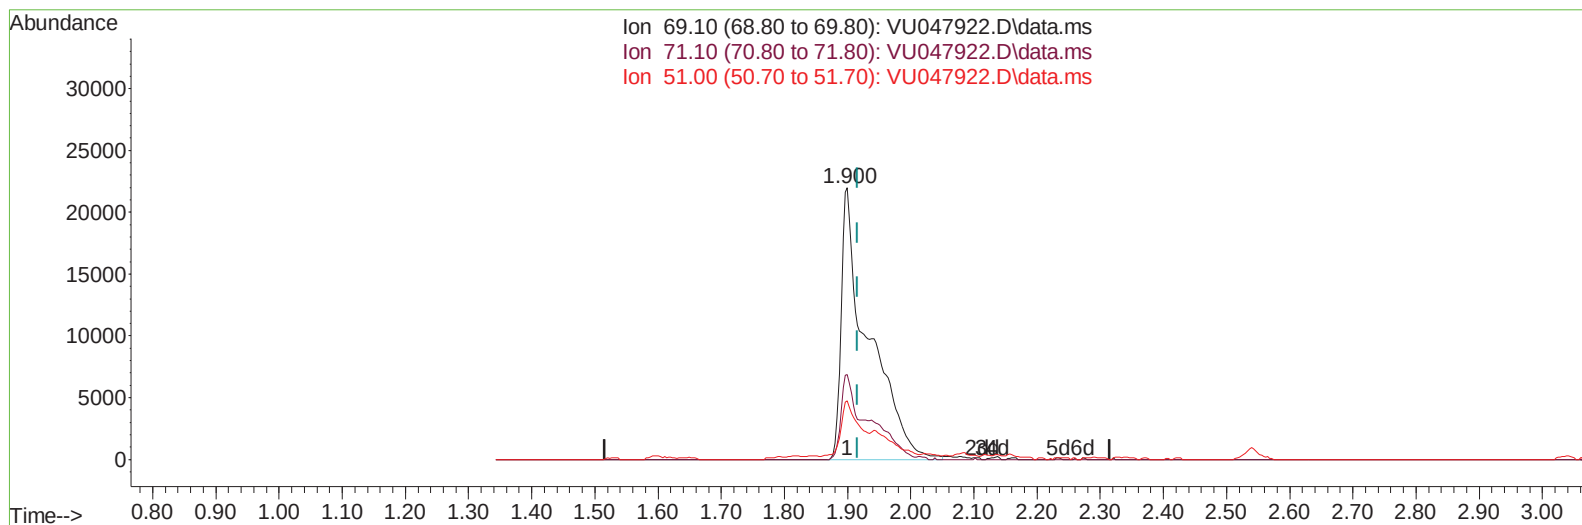

TIC: VU047922.D\data.ms

(7) Chloroethane-d5 (S)

1.900min (-0.016) 25.66 ug/L m

response 65123

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	32.10	15.92#
51.00	24.50	13.88#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047922.D
 Acq On : 11 Apr 2022 21:51
 Operator : SY/MD
 Sample : N2293-04ME
 Misc : 6.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNN4ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	443881	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	468220	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	253002	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	101415m	31.506	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	63.020%	
7) Chloroethane-d5	1.900	69	65123m	25.658	ug/L	-0.02
Spiked Amount 50.000	Range 70	- 130	Recovery	=	51.320%#	
11) 1,1-Dichloroethene-d2	2.539	63	139822	23.742	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125	Recovery	=	47.480%#	
21) 2-Butanone-d5	4.649	46	205187	74.267	ug/L	0.03
Spiked Amount 100.000	Range 40	- 130	Recovery	=	74.270%	
24) Chloroform-d	5.064	84	211952	35.987	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	71.980%	
26) 1,2-Dichloroethane-d4	5.703	65	142656	39.492	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	78.980%	
32) Benzene-d6	5.723	84	431891	36.658	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	73.320%	
36) 1,2-Dichloropropane-d6	6.690	67	140650	38.872	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	77.740%	
41) Toluene-d8	7.899	98	382112	33.288	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	66.580%#	
43) trans-1,3-Dichloroprop...	8.182	79	58502	31.914	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	63.820%	
47) 2-Hexanone-d5	8.668	63	154334	72.863	ug/L	0.04
Spiked Amount 100.000	Range 45	- 130	Recovery	=	72.860%	
56) 1,1,2,2-Tetrachloroeth...	10.767	84	224265	36.116	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	72.240%	
66) 1,2-Dichlorobenzene-d4	12.198	152	173064	38.449	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	76.900%#	
Target Compounds					Qvalue	
33) Benzene	5.771	78	73477	5.422	ug/L	100
42) Toluene	7.970	91	24156	1.624	ug/L	99
51) Chlorobenzene	9.452	112	454429	45.006	ug/L	98
67) 1,2-Dichlorobenzene	12.218	146	15036	1.977	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047922.D
Acq On : 11 Apr 2022 21:51
Operator : SY/MD
Sample : N2293-04ME
Misc : 6.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNN4ME

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:05:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 12 04:48:51 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/14/2022
Supervised By :Mahesh Dadoda 04/14/2022

