




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047926.D
 Acq On : 11 Apr 2022 23:23
 Operator : SY/MD
 Sample : N2293-13ME
 Misc : 6.56g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP1ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:06:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

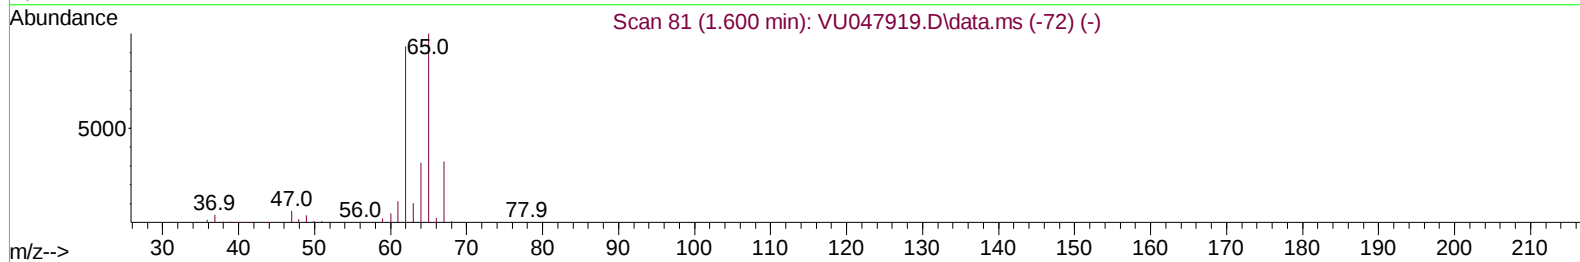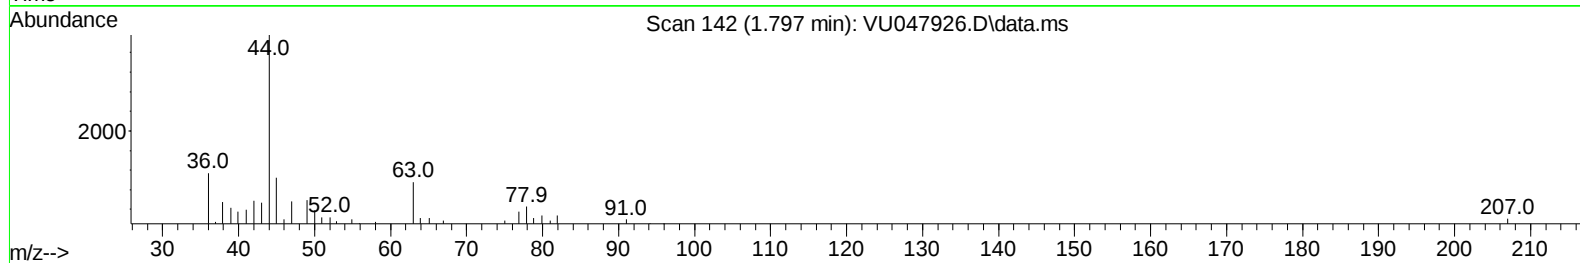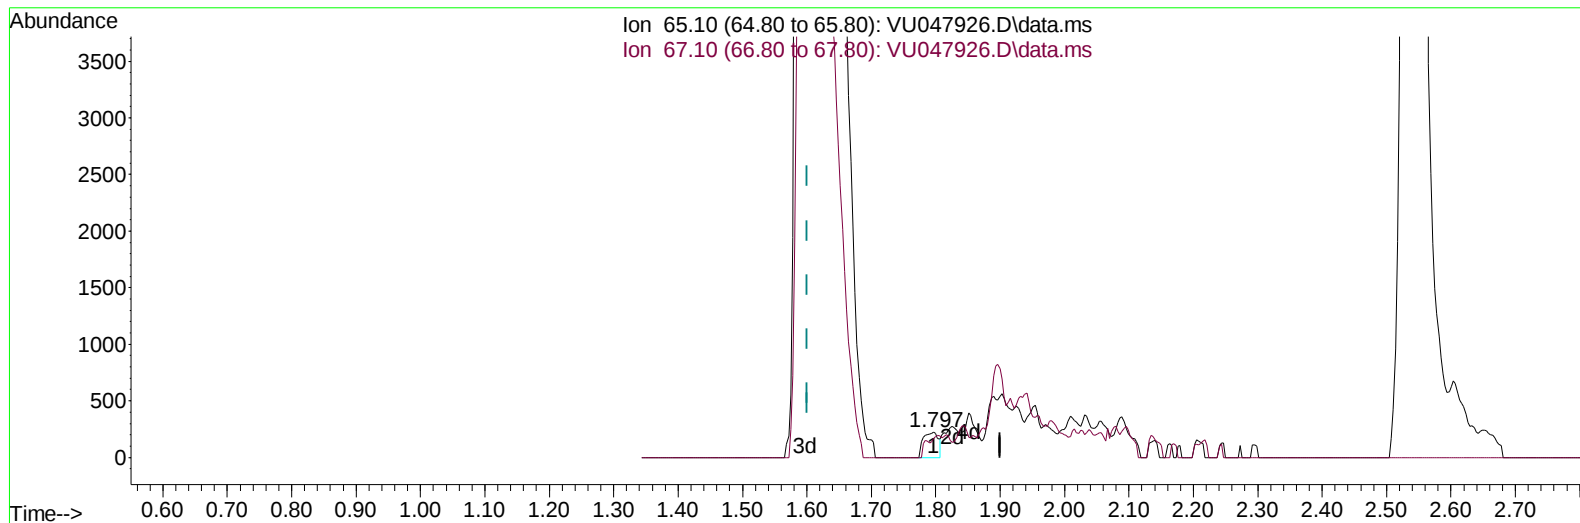

TIC: VU047926.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.797min (+ 0.196) 0.11 ug/L

response 367

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.70	37.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047926.D
Acq On : 11 Apr 2022 23:23
Operator : SY/MD
Sample : N2293-13ME
Misc : 6.56g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNP1ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:06:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 12 04:48:51 2022
Response via : Initial Calibration

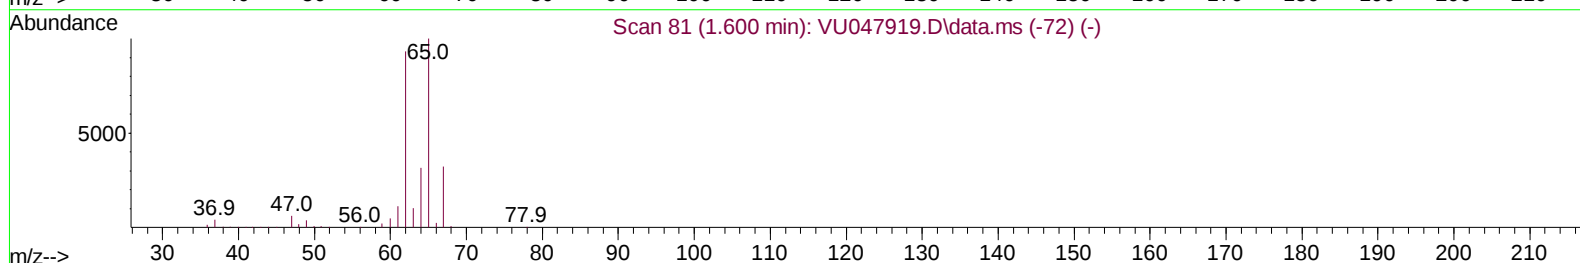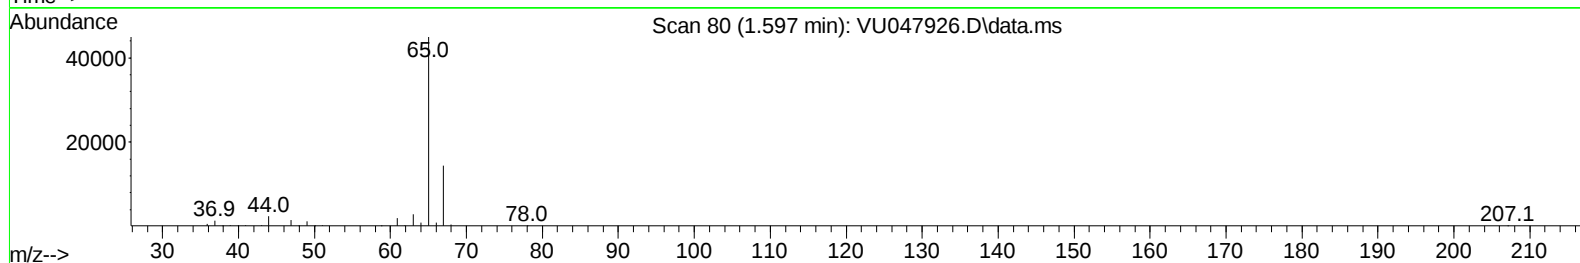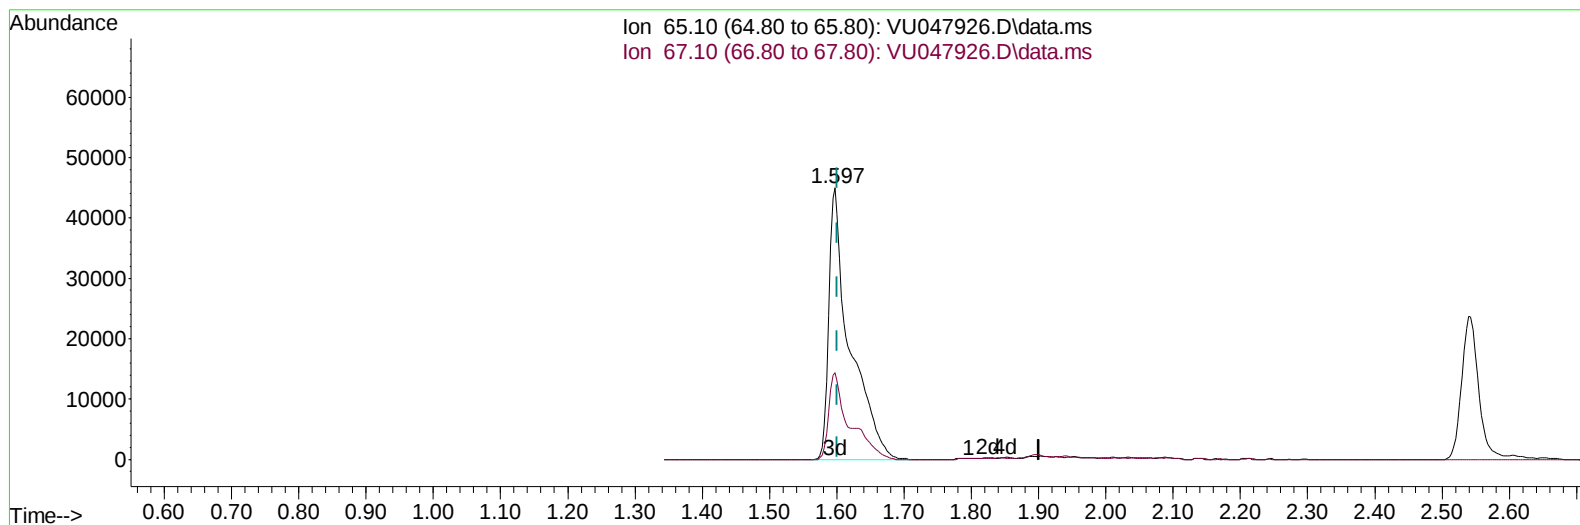

TIC: VU047926.D\data.ms

(4) Vinyl Chloride-d3 (S)

1.597min (-0.003) 29.62 ug/L m

response 97586

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	31.70	0.14#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
 Data File : VU047926.D
 Acq On : 11 Apr 2022 23:23
 Operator : SY/MD
 Sample : N2293-13ME
 Misc : 6.56g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNP1ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/14/2022
 Supervised By :Mahesh Dadoda 04/14/2022

Quant Time: Apr 12 05:06:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 12 04:48:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	454328	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	478154	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	260810	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	97586m	29.620	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	59.240%#		
7) Chloroethane-d5	1.893	69	59294	22.825	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	45.640%#		
11) 1,1-Dichloroethene-d2	2.539	63	136169	22.590	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	45.180%#		
21) 2-Butanone-d5	4.642	46	206004	72.848	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	72.850%		
24) Chloroform-d	5.063	84	207058	34.348	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	68.700%#		
26) 1,2-Dichloroethane-d4	5.700	65	139151	37.636	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.280%		
32) Benzene-d6	5.723	84	424776	35.305	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	70.600%		
36) 1,2-Dichloropropane-d6	6.690	67	139506	37.755	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	75.500%		
41) Toluene-d8	7.899	98	371324	31.676	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	63.360%#		
43) trans-1,3-Dichloroprop...	8.182	79	57512	30.723	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.440%		
47) 2-Hexanone-d5	8.661	63	153254	70.850	ug/L	0.03
Spiked Amount 100.000	Range 45 - 130		Recovery =	70.850%		
56) 1,1,2,2-Tetrachloroeth...	10.767	84	224308	35.372	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	70.740%		
66) 1,2-Dichlorobenzene-d4	12.198	152	170876	36.826	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.660%#		
Target Compounds					Qvalue	
33) Benzene	5.771	78	79971	5.778	ug/L	100
51) Chlorobenzene	9.452	112	391402	37.959	ug/L	99
67) 1,2-Dichlorobenzene	12.217	146	13498	1.722	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041122\
Data File : VU047926.D
Acq On : 11 Apr 2022 23:23
Operator : SY/MD
Sample : N2293-13ME
Misc : 6.56g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNP1ME

Manual IntegrationsAPPROVED

Quant Time: Apr 12 05:06:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 12 04:48:51 2022
Response via : Initial Calibration

Reviewed By :John Carlone 04/14/2022
Supervised By :Mahesh Dadoda 04/14/2022

